

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081622\
 Data File : VW024249.D
 Acq On : 16 Aug 2022 12:37
 Operator : SY/VA
 Sample : VW0816SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK577

Quant Time: Aug 17 01:01:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 17 01:00:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	254420	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	260764	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	142238	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	105510	19.840	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.360%
7) Chloroethane-d5	2.873	69	75255	22.716	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.880%
11) 1,1-Dichloroethene-d2	4.001	63	87983	14.517	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	58.080%
21) 2-Butanone-d5	7.007	46	41	0.041	ug/L	-0.07
Spiked Amount	50.000	Range	20 - 135	Recovery	=	0.080%#
24) Chloroform-d	7.647	84	165498	21.498	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	86.000%
26) 1,2-Dichloroethane-d4	8.299	65	97246	22.753	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	91.000%
32) Benzene-d6	8.269	84	305320	19.853	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	79.400%
36) 1,2-Dichloropropane-d6	9.275	67	99374	21.885	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	87.560%
41) Toluene-d8	10.323	98	271388	18.880	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	75.520%
43) trans-1,3-Dichloroprop...	10.573	79	40837	20.533	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	82.120%
47) 2-Hexanone-d5	10.921	63	42218	50.338	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	100.680%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	112887	25.625	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	102.480%
66) 1,2-Dichlorobenzene-d4	13.847	152	125126	24.039	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	96.160%
Target Compounds						Qvalue
16) Methylene chloride	4.903	84	20144	4.490	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081622\
Data File : VW024249.D
Acq On : 16 Aug 2022 12:37
Operator : SY/VA
Sample : VW0816SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK577


Quant Time: Aug 17 01:01:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Aug 17 01:00:38 2022
Response via : Initial Calibration

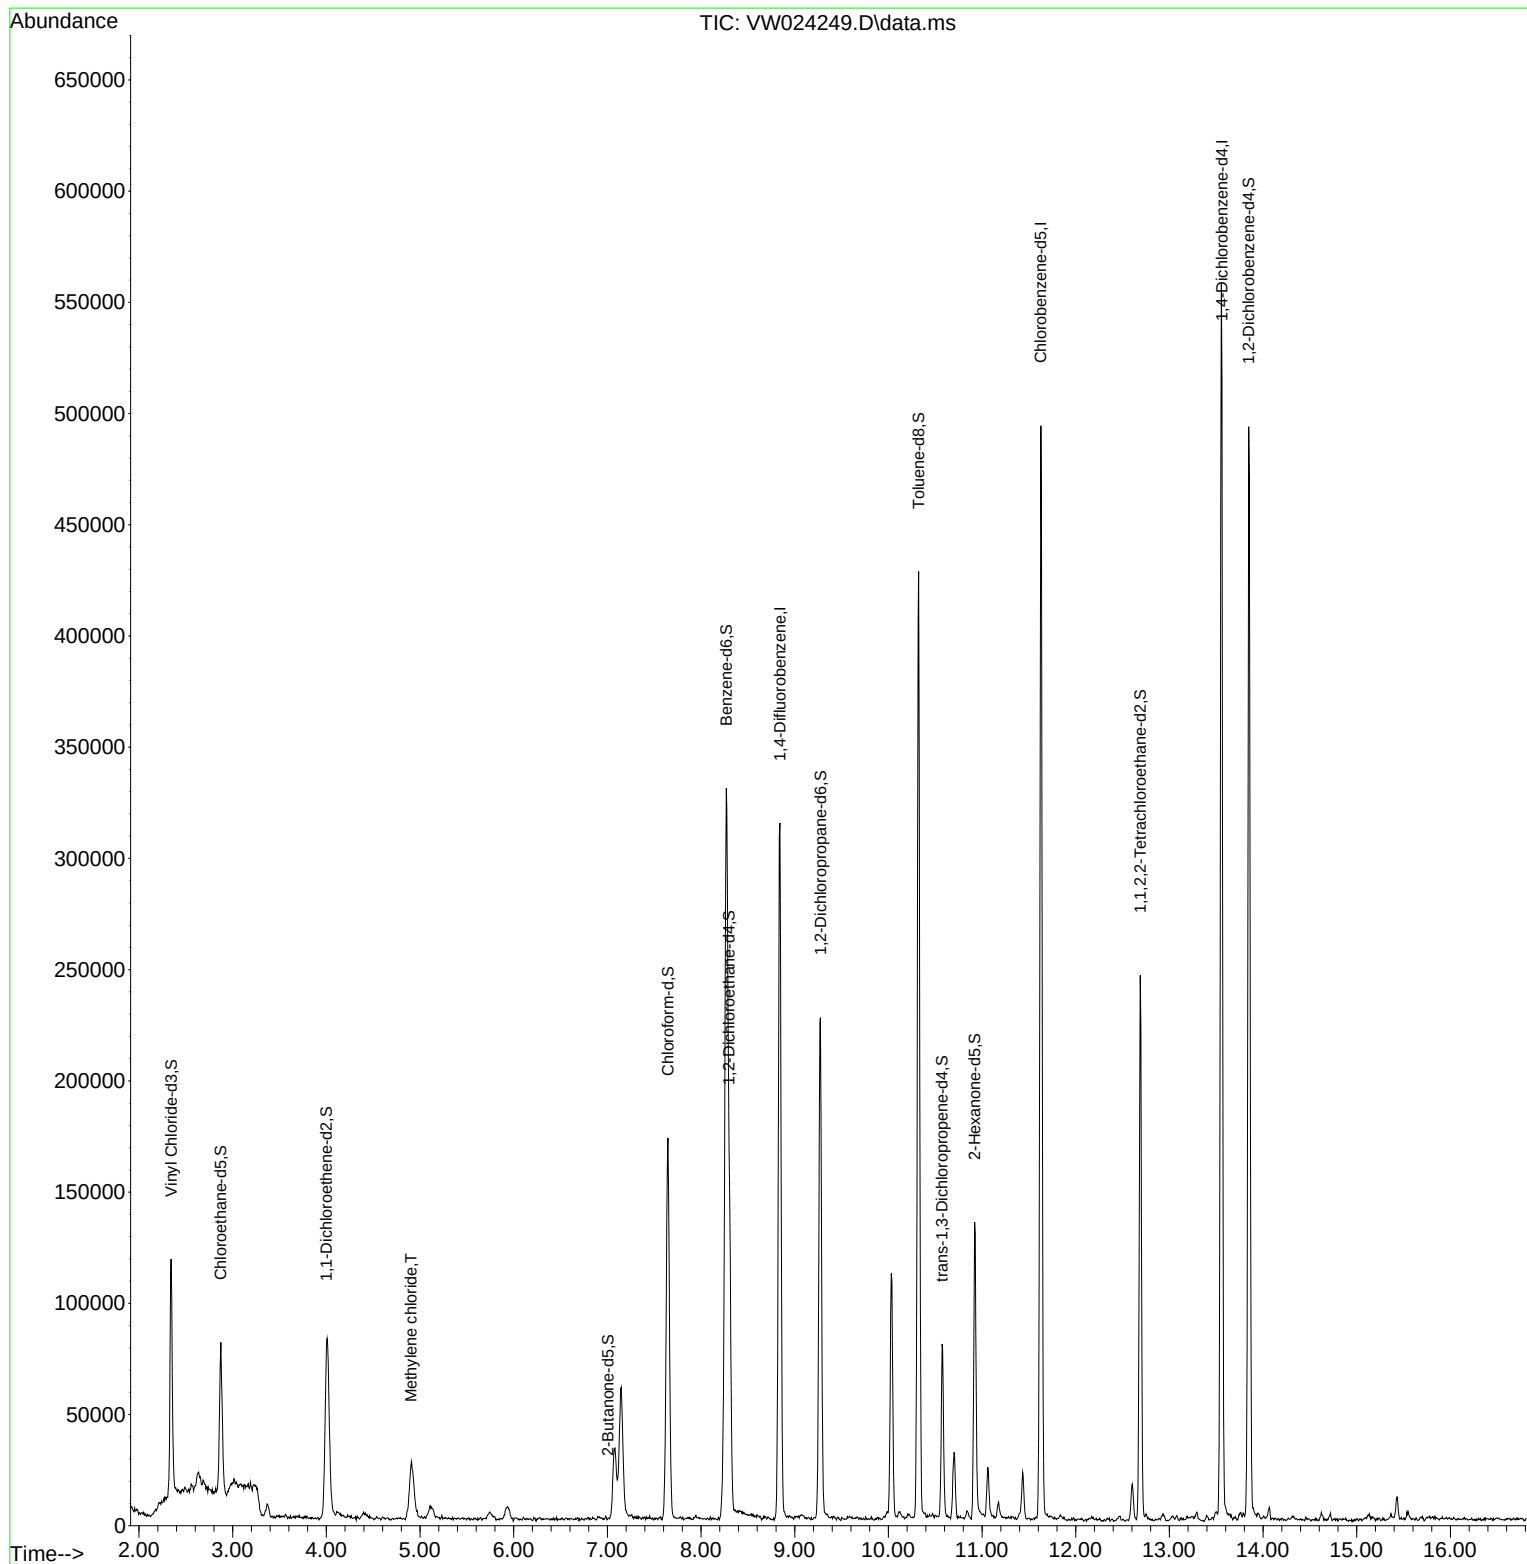

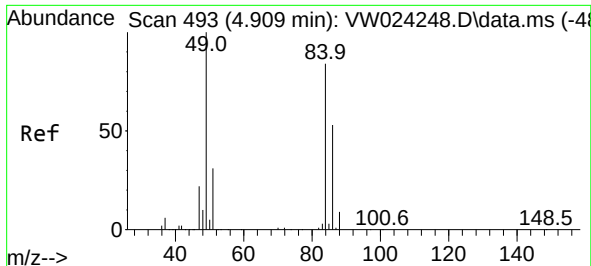

#16
Methylene chloride
Concen: 4.490 ug/L
RT: 4.903 min Scan# 49
Delta R.T. -0.006 min
Lab File: VW024249.D
Acq: 16 Aug 2022 12:37

Instrument :
MSVOA_W
ClientSampleId :
VBLK577

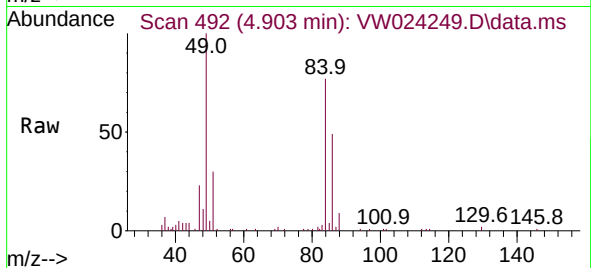

Tgt Ion:	84	Resp:	20144
Ion	Ratio	Lower	Upper
84	100		
86	63.1	42.8	79.6
49	129.9	85.3	158.3

