




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081622\
Data File : VW024249.D
Acq On : 16 Aug 2022 12:37
Operator : SY/VA
Sample : VW0816SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK577

Manual IntegrationsAPPROVED

Quant Time: Aug 17 01:16:12 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Aug 17 01:00:38 2022
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/17/2022
Supervised By :Semsettin Yesilyurt 08/17/2022

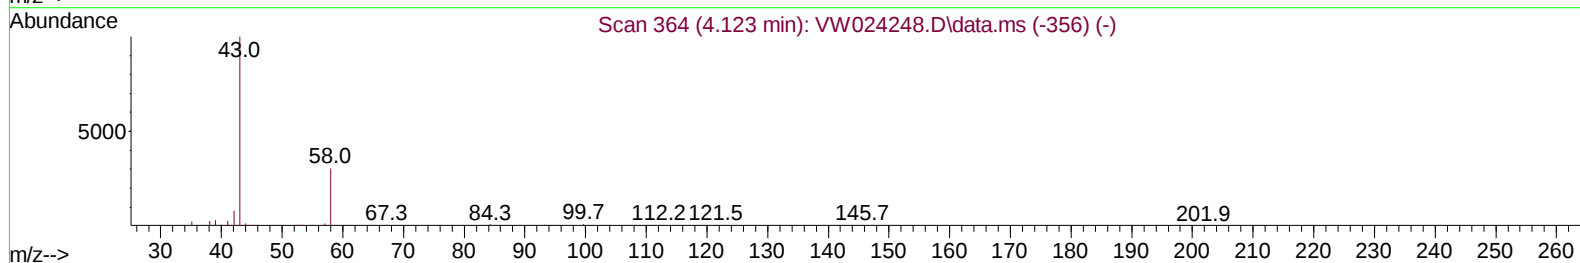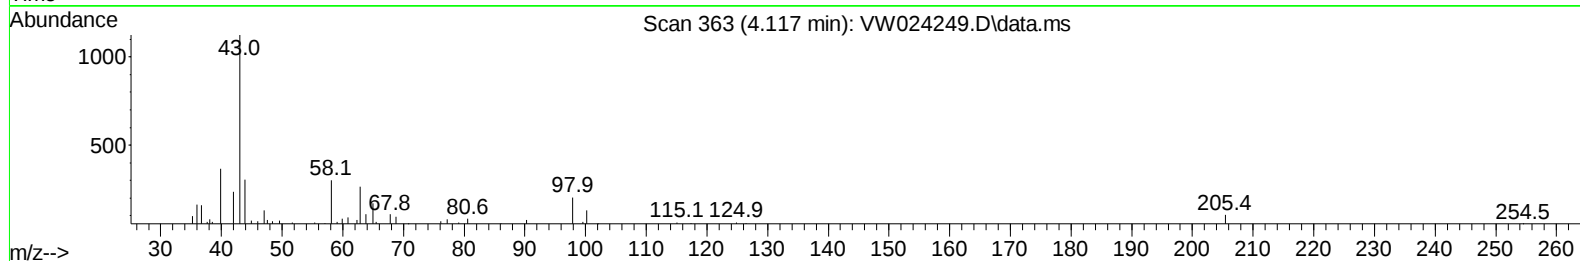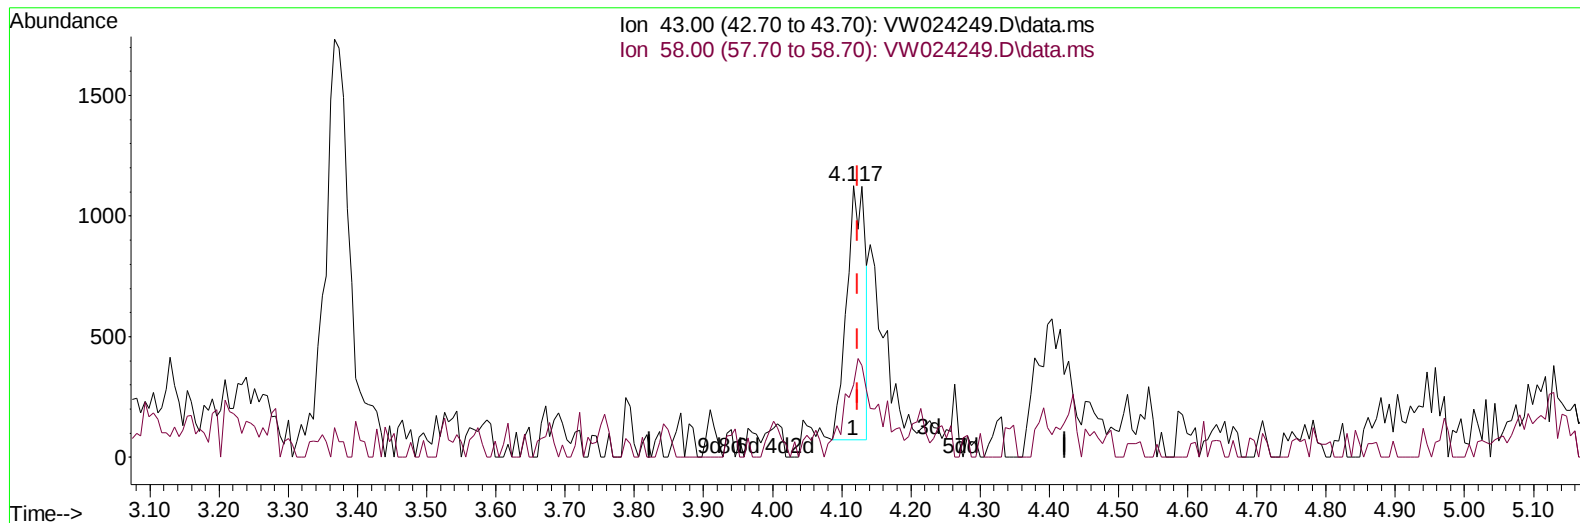

TIC: VW024249.D\data.ms

(13) Acetone (T)

4.117min (-0.006) 2.65 ug/L

response 1930

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	15.90	33.68#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081622\
Data File : VW024249.D
Acq On : 16 Aug 2022 12:37
Operator : SY/VA
Sample : VW0816SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK577

Manual IntegrationsAPPROVED

Quant Time: Aug 17 01:01:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Aug 17 01:00:38 2022
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/17/2022
Supervised By :Semsettin Yesilyurt 08/17/2022

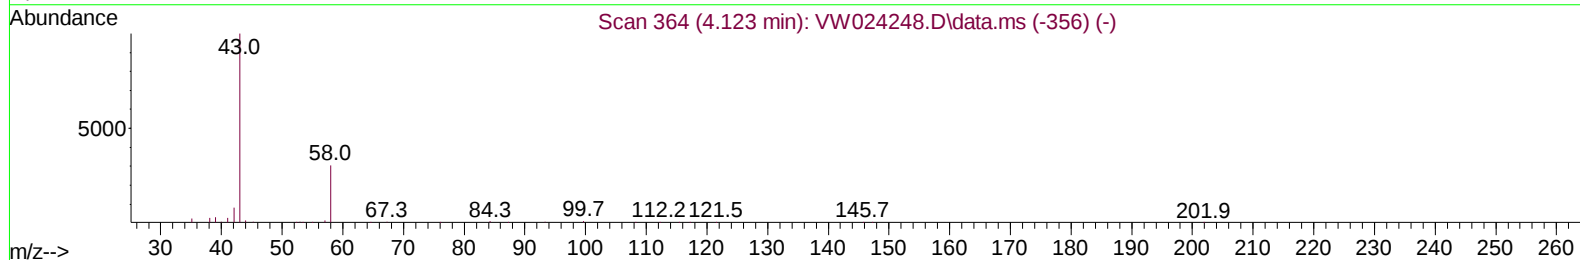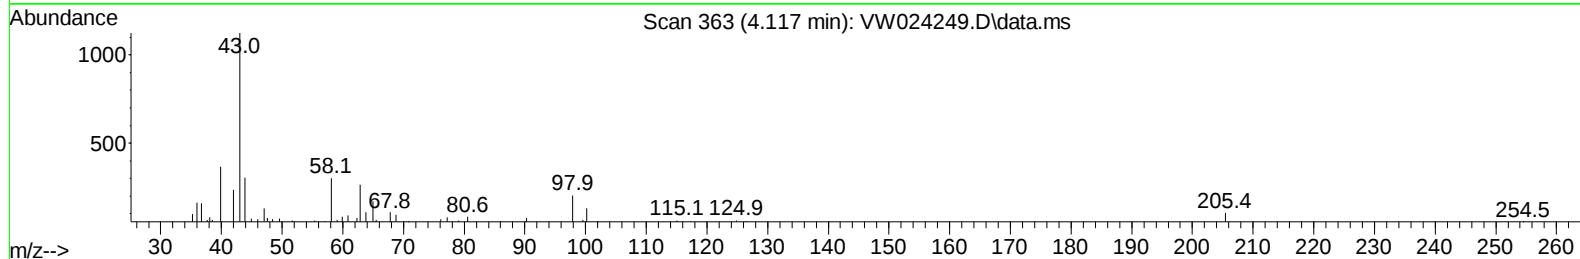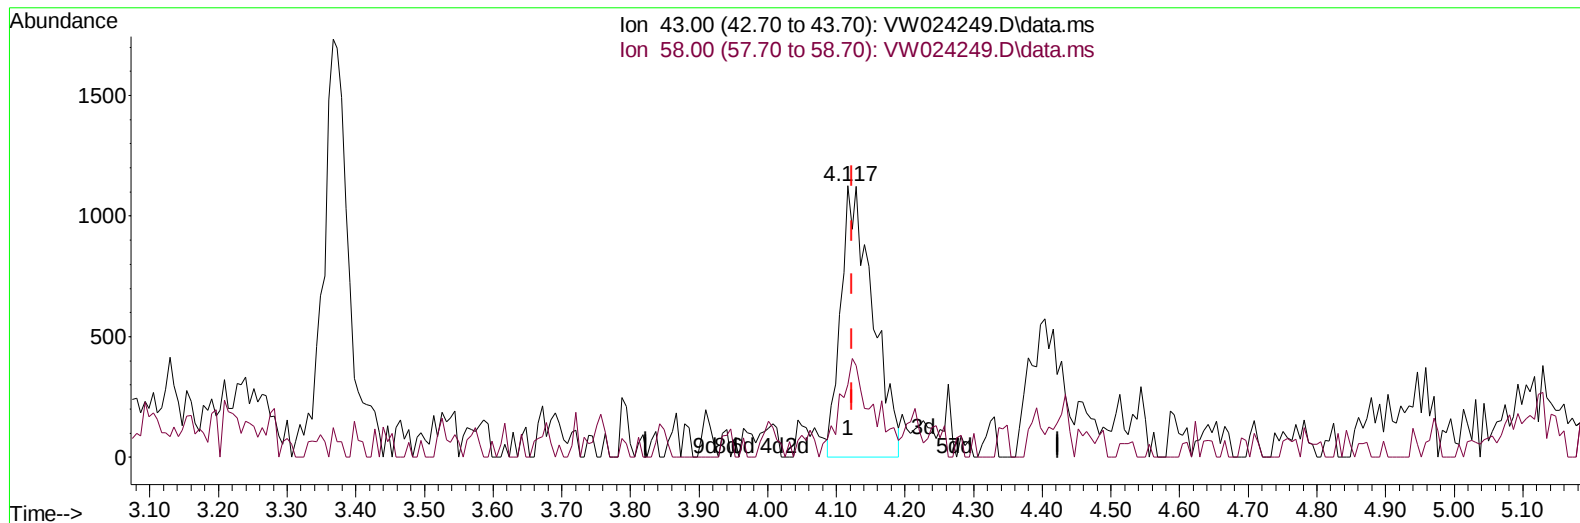

TIC: VW024249.D\data.ms

(13) Acetone (T)

4.117min (-0.006) 4.99 ug/L m

response 3637

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	15.90	0.00
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081622\
 Data File : VW024249.D
 Acq On : 16 Aug 2022 12:37
 Operator : SY/VA
 Sample : VW0816SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK577

Manual IntegrationsAPPROVED

Quant Time: Aug 17 01:01:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 17 01:00:38 2022
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/17/2022
 Supervised By :Semsettin Yesilyurt 08/17/2022

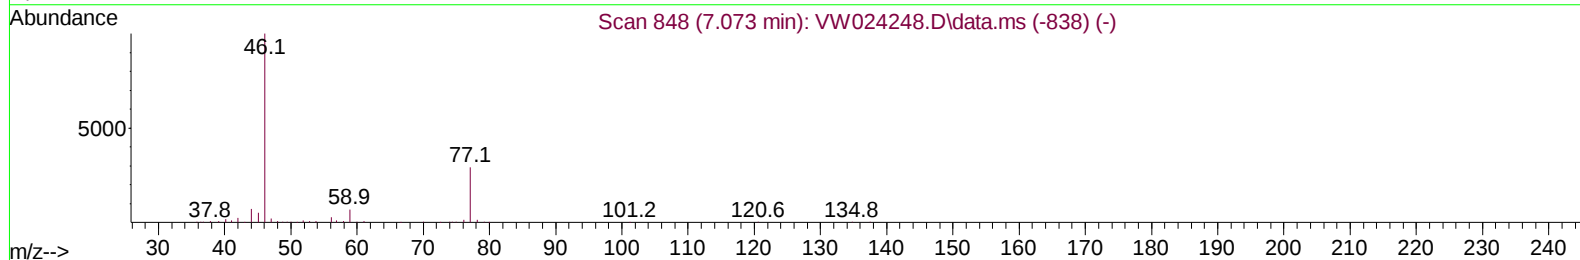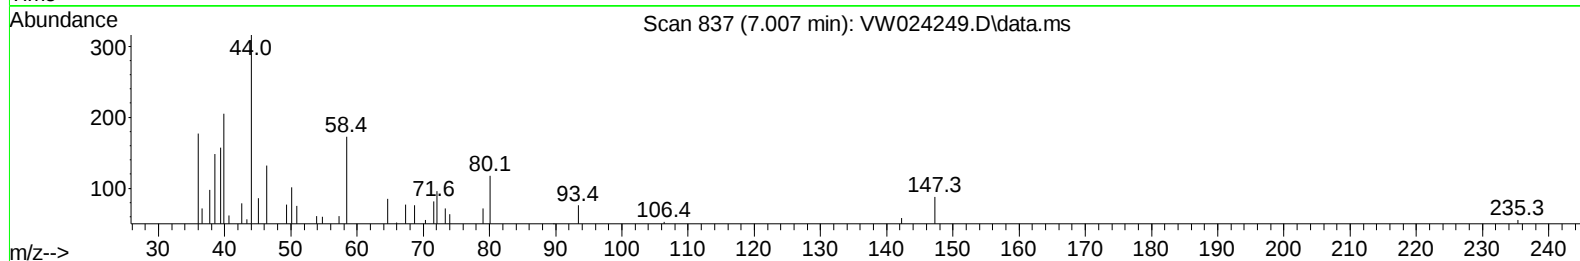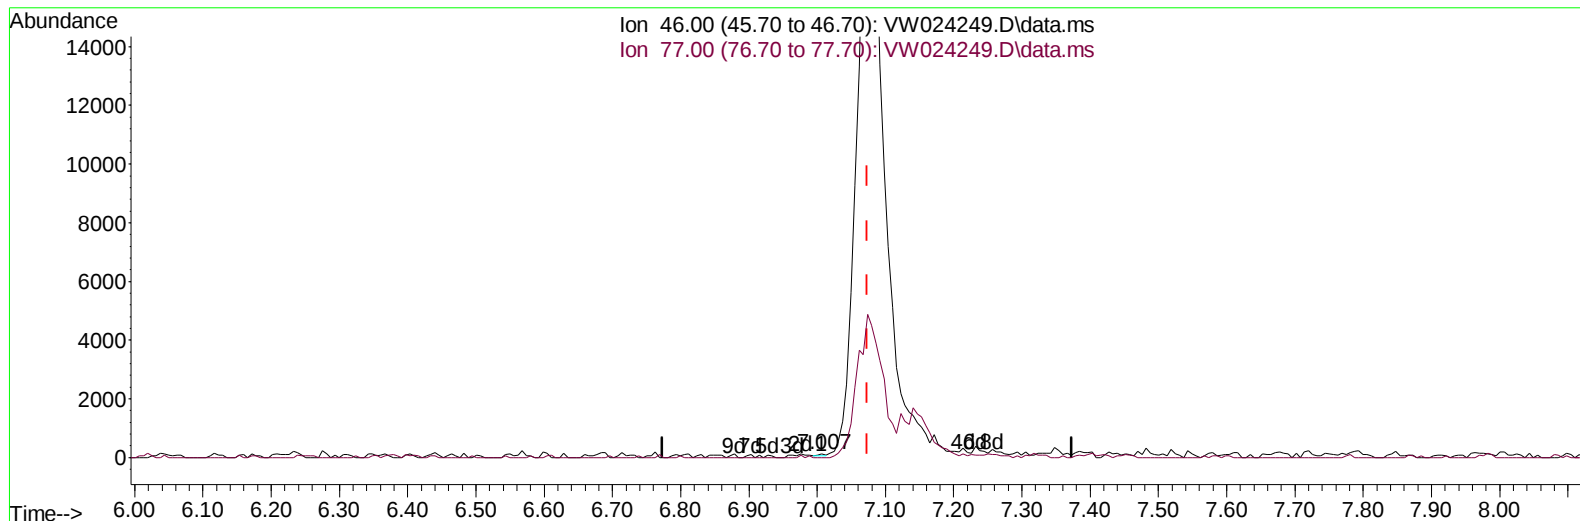

TIC: VW024249.D\data.ms

(21) 2-Butanone-d5 (S)

7.007min (-0.067) 0.04 ug/L

response 41

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.10	43.90#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081622\
 Data File : VW024249.D
 Acq On : 16 Aug 2022 12:37
 Operator : SY/VA
 Sample : VW0816SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK577

Manual IntegrationsAPPROVED

Quant Time: Aug 17 01:01:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 17 01:00:38 2022
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/17/2022
 Supervised By :Semsettin Yesilyurt 08/17/2022

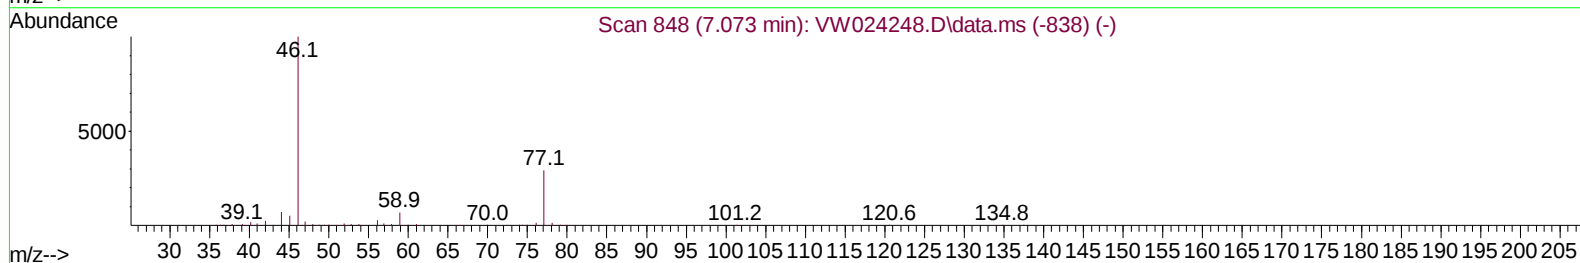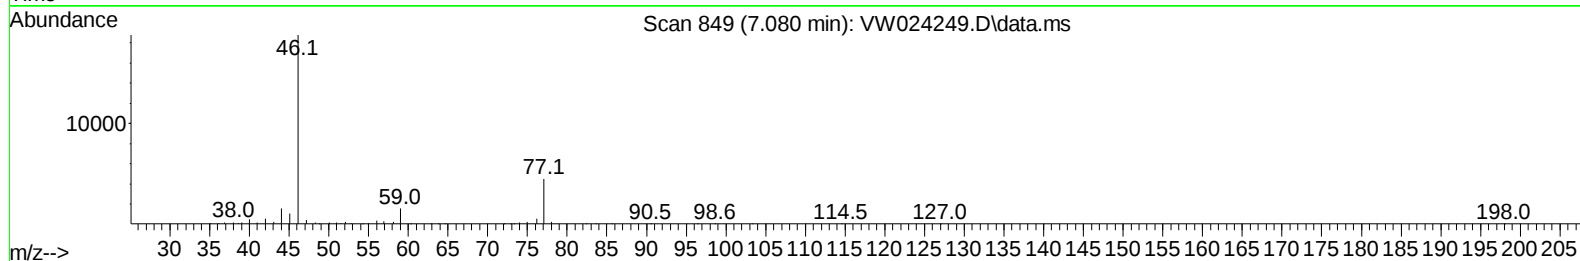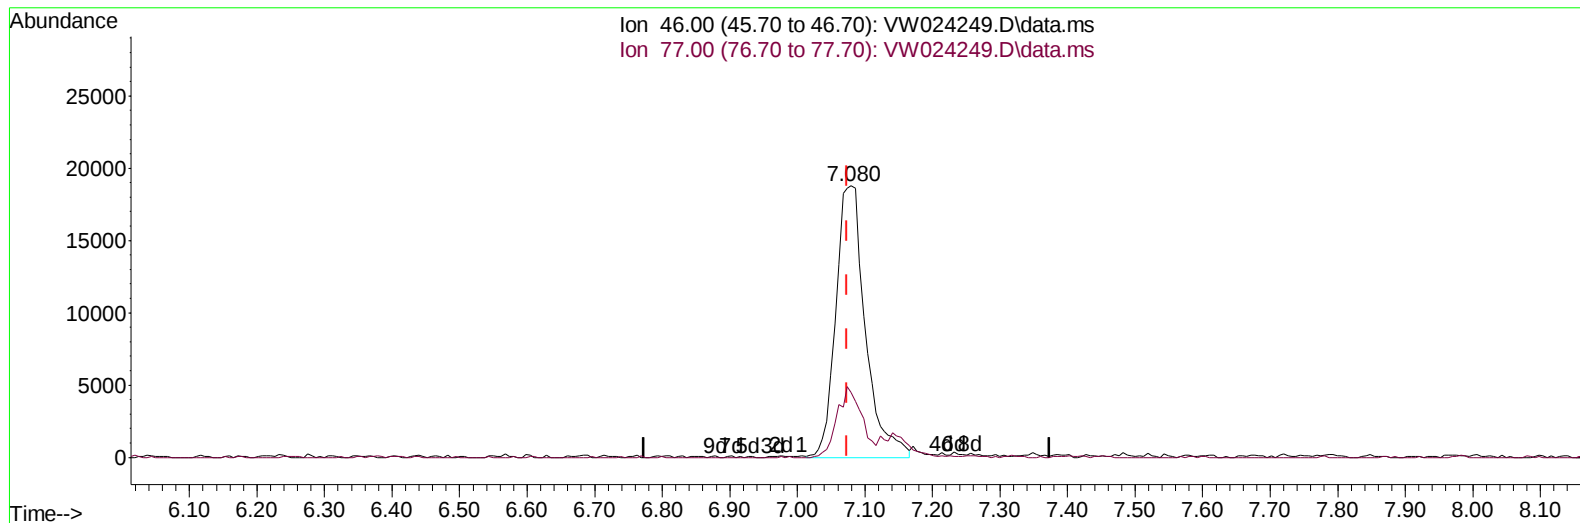

TIC: VW024249.D\data.ms

(21) 2-Butanone-d5 (S)

7.080min (+ 0.007) 57.69 ug/L m

response 57076

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.10	0.03#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081622\
 Data File : VW024249.D
 Acq On : 16 Aug 2022 12:37
 Operator : SY/VA
 Sample : VW0816SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK577

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 08/17/2022
 Supervised By :Semsettin Yesilyurt 08/17/2022

Quant Time: Aug 17 01:01:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 17 01:00:38 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		254420	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		260764	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152		142238	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.343	65		105510	19.840	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	79.360%		
7) Chloroethane-d5	2.873	69		75255	22.716	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	90.880%		
11) 1,1-Dichloroethene-d2	4.001	63		87983	14.517	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110		Recovery =	58.080%		
21) 2-Butanone-d5	7.080	46		57076m	57.688	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	115.380%		
24) Chloroform-d	7.647	84		165498	21.498	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	86.000%		
26) 1,2-Dichloroethane-d4	8.299	65		97246	22.753	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	91.000%		
32) Benzene-d6	8.269	84		305320	19.853	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	79.400%		
36) 1,2-Dichloropropane-d6	9.275	67		99374	21.885	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	87.560%		
41) Toluene-d8	10.323	98		271388	18.880	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	75.520%		
43) trans-1,3-Dichloroprop...	10.573	79		40837	20.533	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	82.120%		
47) 2-Hexanone-d5	10.921	63		42218	50.338	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	100.680%		
56) 1,1,2,2-Tetrachloroeth...	12.689	84		112887	25.625	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	102.480%		
66) 1,2-Dichlorobenzene-d4	13.847	152		125126	24.039	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	96.160%		
Target Compounds							
13) Acetone	4.117	43		3637m	4.993	ug/L	
16) Methylene chloride	4.903	84		20144	4.490	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081622\
Data File : VW024249.D
Acq On : 16 Aug 2022 12:37
Operator : SY/VA
Sample : VW0816SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK577

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 08/17/2022
Supervised By :Semsettin Yesilyurt 08/17/2022

Quant Time: Aug 17 01:01:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Aug 17 01:00:38 2022
Response via : Initial Calibration

