




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081622\
Data File : VW024252.D
Acq On : 16 Aug 2022 14:35
Operator : SY/VA
Sample : N4210-05RE
Misc : 4.34g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGC48RE

Manual IntegrationsAPPROVED

Quant Time: Aug 17 01:02:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Aug 17 01:00:38 2022
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/17/2022
Supervised By :Semsettin Yesilyurt 08/17/2022

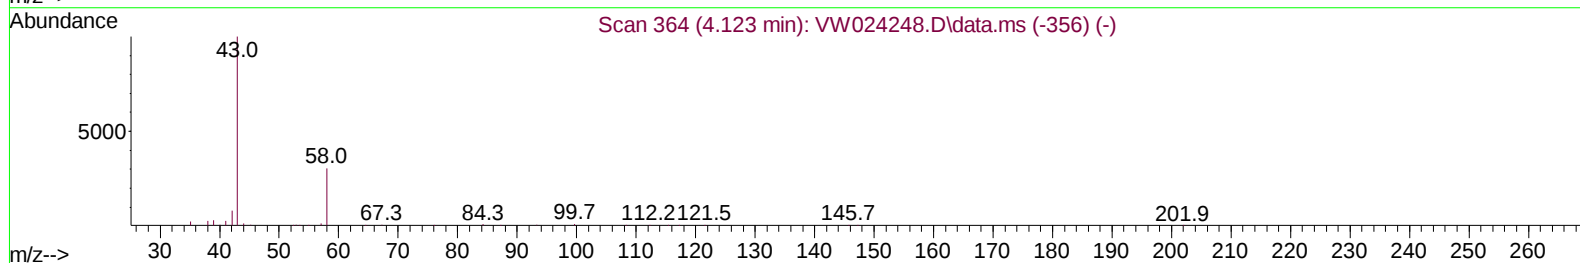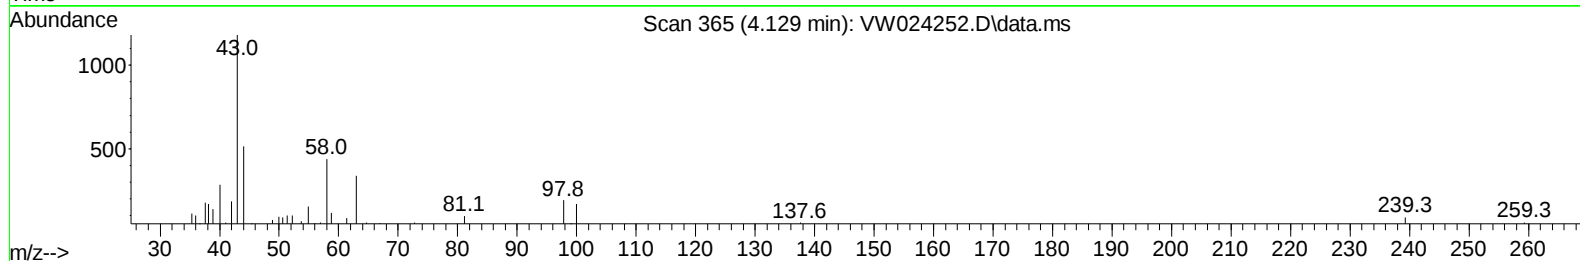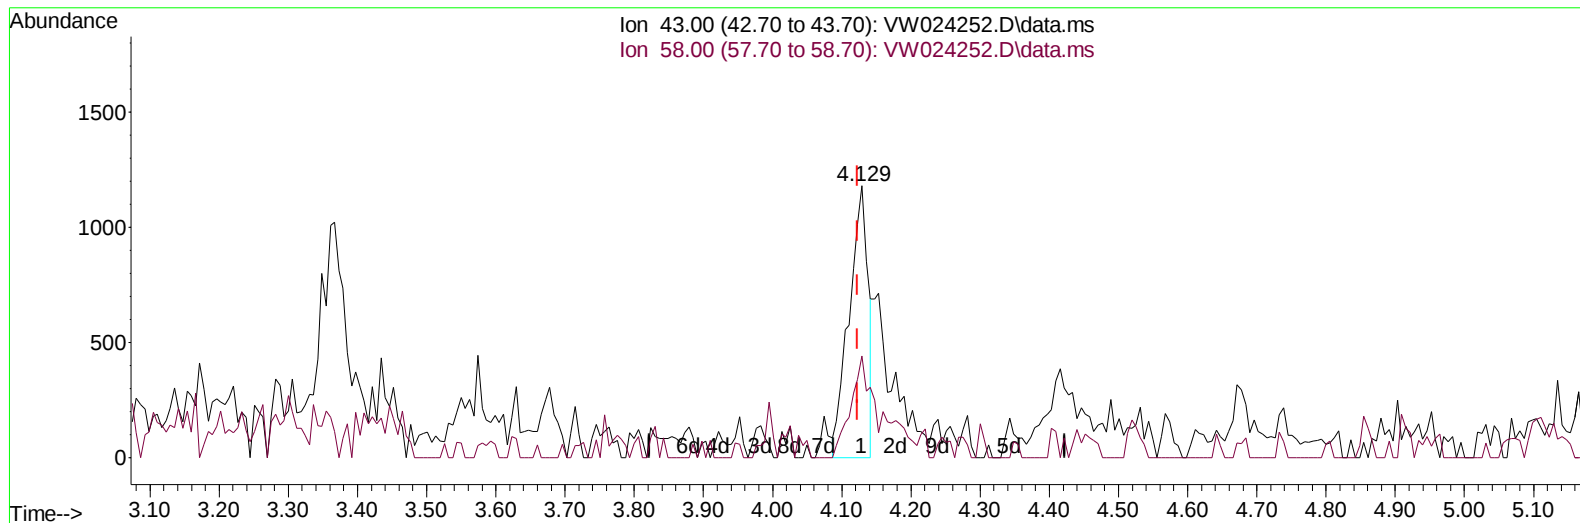

TIC: VW024252.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 2.47 ug/L

response 2254

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	15.90	29.72
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081622\
 Data File : VW024252.D
 Acq On : 16 Aug 2022 14:35
 Operator : SY/VA
 Sample : N4210-05RE
 Misc : 4.34g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGC48RE

Manual IntegrationsAPPROVED

Quant Time: Aug 17 01:02:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 17 01:00:38 2022
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/17/2022
 Supervised By :Semsettin Yesilyurt 08/17/2022

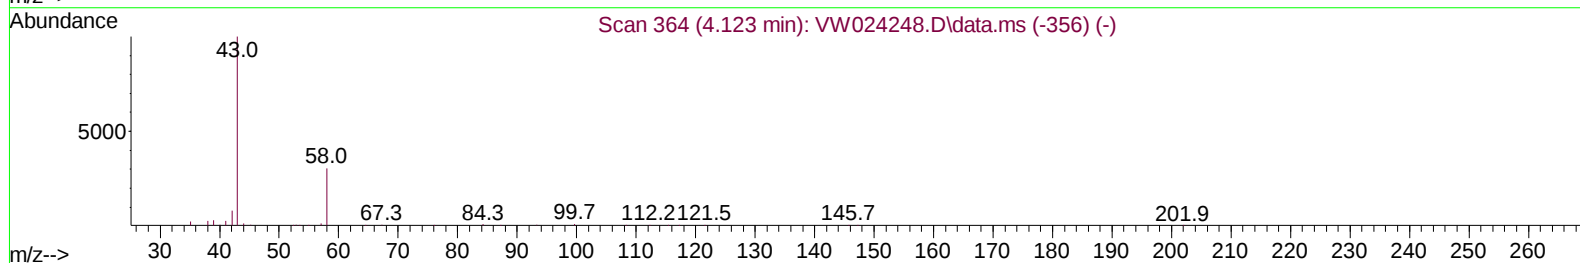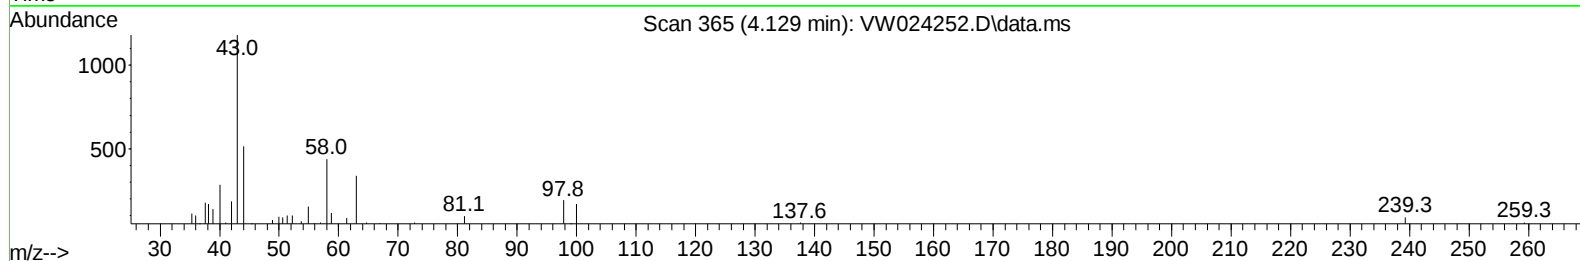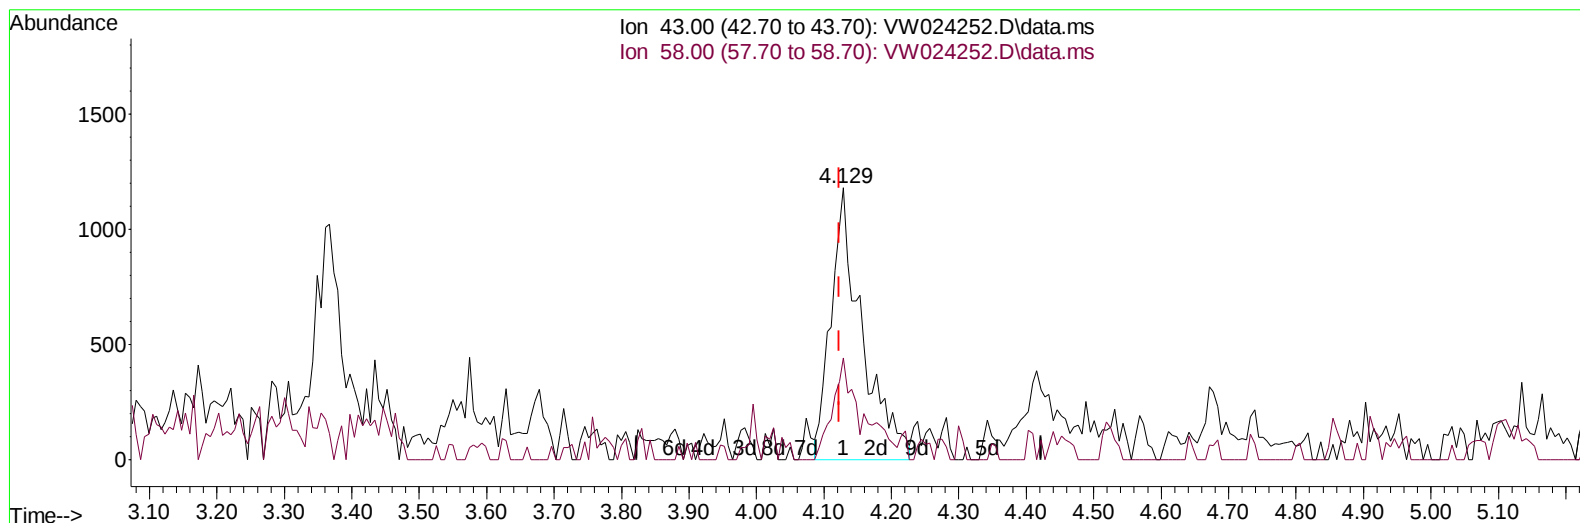

TIC: VW024252.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 4.10 ug/L m

response 3747

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	15.90	17.88
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081622\
 Data File : VW024252.D
 Acq On : 16 Aug 2022 14:35
 Operator : SY/VA
 Sample : N4210-05RE
 Misc : 4.34g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGC48RE

Manual IntegrationsAPPROVED

Quant Time: Aug 17 01:02:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 17 01:00:38 2022
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/17/2022
 Supervised By :Semsettin Yesilyurt 08/17/2022

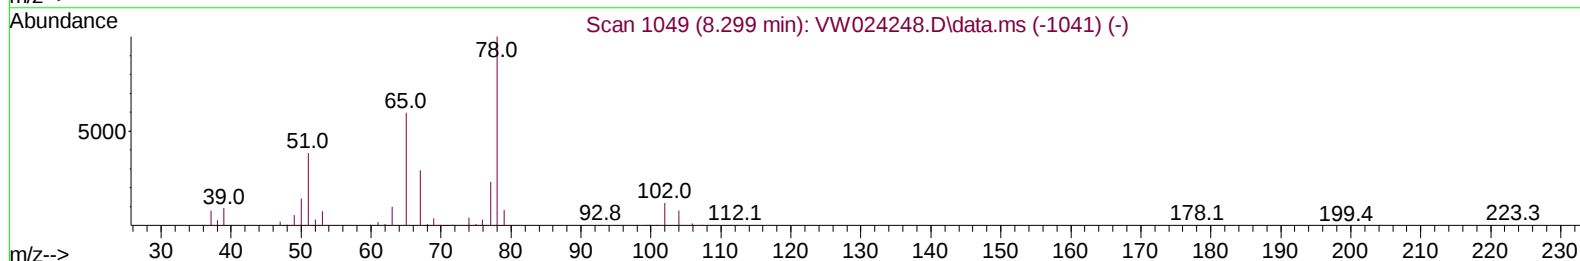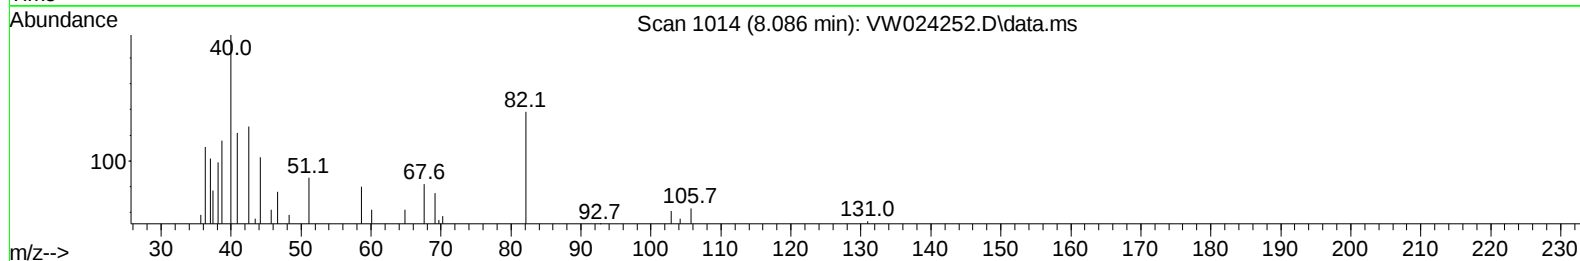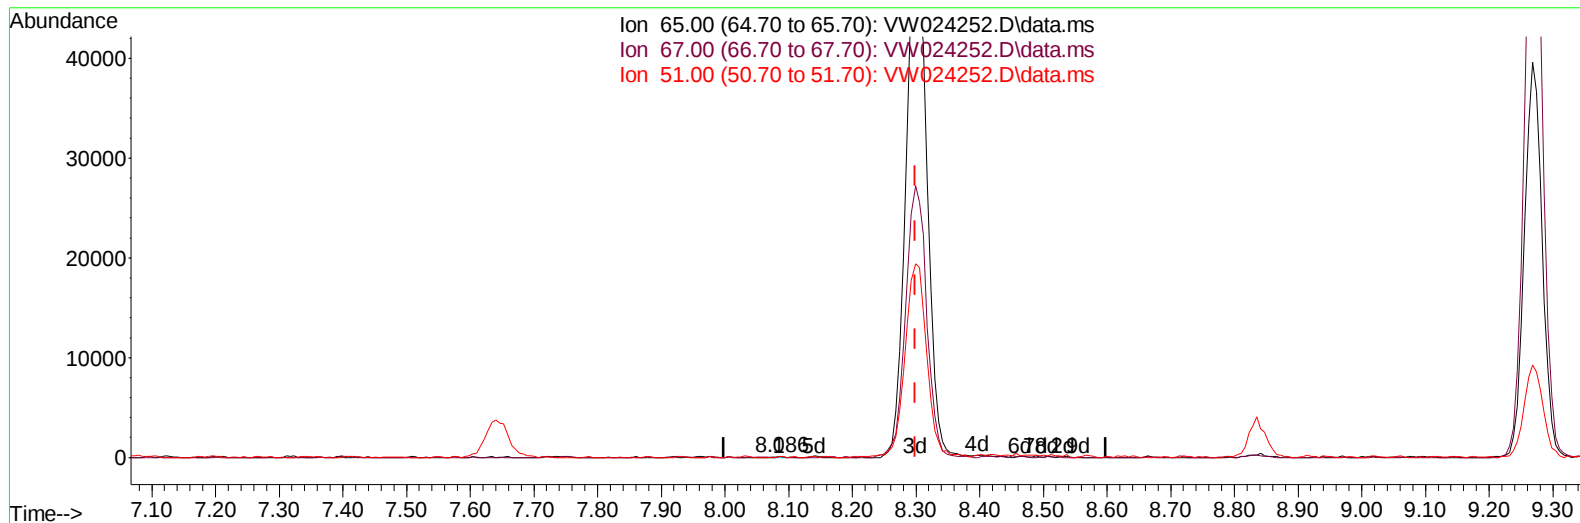

TIC: VW024252.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.086min (-0.213) 0.02 ug/L

response 85

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.00	60.00
51.00	95.20	80.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081622\
Data File : VW024252.D
Acq On : 16 Aug 2022 14:35
Operator : SY/VA
Sample : N4210-05RE
Misc : 4.34g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGC48RE

Manual IntegrationsAPPROVED

Quant Time: Aug 17 01:02:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Aug 17 01:00:38 2022
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/17/2022
Supervised By :Semsettin Yesilyurt 08/17/2022

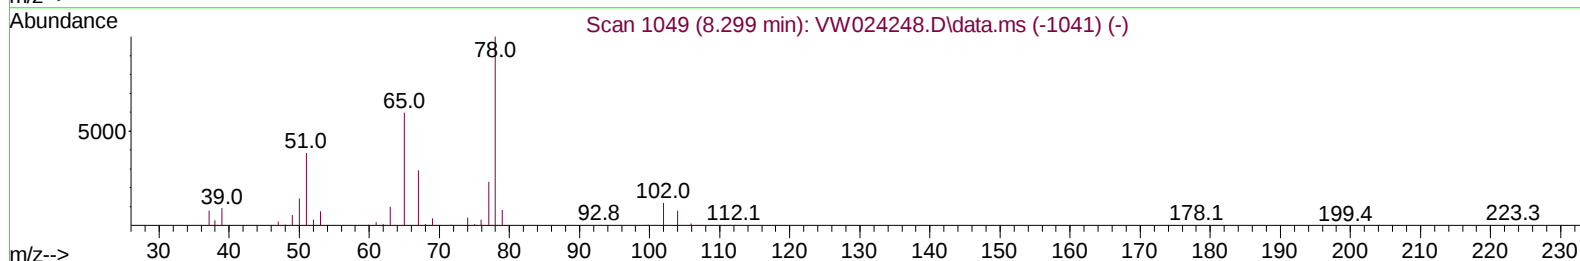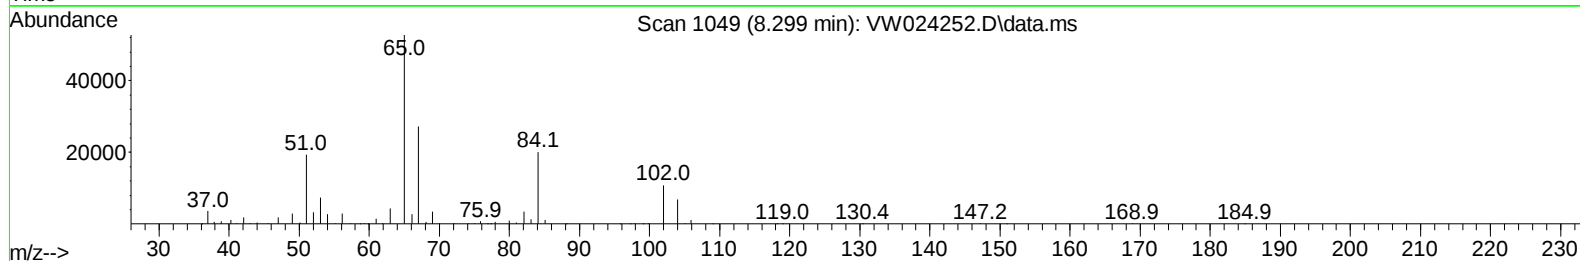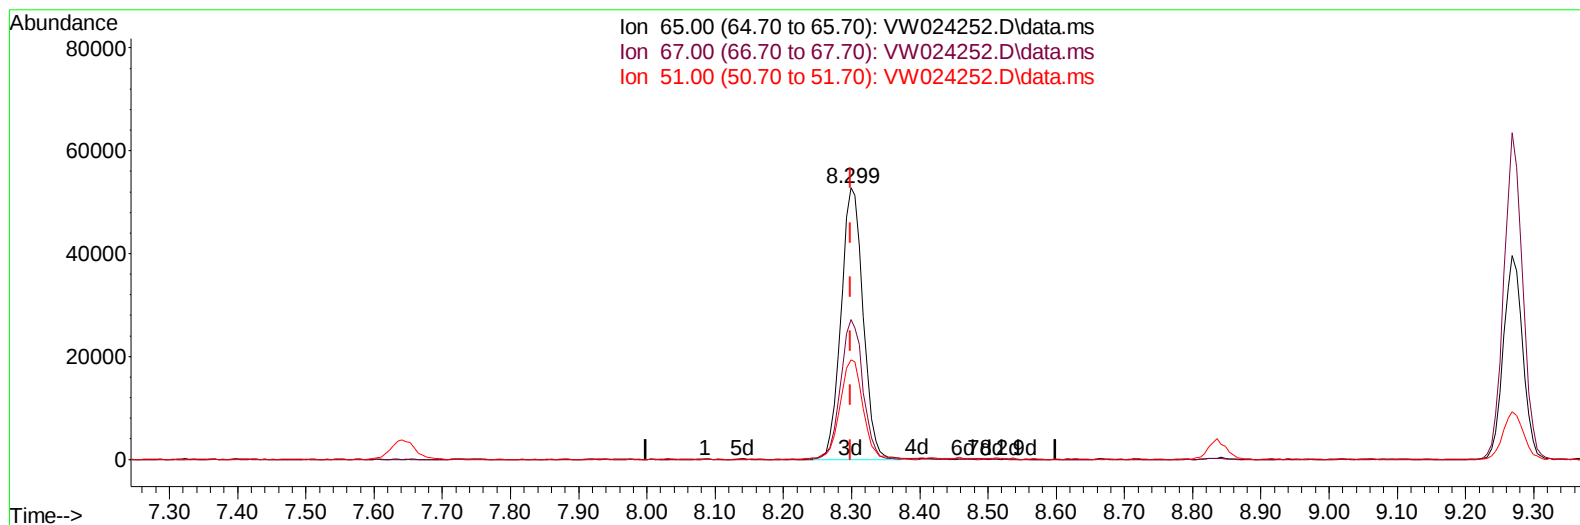

TIC: VW024252.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.299min (+ 0.000) 22.09 ug/L m

response 118316

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.00	0.04#
51.00	95.20	0.06#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081622\
 Data File : VW024252.D
 Acq On : 16 Aug 2022 14:35
 Operator : SY/VA
 Sample : N4210-05RE
 Misc : 4.34g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGC48RE

Manual IntegrationsAPPROVED

Quant Time: Aug 17 01:02:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 17 01:00:38 2022
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/17/2022
 Supervised By :Semsettin Yesilyurt 08/17/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.835	114	318817	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	249032	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	72968	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	144358	21.662	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	86.640%	
7) Chloroethane-d5	2.873	69	90393	21.775	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	87.080%	
11) 1,1-Dichloroethene-d2	4.001	63	126445	16.649	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110	Recovery	=	66.600%	
21) 2-Butanone-d5	7.080	46	46462	37.475	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	74.940%	
24) Chloroform-d	7.641	84	218586	22.659	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	90.640%	
26) 1,2-Dichloroethane-d4	8.299	65	118316m	22.091	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	88.360%	
32) Benzene-d6	8.269	84	395907	26.956	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	107.840%	
36) 1,2-Dichloropropane-d6	9.268	67	121355	27.985	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	111.960%	
41) Toluene-d8	10.317	98	327380	23.848	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	95.400%	
43) trans-1,3-Dichloroprop...	10.573	79	42879	22.576	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	90.320%	
47) 2-Hexanone-d5	10.920	63	34991	43.686	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	87.380%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	93508	22.226	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	88.920%	
66) 1,2-Dichlorobenzene-d4	13.853	152	64962	24.329	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	97.320%	
Target Compounds						
13) Acetone	4.129	43	3747m	4.105	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081622\
Data File : VW024252.D
Acq On : 16 Aug 2022 14:35
Operator : SY/VA
Sample : N4210-05RE
Misc : 4.34g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGC48RE

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 08/17/2022
Supervised By :Semsettin Yesilyurt 08/17/2022

Quant Time: Aug 17 01:02:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Aug 17 01:00:38 2022
Response via : Initial Calibration

