




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081622\
 Data File : VW024254.D
 Acq On : 16 Aug 2022 15:24
 Operator : SY/VA
 Sample : N4210-10RE
 Misc : 5.99g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGC53RE

Manual IntegrationsAPPROVED

Quant Time: Aug 17 01:02:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 17 01:00:38 2022
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/17/2022
 Supervised By :Semsettin Yesilyurt 08/17/2022

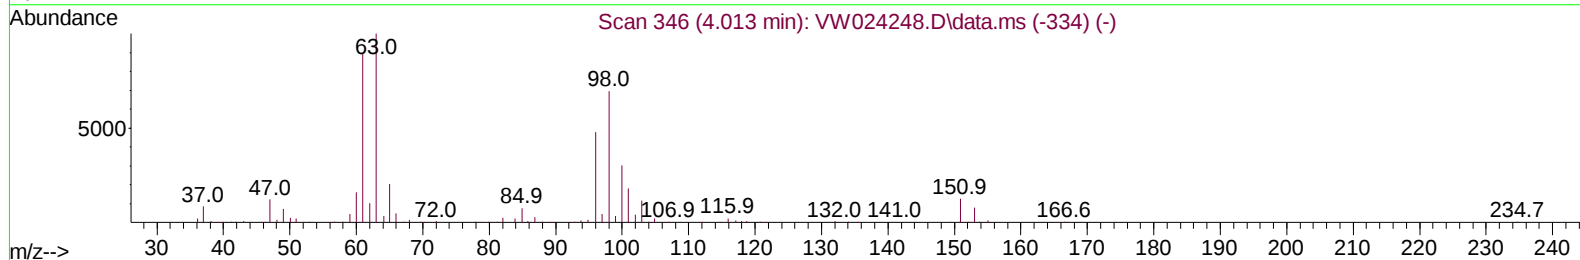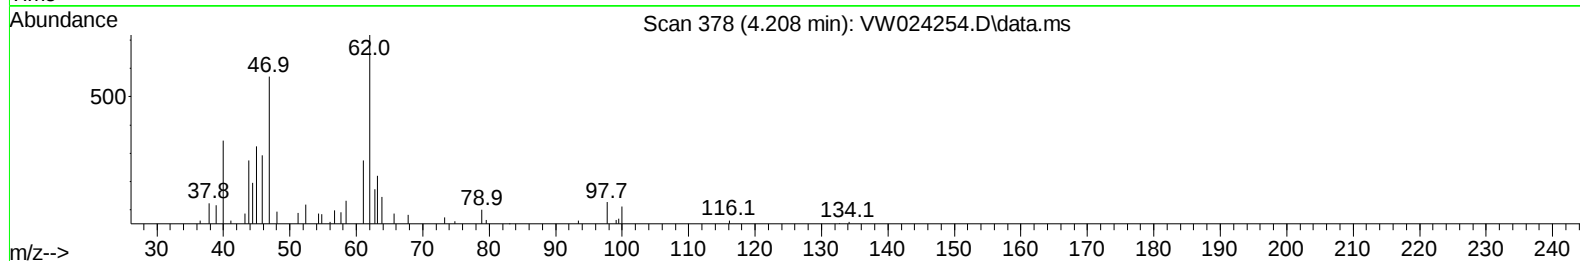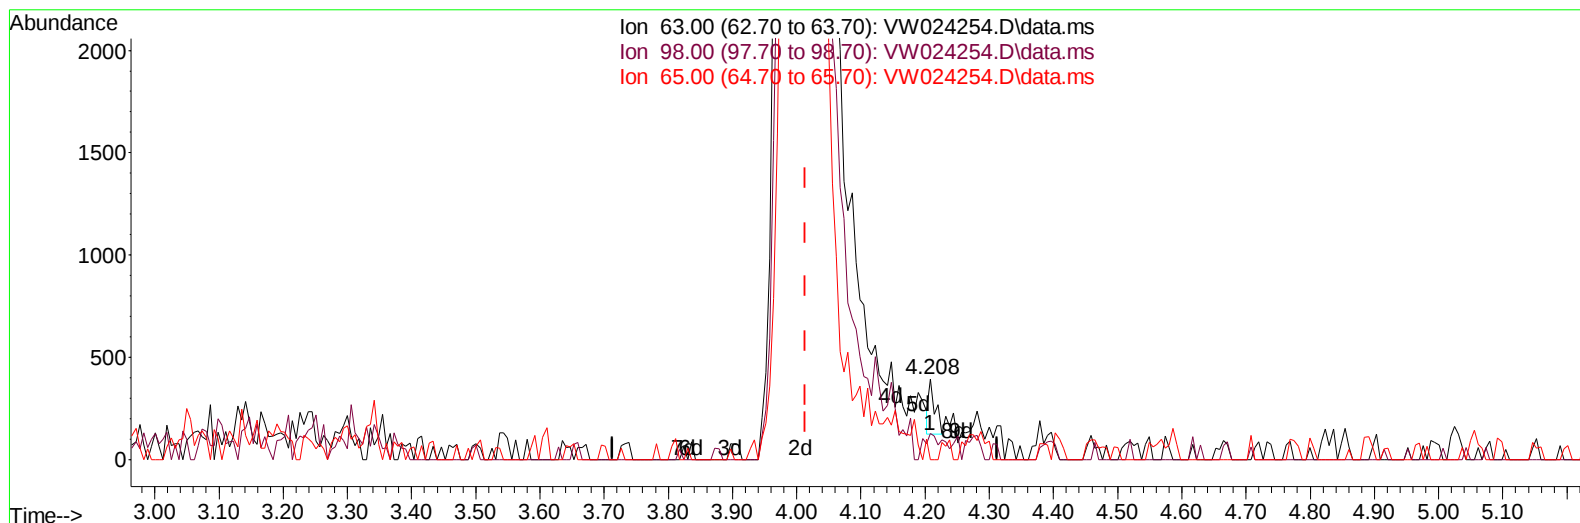

TIC: VW024254.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.208min (+ 0.195) 0.03 ug/L

response 188

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	75.50	95.21
65.00	23.50	19.15
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081622\
 Data File : VW024254.D
 Acq On : 16 Aug 2022 15:24
 Operator : SY/VA
 Sample : N4210-10RE
 Misc : 5.99g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGC53RE

Manual IntegrationsAPPROVED

Quant Time: Aug 17 01:02:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 17 01:00:38 2022
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/17/2022
 Supervised By :Semsettin Yesilyurt 08/17/2022

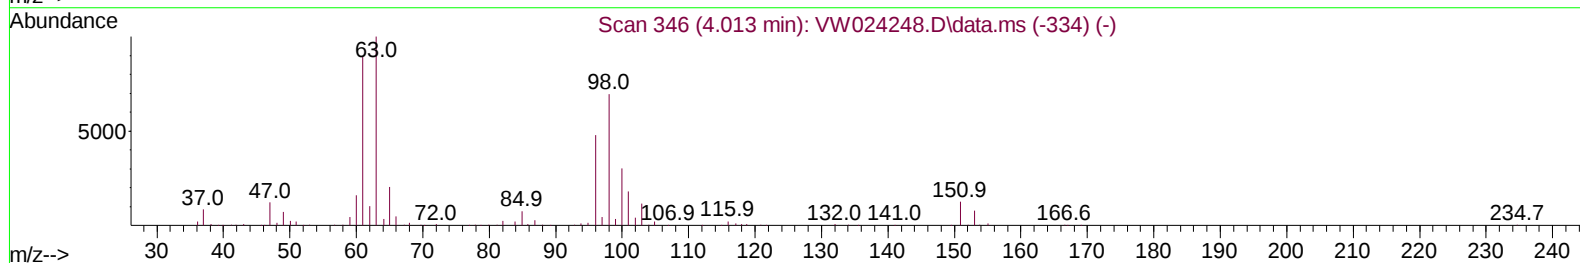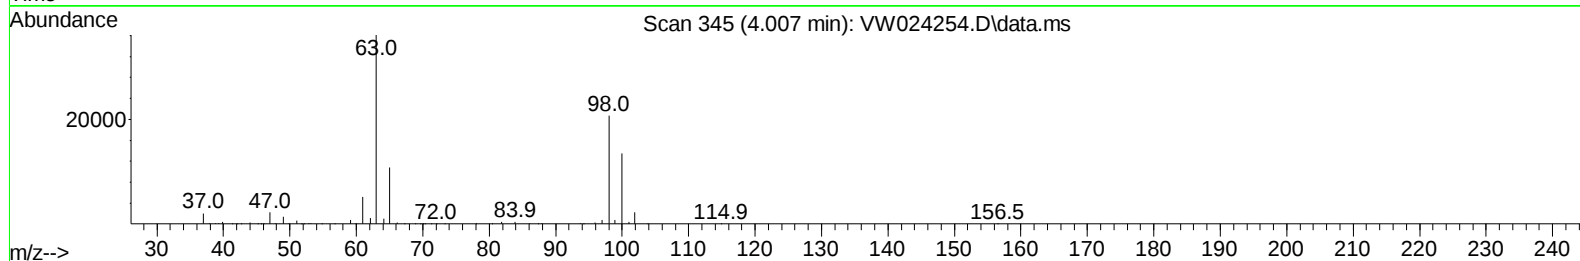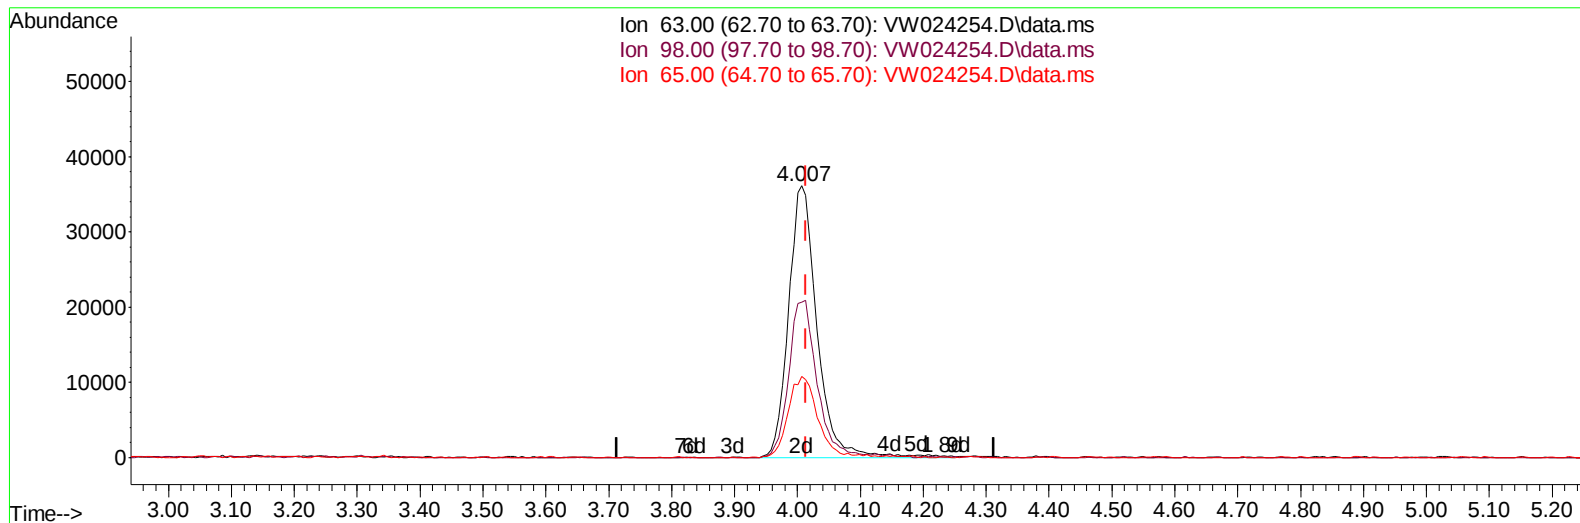

TIC: VW024254.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.007min (-0.006) 18.00 ug/L m

response 113379

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	75.50	0.16#
65.00	23.50	0.03#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081622\
 Data File : VW024254.D
 Acq On : 16 Aug 2022 15:24
 Operator : SY/VA
 Sample : N4210-10RE
 Misc : 5.99g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGC53RE

Manual IntegrationsAPPROVED

Quant Time: Aug 17 01:02:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 17 01:00:38 2022
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/17/2022
 Supervised By :Semsettin Yesilyurt 08/17/2022

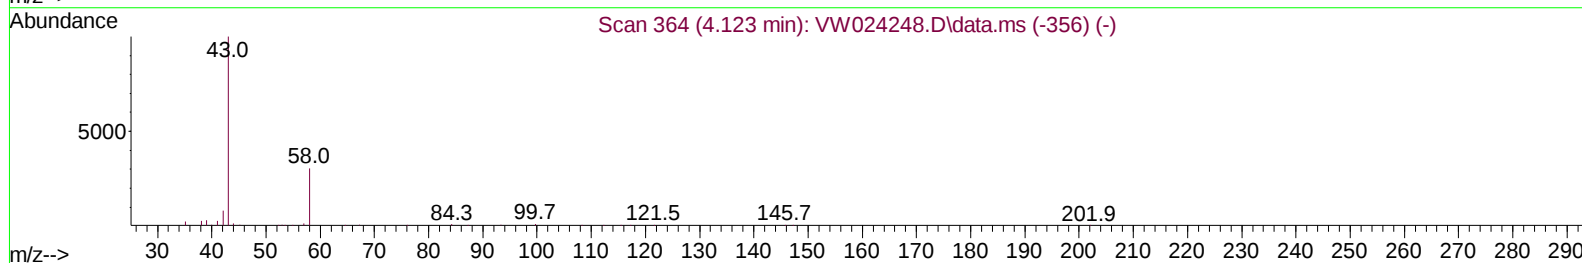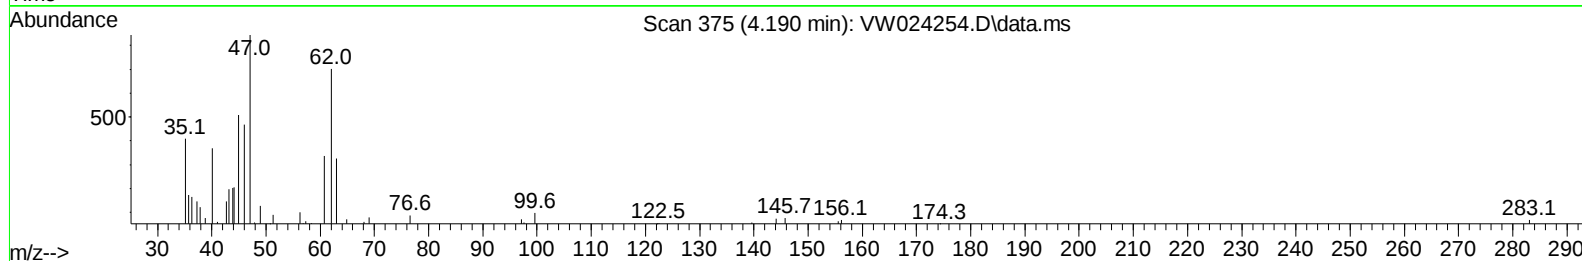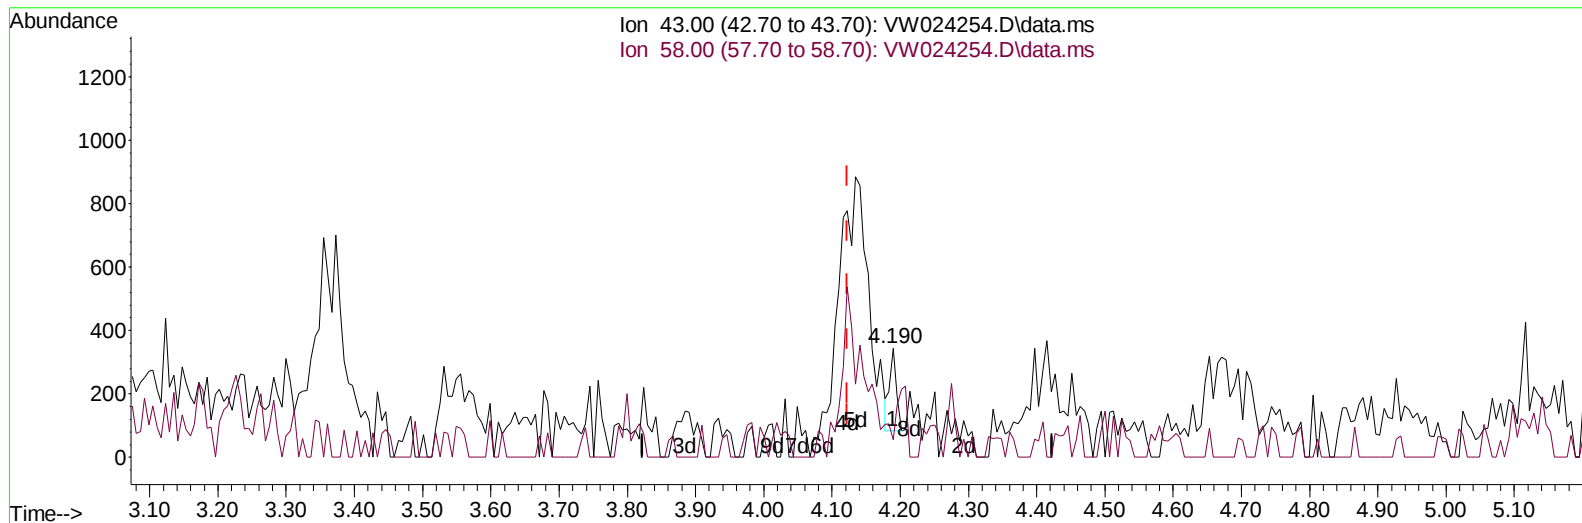

TIC: VW024254.D\data.ms

(13) Acetone (T)

4.190min (+ 0.067) 0.24 ug/L

response 180

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	15.90	20.00
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081622\
 Data File : VW024254.D
 Acq On : 16 Aug 2022 15:24
 Operator : SY/VA
 Sample : N4210-10RE
 Misc : 5.99g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGC53RE

Manual IntegrationsAPPROVED

Quant Time: Aug 17 01:02:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 17 01:00:38 2022
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/17/2022
 Supervised By :Semsettin Yesilyurt 08/17/2022

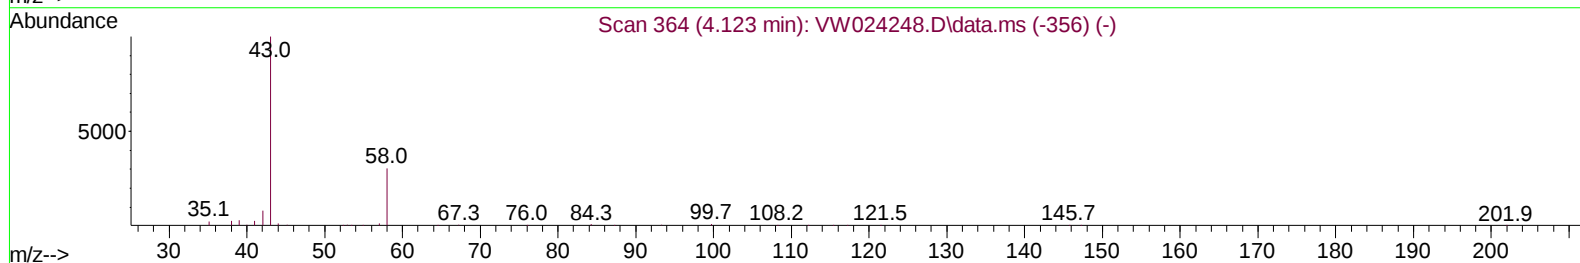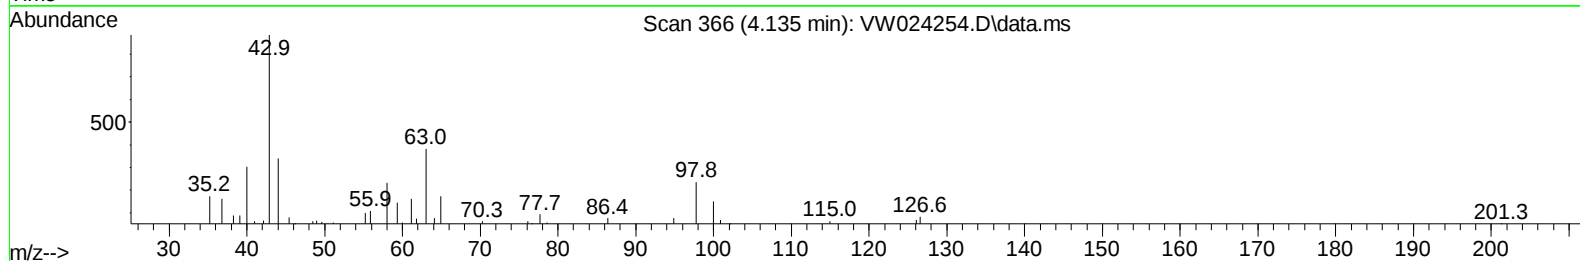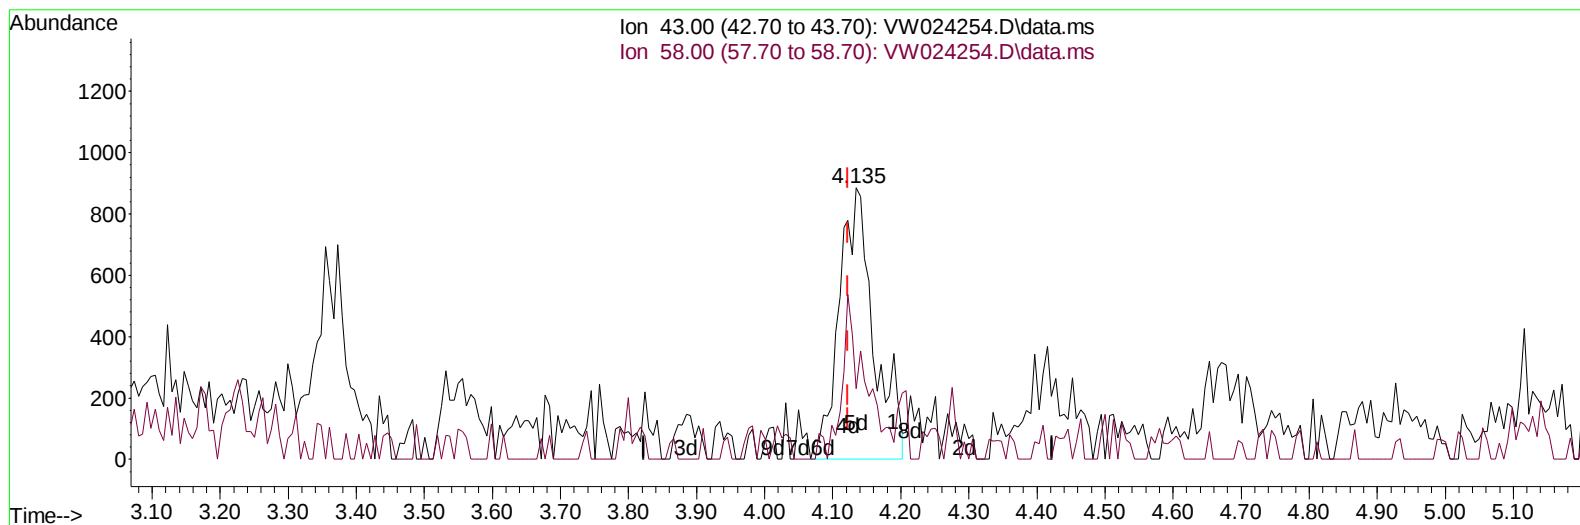

TIC: VW024254.D\data.ms

(13) Acetone (T)

4.135min (+ 0.012) 4.15 ug/L m

response 3142

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	15.90	1.15
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081622\
 Data File : VW024254.D
 Acq On : 16 Aug 2022 15:24
 Operator : SY/VA
 Sample : N4210-10RE
 Misc : 5.99g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGC53RE

Manual IntegrationsAPPROVED

Quant Time: Aug 17 01:02:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 17 01:00:38 2022
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/17/2022
 Supervised By :Semsettin Yesilyurt 08/17/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	264365	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.633	117	203454	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	56902	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.342	65	137235	24.835	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	99.320%	
7) Chloroethane-d5	2.873	69	90871	26.398	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	105.600%	
11) 1,1-Dichloroethene-d2	4.007	63	113379m	18.003	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	72.000%	
21) 2-Butanone-d5	7.073	46	47115	45.829	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	91.660%	
24) Chloroform-d	7.646	84	201505	25.191	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	100.760%	
26) 1,2-Dichloroethane-d4	8.305	65	112904	25.423	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	101.680%	
32) Benzene-d6	8.268	84	346553	28.882	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	115.520%	
36) 1,2-Dichloropropane-d6	9.274	67	109383	30.875	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	123.520%#	
41) Toluene-d8	10.323	98	279925	24.959	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	99.840%	
43) trans-1,3-Dichloroprop...	10.573	79	38644	24.904	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	99.600%	
47) 2-Hexanone-d5	10.926	63	34197	52.260	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	104.520%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	98589	28.683	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	114.720%	
66) 1,2-Dichlorobenzene-d4	13.853	152	56753	27.255	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	109.040%	
Target Compounds						
13) Acetone	4.135	43	3142m	4.151	ug/L	
16) Methylene chloride	4.909	84	22122	4.745	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081622\
Data File : VW024254.D
Acq On : 16 Aug 2022 15:24
Operator : SY/VA
Sample : N4210-10RE
Misc : 5.99g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGC53RE

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 08/17/2022
Supervised By :Semsettin Yesilyurt 08/17/2022

Quant Time: Aug 17 01:02:47 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Aug 17 01:00:38 2022
Response via : Initial Calibration

