




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081623\
Data File : VW026753.D
Acq On : 16 Aug 2023 10:55
Operator : SY/MD
Sample : 03965-11
Misc : 5.38g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A48J5

Manual IntegrationsAPPROVED

Quant Time: Aug 17 01:30:02 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Aug 17 01:28:59 2023
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/17/2023
Supervised By :Mahesh Dadoda 08/17/2023

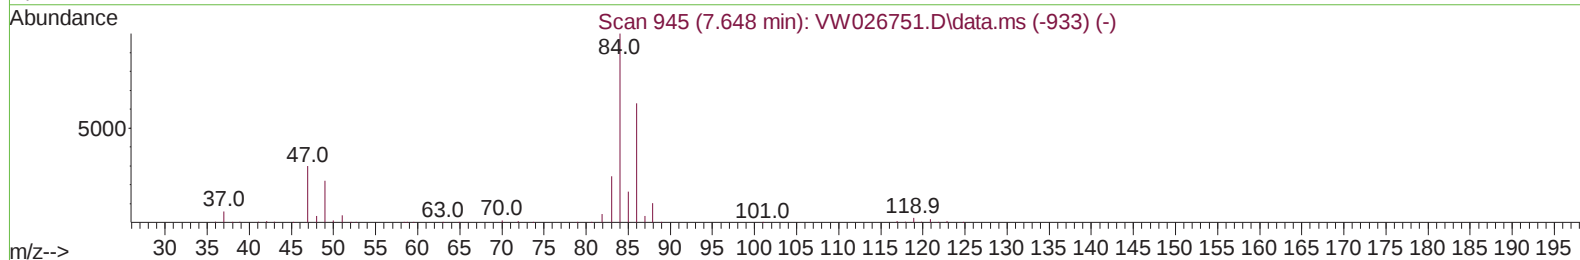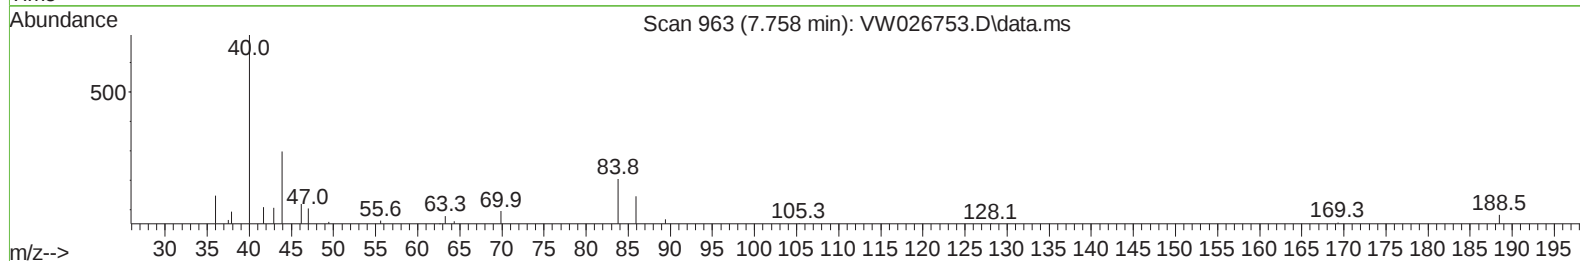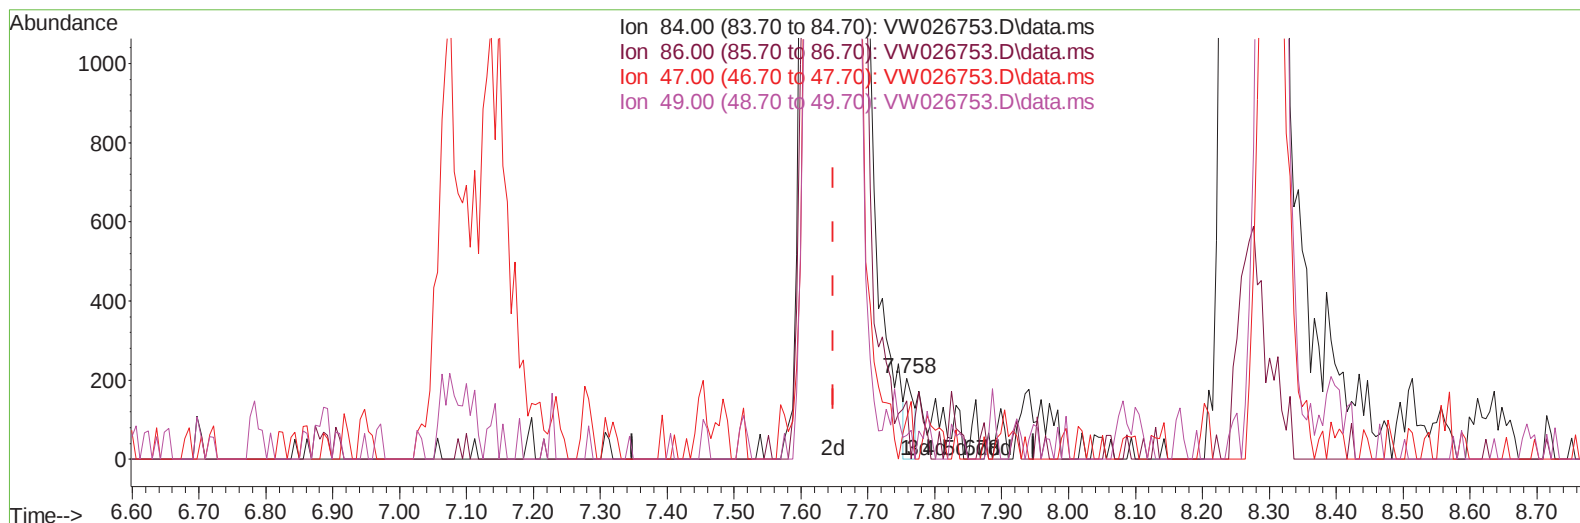

TIC: VW026753.D\data.ms

(24) Chloroform-d (S)

7.758min (+ 0.110) 0.01 ug/L

response 181

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.80	78.45
47.00	49.30	64.09
49.00	28.20	27.07




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081623\
 Data File : VW026753.D
 Acq On : 16 Aug 2023 10:55
 Operator : SY/MD
 Sample : 03965-11
 Misc : 5.38g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A48J5

Manual IntegrationsAPPROVED

Quant Time: Aug 17 01:30:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Aug 17 01:28:59 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/17/2023
 Supervised By :Mahesh Dadoda 08/17/2023

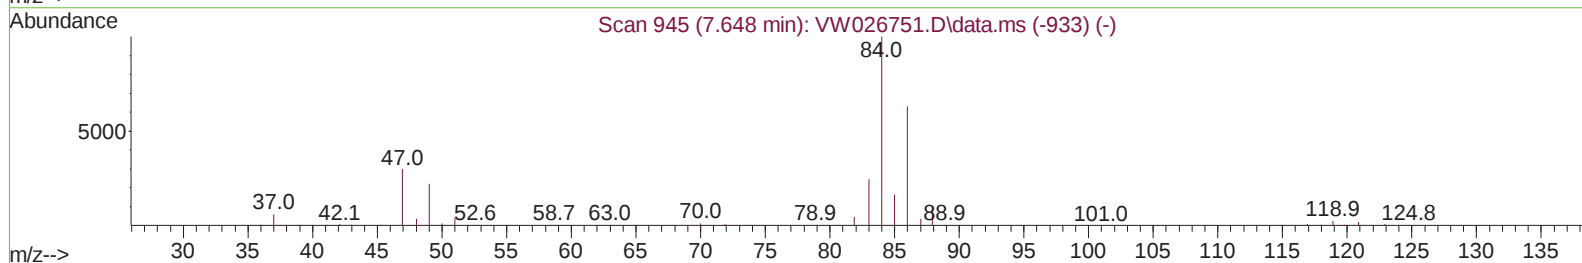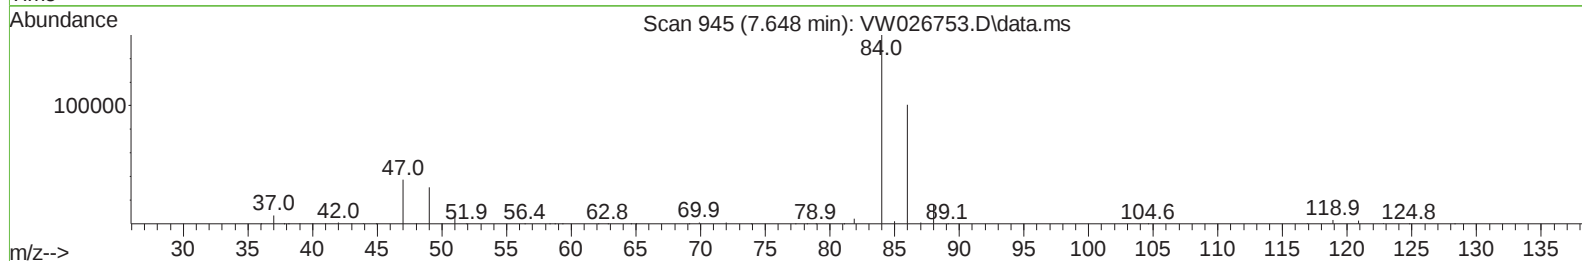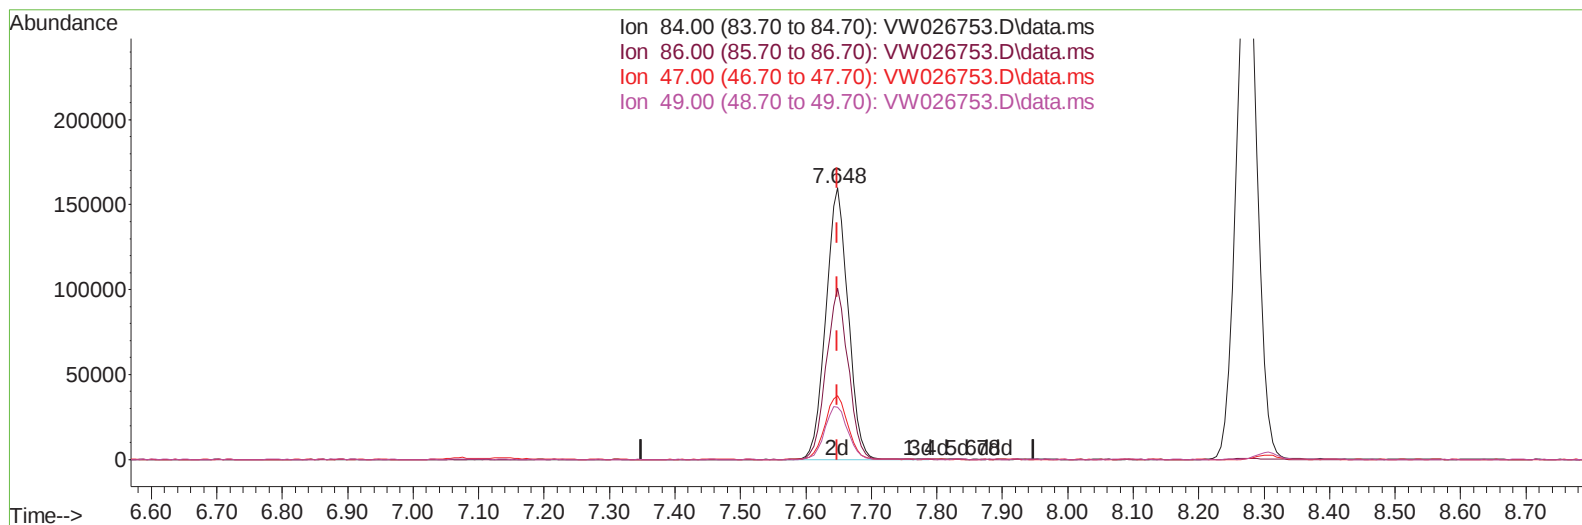

TIC: VW026753.D\data.ms

(24) Chloroform-d (S)

7.648min (+ 0.000) 20.03 ug/L m

response 378997

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.80	0.04#
47.00	49.30	0.03#
49.00	28.20	0.01#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081623\
 Data File : VW026753.D
 Acq On : 16 Aug 2023 10:55
 Operator : SY/MD
 Sample : 03965-11
 Misc : 5.38g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A48J5

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/17/2023
 Supervised By :Mahesh Dadoda 08/17/2023

Quant Time: Aug 17 01:30:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Aug 17 01:28:59 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	563892	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	443208	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	139409	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	134695	14.531	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	58.120%	
7) Chloroethane-d5	2.893	69	112141	16.269	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	65.080%	
11) 1,1-Dichloroethene-d2	4.021	65	74078	16.248	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	65.000%	
21) 2-Butanone-d5	7.075	46	98330	36.906	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	73.820%	
24) Chloroform-d	7.648	84	378997m	20.025	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	80.120%	
26) 1,2-Dichloroethane-d4	8.307	65	235043	22.505	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	90.000%	
32) Benzene-d6	8.276	84	704566	23.066	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	92.280%	
36) 1,2-Dichloropropane-d6	9.276	67	239660	25.188	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	100.760%	
41) Toluene-d8	10.319	98	544147	20.753	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	83.000%	
43) trans-1,3-Dichloroprop...	10.581	79	80773	20.561	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	82.240%	
47) 2-Hexanone-d5	10.922	63	48261	48.272	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	96.540%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	180649	24.042	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	96.160%	
66) 1,2-Dichlorobenzene-d4	13.848	152	99198	19.880	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	79.520%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081623\
Data File : VW026753.D
Acq On : 16 Aug 2023 10:55
Operator : SY/MD
Sample : 03965-11
Misc : 5.38g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A48J5

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/17/2023
Supervised By :Mahesh Dadoda 08/17/2023

Quant Time: Aug 17 01:30:02 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Aug 17 01:28:59 2023
Response via : Initial Calibration

