

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW081818\
 Data File : VW004727.D
 Acq On : 16 Aug 2018 11:07
 Operator : SY/AP
 Sample : VW0818SBL01
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Aug 16 18:26:43 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM081418S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 16 02:39:24 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	843646	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	843457	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	384195	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	310735	23.17	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	92.68%
7) Chloroethane-d5	2.90	69	242344	23.38	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.52%
10) 1,1-Dichloroethene-d2	4.01	63	425976	17.37	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	69.48%
20) 2-Butanone-d5	7.09	46	198922	54.82	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	109.64%
24) Chloroform-d	7.65	84	544366	24.08	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	96.32%
26) 1,2-Dichloroethane-d4	8.31	65	303581	25.34	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	101.36%
29) Benzene-d6	8.28	84	1114021	23.55	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	94.20%
33) 1,2-Dichloropropane-d6	9.28	67	350217	23.84	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.36%
37) Toluene-d8	10.33	98	985446	23.22	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	92.88%
38) trans-1,3-Dichloropropene-	10.58	79	139501	23.38	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	93.52%
39) 2-Hexanone-d5	10.93	63	155950	53.11	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	106.22%
48) 1,1,2,2-Tetrachloroethane-	12.70	84	344872	25.02	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	100.08%
61) 1,2-Dichlorobenzene-d4	13.86	152	386115	26.49	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	105.96%


Target Compounds					Ovalue
59) 1,2,3-Trichloropropane	13.57	75	43915	4.201 ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW081818\
Data File : VW004727.D
Acq On : 16 Aug 2018 11:07
Operator : SY/AP
Sample : VW0818SBL01
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Aug 16 18:26:43 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM081418S.M
Quant Title : VOC Analysis
QLast Update : Thu Aug 16 02:39:24 2018
Response via : Initial Calibration

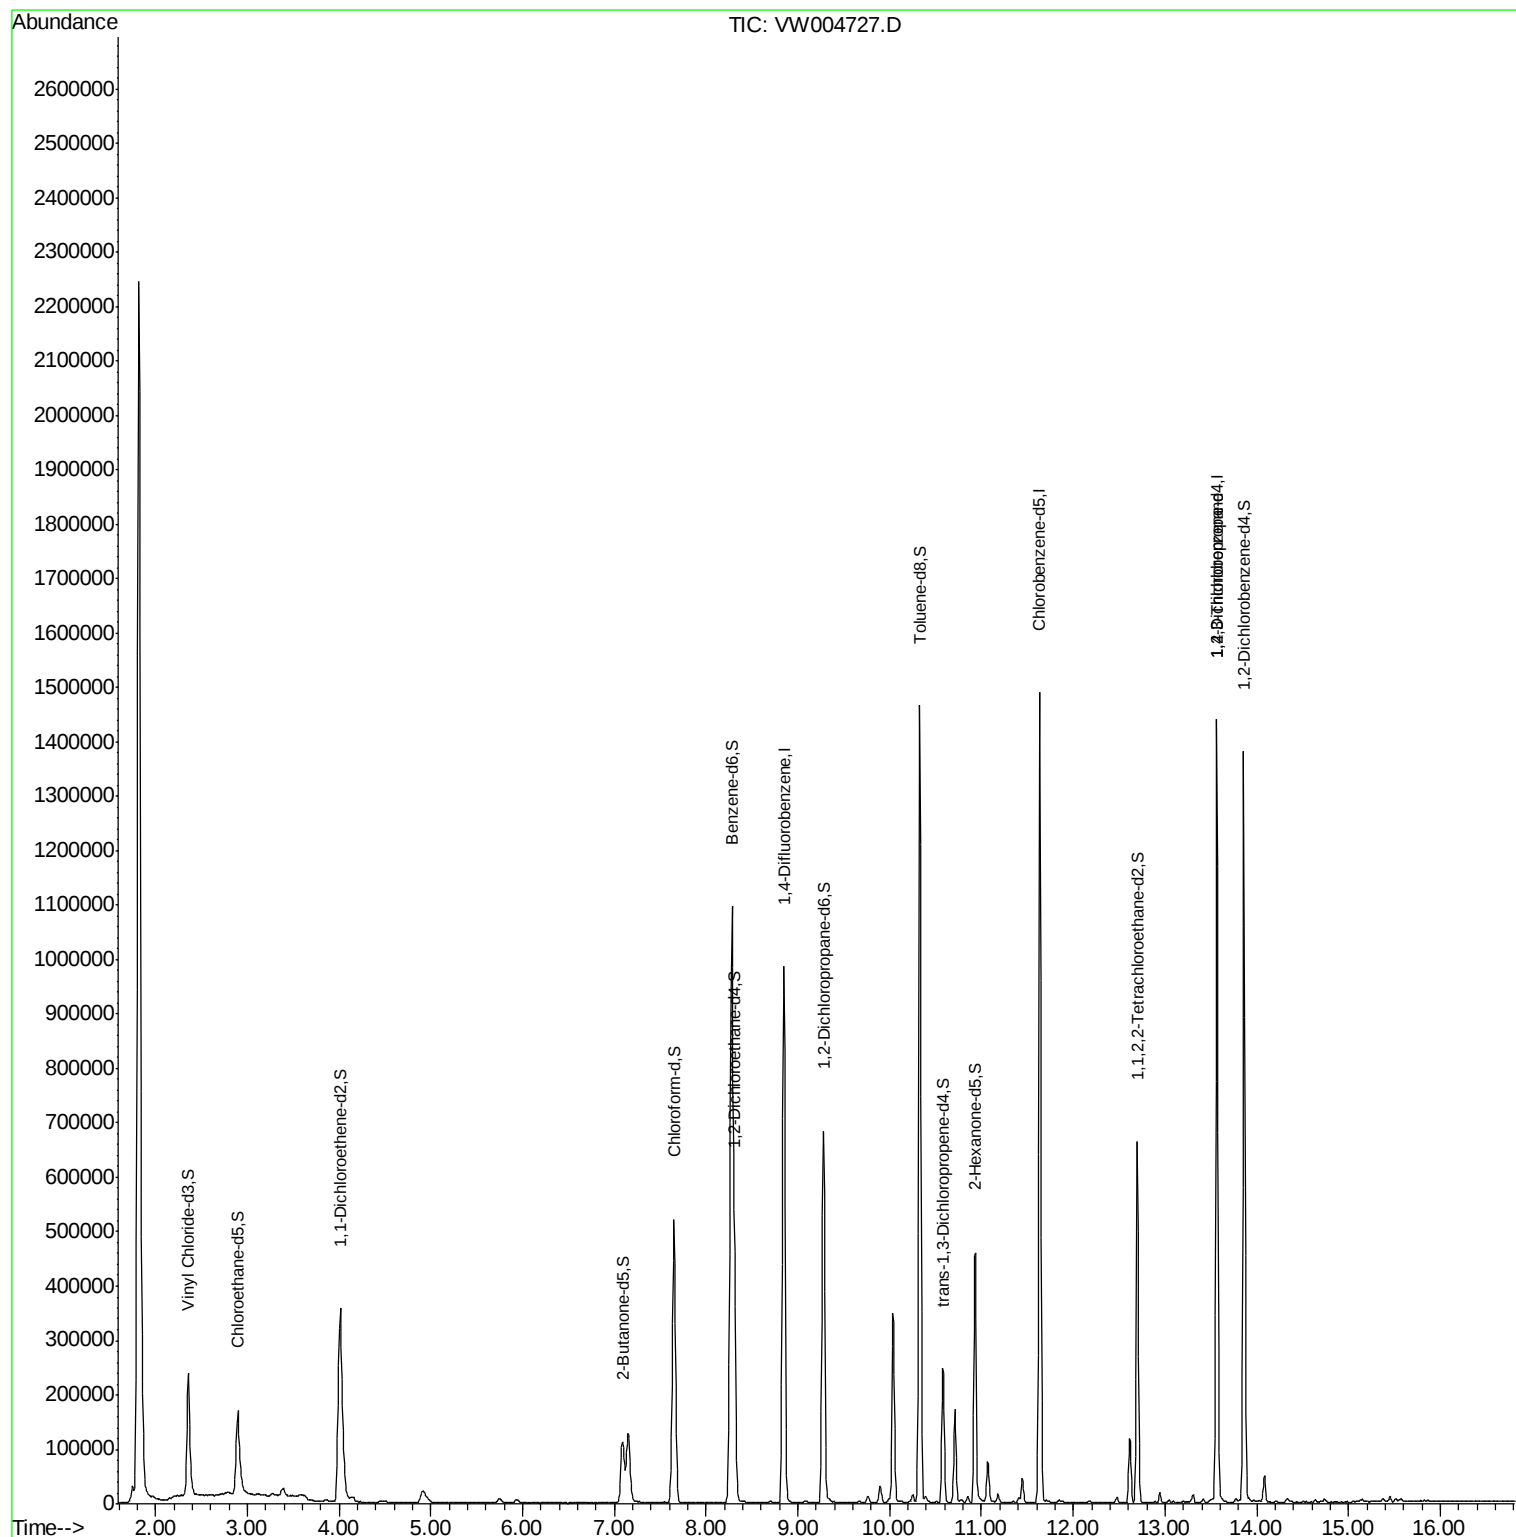

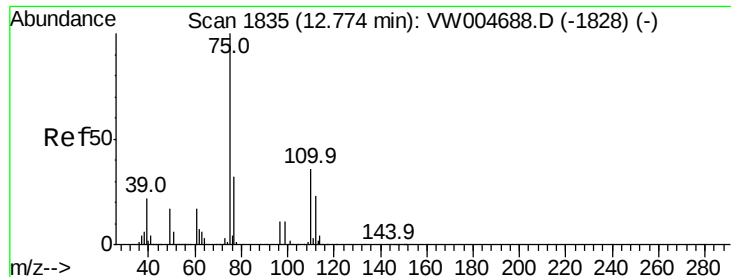

#59

1,2,3-Trichloropropane

Concen: 4.201 ug/L

RT: 13.57 min Scan# 1965

Delta R.T. 0.79 min

Lab File: VW004727.D

Acq: 16 Aug 2018 11:07

Instrument :

MSVOA_W

ClientSampleId :

Tot Ion: 75 Resp: 43915

Ion Ratio Lower Upper

75 100

77 37.4 25.8 38.6

