
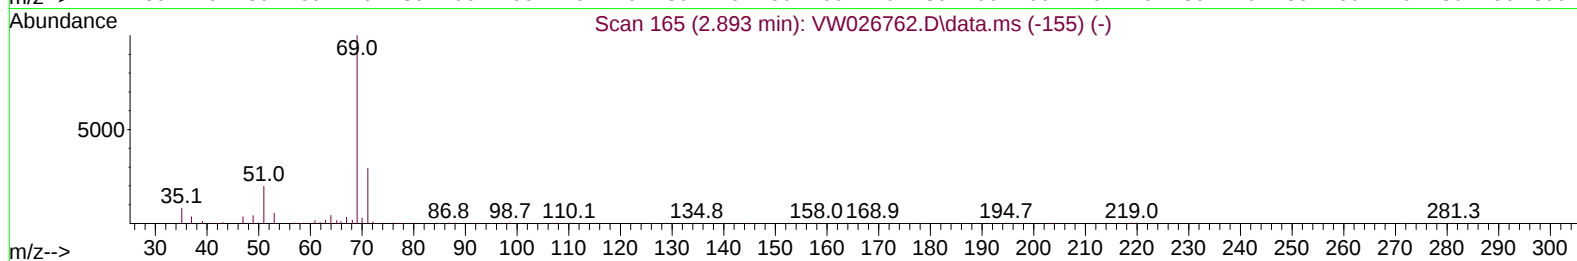
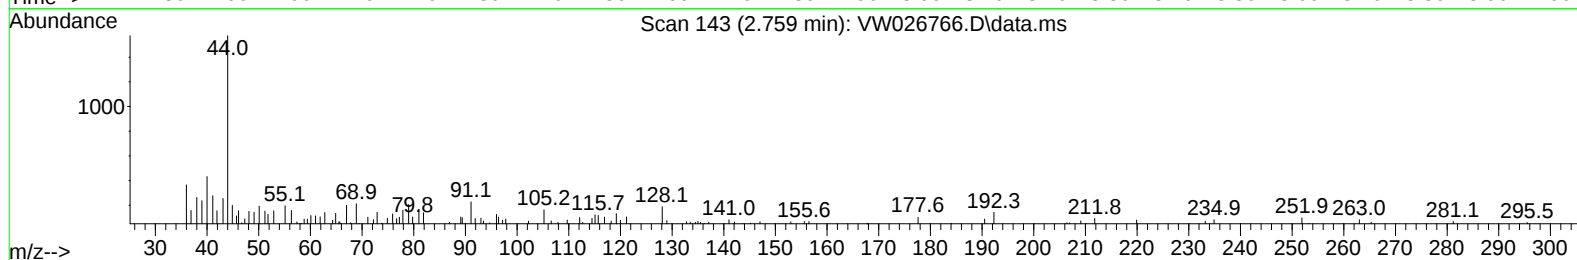


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081823\
Data File : VW026766.D
Acq On : 18 Aug 2023 13:44
Operator : SY/MD
Sample : 04037-03
Misc : 5.43g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 18 23:43:48 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 18 23:42:21 2023
Response via : Initial Calibration

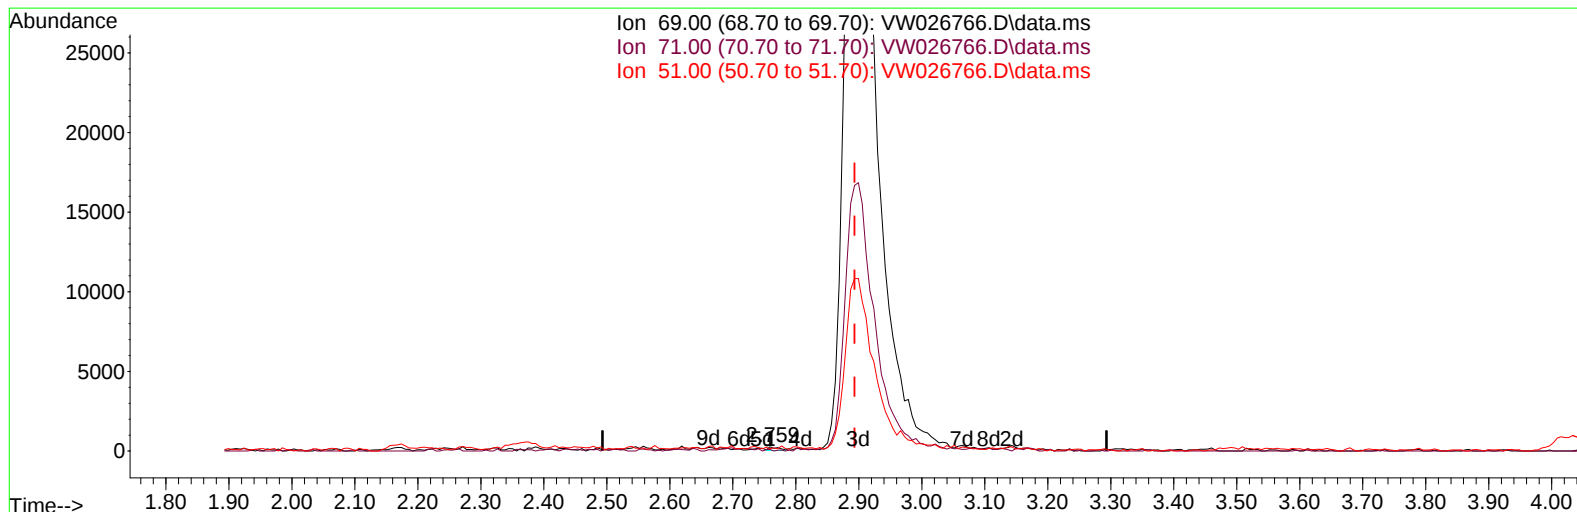

TIC: VW026766.D\data.ms

(7) Chloroethane-d5 (S)

2.759min (-0.134) 0.02 ug/L

response	251	
Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.30	27.49
51.00	28.30	20.32
0.00	0.00	0.00