




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081823\
 Data File : VW026778.D
 Acq On : 18 Aug 2023 18:34
 Operator : SY/MD
 Sample : 04037-02
 Misc : 6.06g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EYZJ7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/22/2023
 Supervised By :Mahesh Dadoda 08/22/2023

Quant Time: Aug 26 02:27:51 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 26 01:43:45 2023
 Response via : Initial Calibration

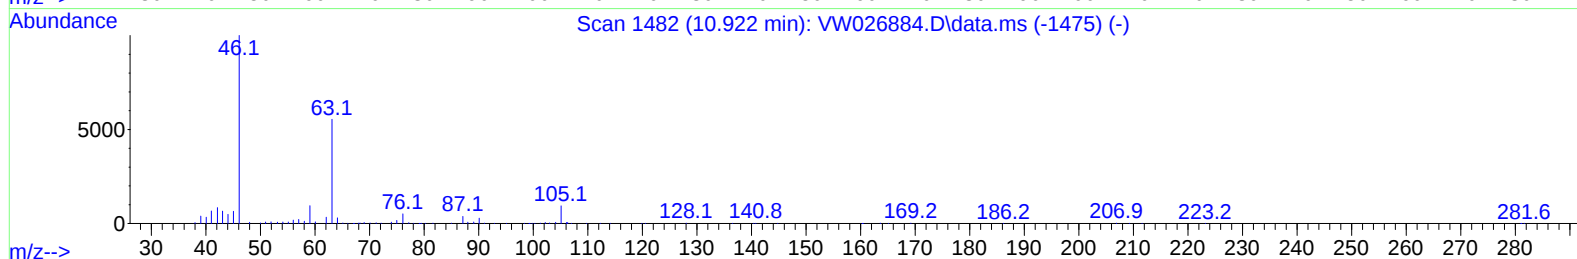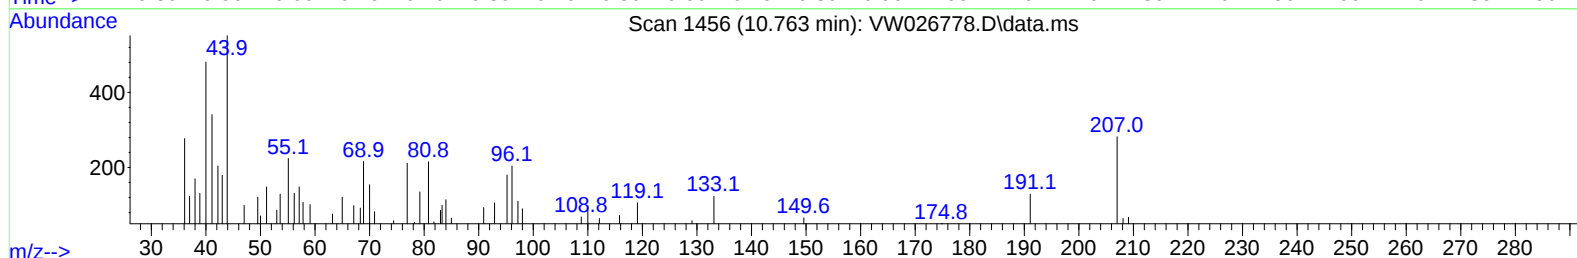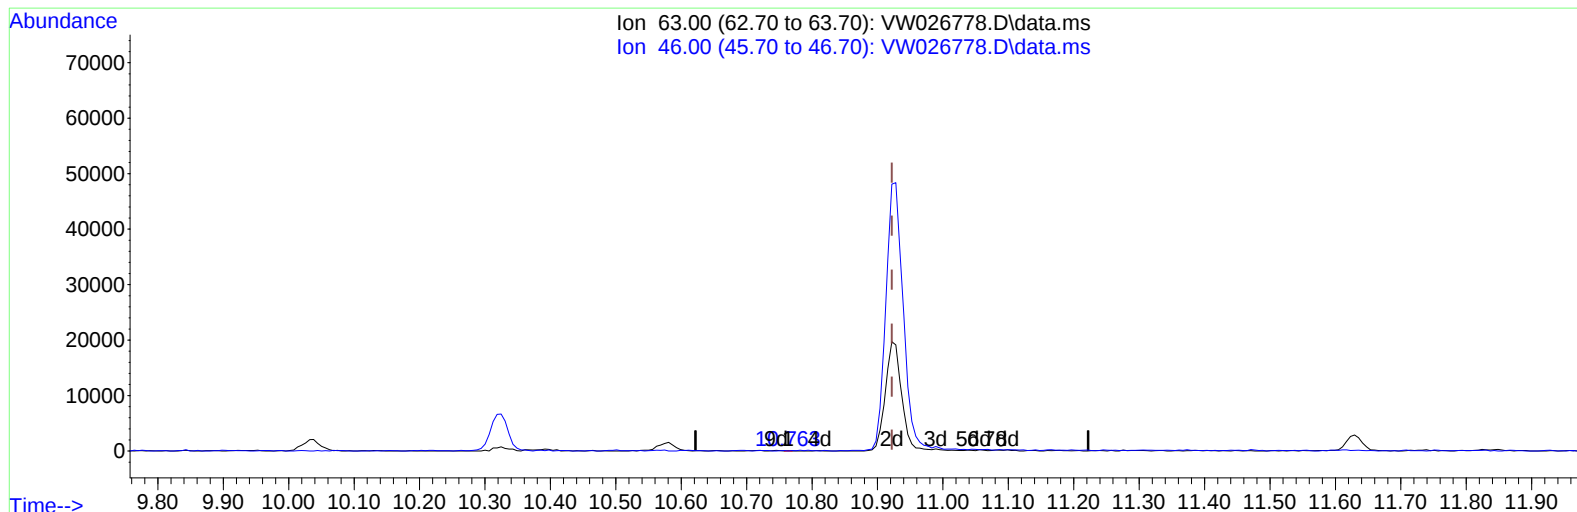

TIC: VW026778.D\data.ms

(47) 2-Hexanone-d5 (S)

10.763min (-0.159) 0.02 ug/L

response	28	
Ion	Exp%	Act%
63.00	100.00	100.00
46.00	184.70	221.43
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081823\
 Data File : VW026778.D
 Acq On : 18 Aug 2023 18:34
 Operator : SY/MD
 Sample : 04037-02
 Misc : 6.06g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EYZJ7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/22/2023
 Supervised By :Mahesh Dadoda 08/22/2023

Quant Time: Aug 18 23:47:03 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 18 23:42:21 2023
 Response via : Initial Calibration

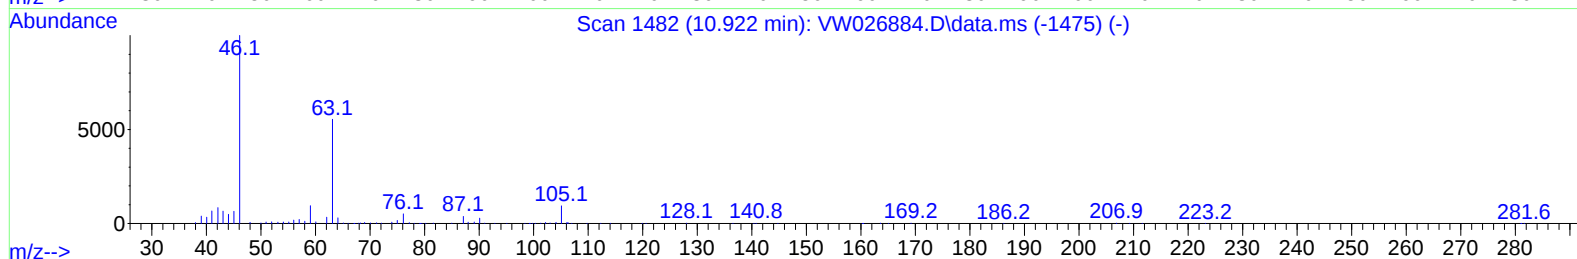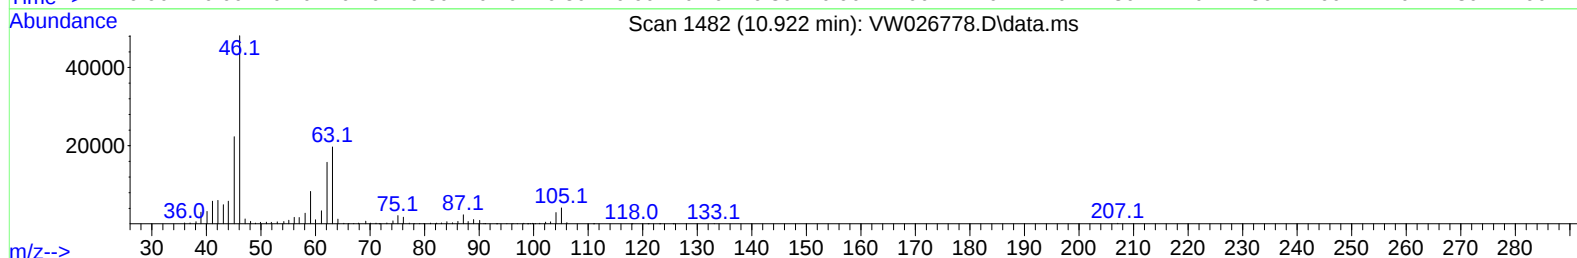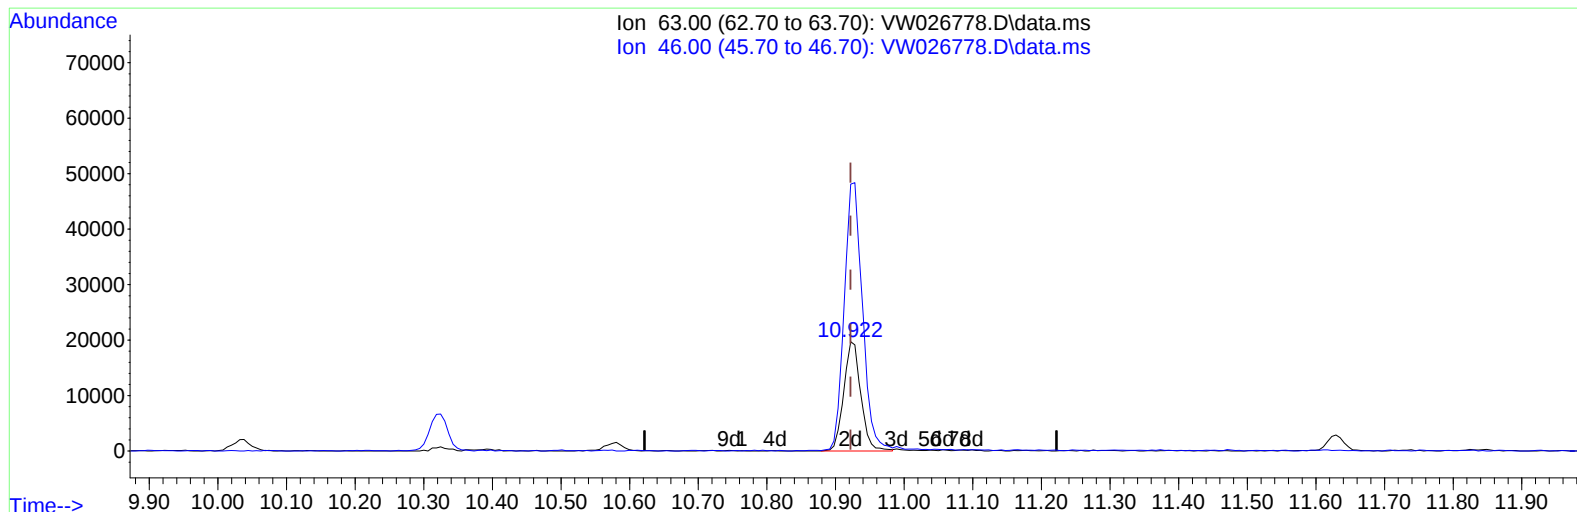

TIC: VW026778.D\data.ms

(47) 2-Hexanone-d5 (S)

10.922min (0.000) 23.11 ug/L m

response 34014

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	184.70	0.18#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081823\
 Data File : VW026778.D
 Acq On : 18 Aug 2023 18:34
 Operator : SY/MD
 Sample : 04037-02
 Misc : 6.06g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZYJ7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/22/2023
 Supervised By :Mahesh Dadoda 08/22/2023

Quant Time: Aug 18 23:47:03 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 18 23:42:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	722260	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	652419	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	300271	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	178996	15.076	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	60.320%		
7) Chloroethane-d5	2.899	69	151631	17.174	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	68.680%		
11) 1,1-Dichloroethene-d2	4.027	65	112056	19.189	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	76.760%		
21) 2-Butanone-d5	7.087	46	98402	28.835	ug/L	0.01
Spiked Amount 50.000	Range 20 - 135		Recovery =	57.680%		
24) Chloroform-d	7.666	84	36122	1.490	ug/L	0.02
Spiked Amount 25.000	Range 40 - 150		Recovery =	5.960%#		
26) 1,2-Dichloroethane-d4	8.307	65	340604	25.461	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	101.840%		
32) Benzene-d6	8.276	84	1172378	26.074	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	104.280%		
36) 1,2-Dichloropropane-d6	9.276	67	394896	28.195	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	112.760%		
41) Toluene-d8	10.325	98	956531	24.782	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	99.120%		
43) trans-1,3-Dichloroprop...	10.574	79	145352	25.135	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	100.560%		
47) 2-Hexanone-d5	10.922	63	34014m	23.112	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	46.220%		
56) 1,1,2,2-Tetrachloroeth...	0.000	84	0d	0.000	ug/L	
Spiked Amount 25.000	Range 45 - 120		Recovery =	0.000%#		
66) 1,2-Dichlorobenzene-d4	13.848	152	263891	24.554	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	98.200%		
Target Compounds						
13) Acetone	4.137	43	14017	4.131	ug/L	91
14) Carbon disulfide	4.393	76	94854	2.470	ug/L	99
16) Methylene chloride	4.929	84	36289	2.597	ug/L	92
25) Chloroform	7.679	83	547529	23.115	ug/L	99
34) Trichloroethene	9.093	95	158499	13.099	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081823\
Data File : VW026778.D
Acq On : 18 Aug 2023 18:34
Operator : SY/MD
Sample : 04037-02
Misc : 6.06g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EZYJ7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/22/2023
Supervised By :Mahesh Dadoda 08/22/2023

Quant Time: Aug 18 23:47:03 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 18 23:42:21 2023
Response via : Initial Calibration

