

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081922\
 Data File : VW024285.D
 Acq On : 19 Aug 2022 12:15
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK537

Quant Time: Aug 20 00:57:03 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 20 00:56:10 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	254473	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	244416	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	120265	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.337	65	108702	20.436	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.760%
7) Chloroethane-d5	2.873	69	79097	23.871	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	95.480%
11) 1,1-Dichloroethene-d2	4.007	63	96760	15.962	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	63.840%
21) 2-Butanone-d5	7.074	46	48122	48.628	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.260%
24) Chloroform-d	7.647	84	174525	22.666	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	90.680%
26) 1,2-Dichloroethane-d4	8.452	65	139	0.033	ug/L	0.15
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.120%#
32) Benzene-d6	8.269	84	323046	22.411	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	89.640%
36) 1,2-Dichloropropane-d6	9.275	67	98898	23.237	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	92.960%
41) Toluene-d8	10.323	98	284418	21.110	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	84.440%
43) trans-1,3-Dichloroprop...	10.573	79	40615	21.787	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	87.160%
47) 2-Hexanone-d5	10.921	63	38132	48.507	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.020%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	100028	24.224	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	96.880%
66) 1,2-Dichlorobenzene-d4	13.853	152	108843	24.732	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.920%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.037	75	3695	0.704	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081922\
Data File : VW024285.D
Acq On : 19 Aug 2022 12:15
Operator : SY/VA
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK537

Quant Time: Aug 20 00:57:03 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Aug 20 00:56:10 2022
Response via : Initial Calibration

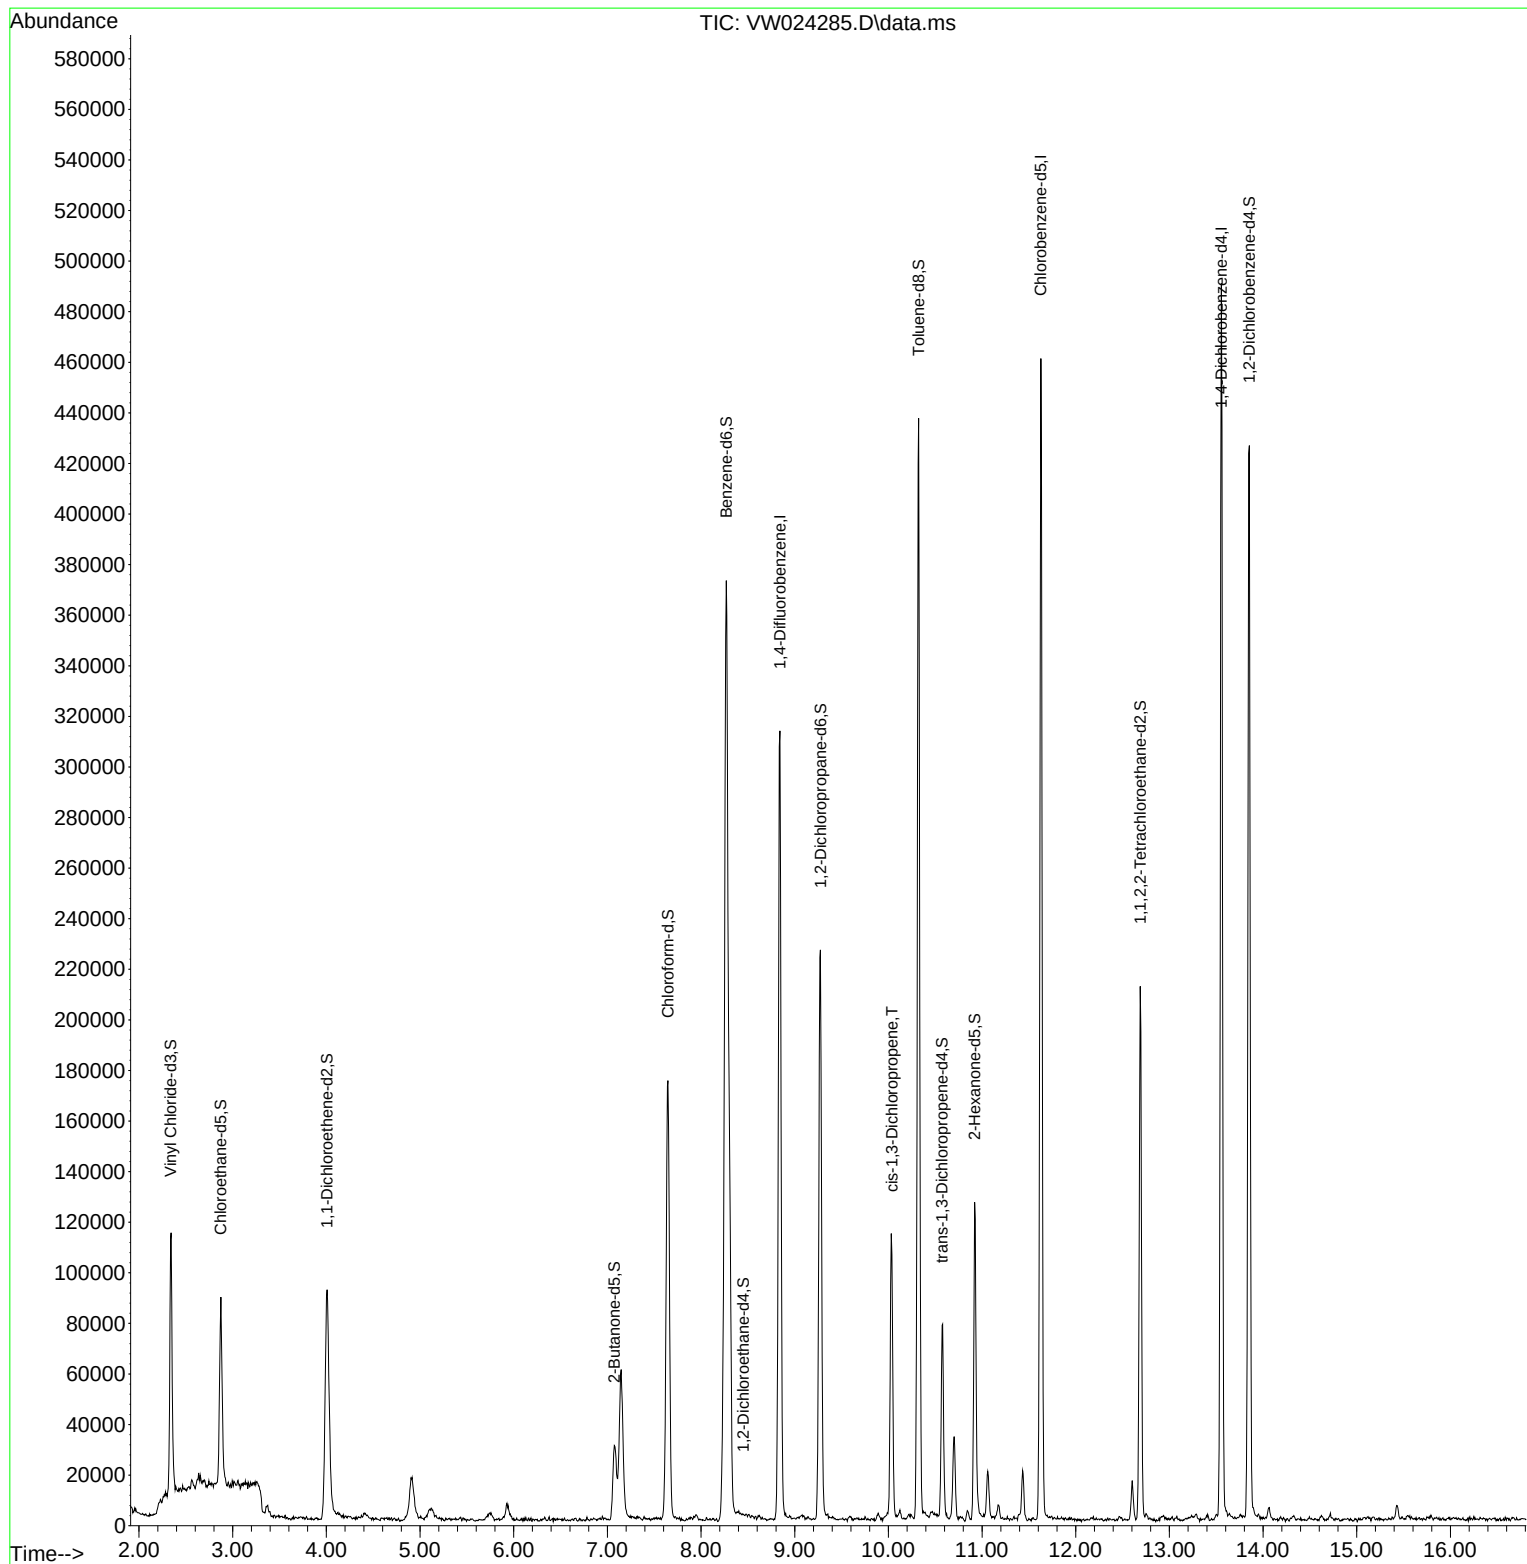

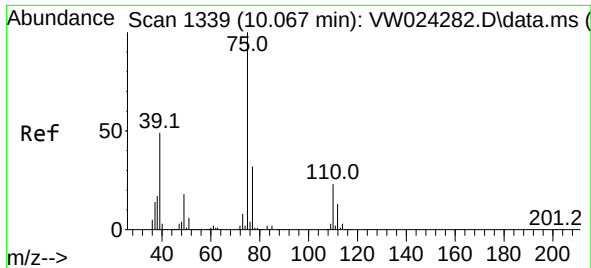

#39
 cis-1,3-Dichloropropene
 Concen: 0.704 ug/L
 RT: 10.037 min Scan# 11
 Delta R.T. -0.030 min
 Lab File: VW024285.D
 Acq: 19 Aug 2022 12:15

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK537

Tgt Ion: 75 Resp: 3695
 Ion Ratio Lower Upper
 75 100
 77 38.5 23.4 43.6

