




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081922\
 Data File : VW024283.D
 Acq On : 19 Aug 2022 11:15
 Operator : SY/VA
 Sample : VW0819SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK582

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/22/2022
 Supervised By :Mahesh Dadoda 08/22/2022

Quant Time: Aug 20 00:56:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 20 00:56:10 2022
 Response via : Initial Calibration

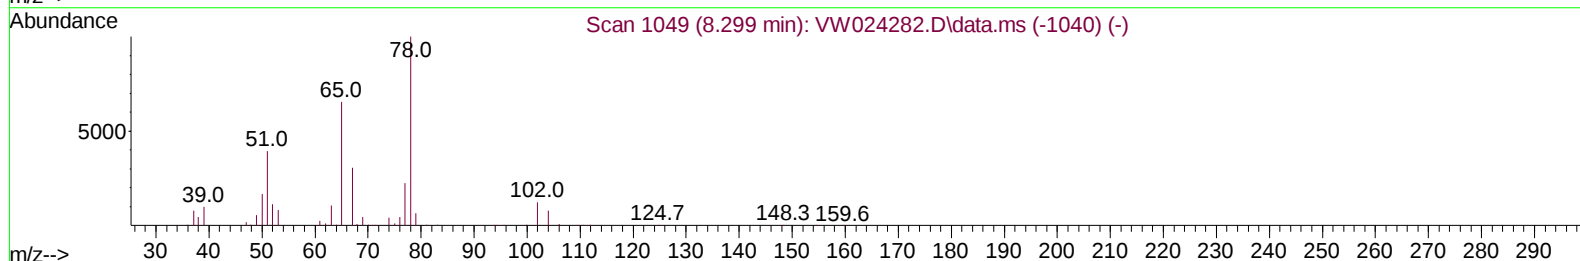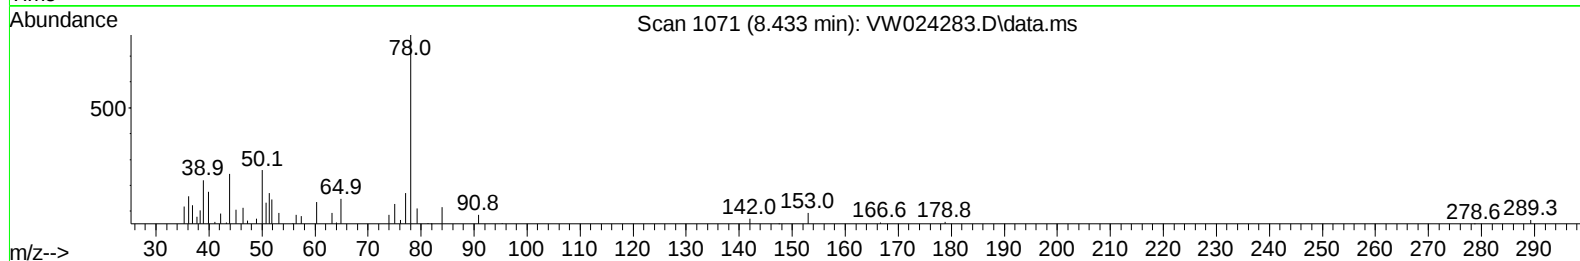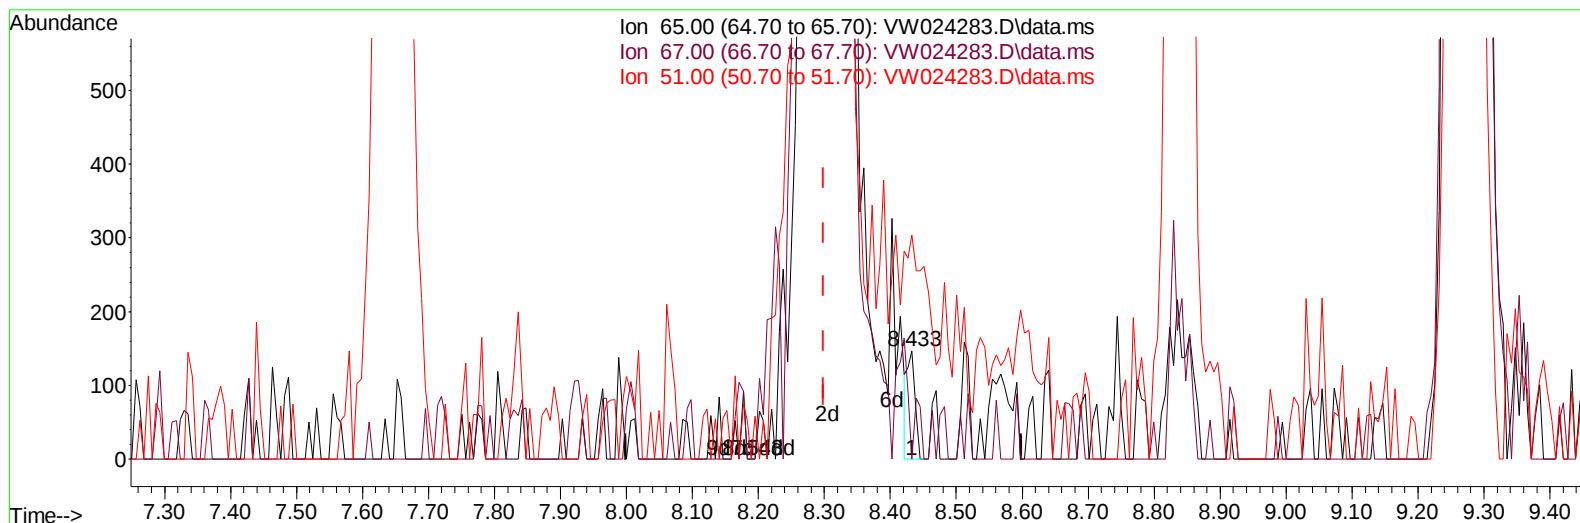

TIC: VW024283.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.433min (+ 0.134) 0.03 ug/L

response 121

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.00	46.28
51.00	95.20	84.30
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081922\
 Data File : VW024283.D
 Acq On : 19 Aug 2022 11:15
 Operator : SY/VA
 Sample : VW0819SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK582

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/22/2022
 Supervised By :Mahesh Dadoda 08/22/2022

Quant Time: Aug 20 00:56:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 20 00:56:10 2022
 Response via : Initial Calibration

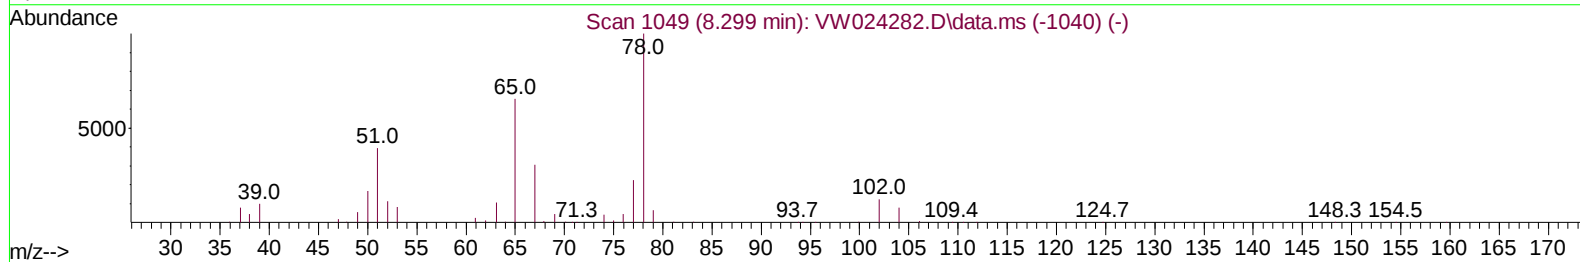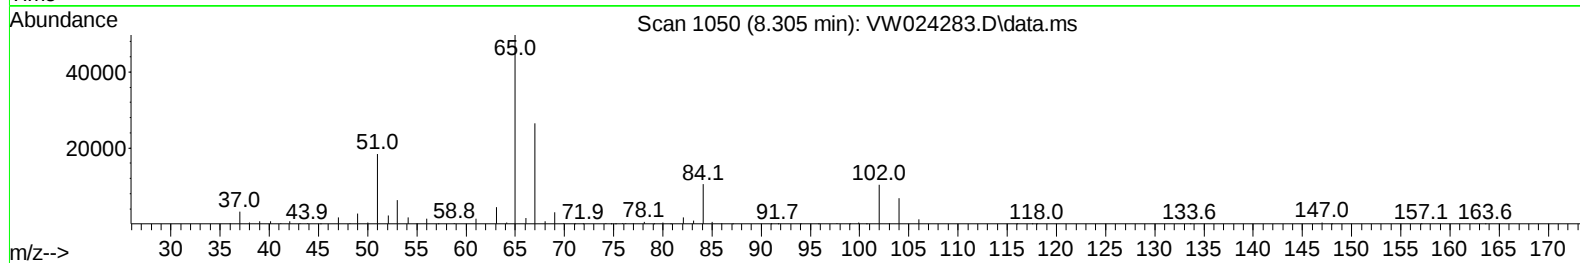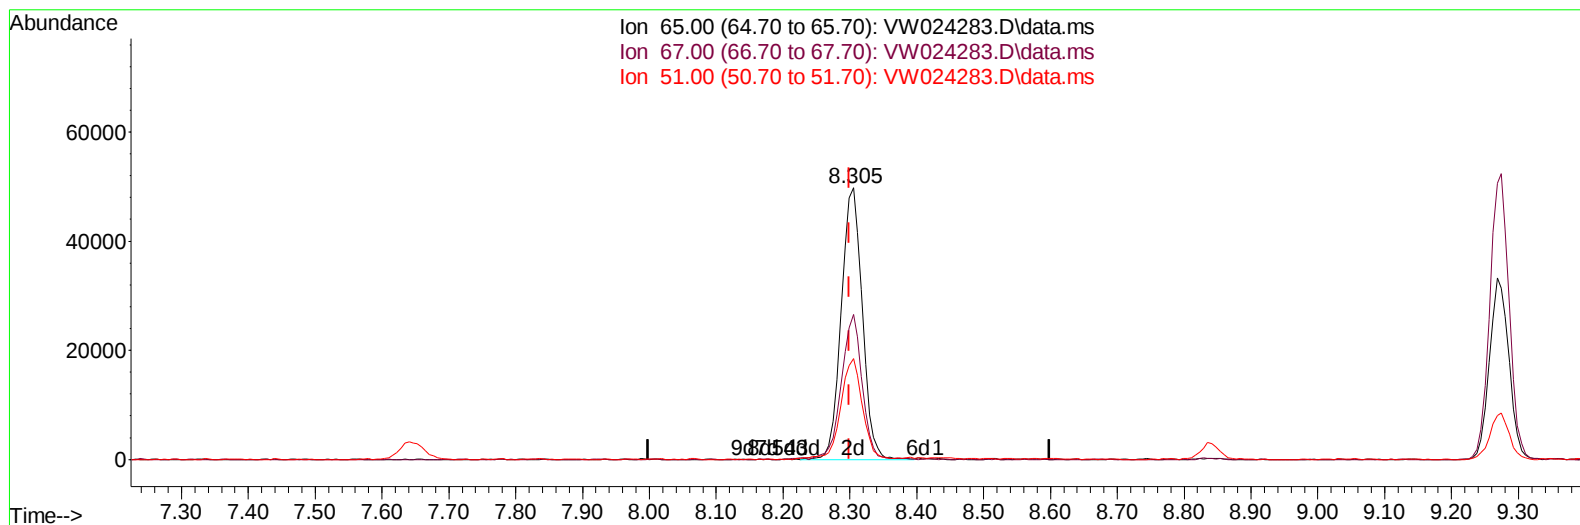

TIC: VW024283.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (+ 0.006) 25.65 ug/L m

response 108506

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.00	0.05#
51.00	95.20	0.09#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081922\
 Data File : VW024283.D
 Acq On : 19 Aug 2022 11:15
 Operator : SY/VA
 Sample : VW0819SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK582

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/22/2022
 Supervised By :Mahesh Dadoda 08/22/2022

Quant Time: Aug 20 00:56:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 20 00:56:10 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	251829	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	246891	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	120251	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	106846	20.298	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	81.200%	
7) Chloroethane-d5	2.873	69	75566	23.045	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	92.160%	
11) 1,1-Dichloroethene-d2	4.007	63	93055	15.512	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	62.040%	
21) 2-Butanone-d5	7.080	46	56708	57.906	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	115.820%	
24) Chloroform-d	7.641	84	188071	24.682	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	98.720%	
26) 1,2-Dichloroethane-d4	8.305	65	108506m	25.649	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	102.600%	
32) Benzene-d6	8.275	84	343415	23.585	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	94.360%	
36) 1,2-Dichloropropane-d6	9.274	67	105141	24.457	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	97.840%	
41) Toluene-d8	10.323	98	302847	22.252	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	89.000%	
43) trans-1,3-Dichloroprop...	10.573	79	43827	23.275	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	93.080%	
47) 2-Hexanone-d5	10.920	63	43251	54.467	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	108.940%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	107646	25.808	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	103.240%	
66) 1,2-Dichlorobenzene-d4	13.853	152	126565	28.762	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	115.040%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081922\
Data File : VW024283.D
Acq On : 19 Aug 2022 11:15
Operator : SY/VA
Sample : VW0819SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK582

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/22/2022
Supervised By :Mahesh Dadoda 08/22/2022

Quant Time: Aug 20 00:56:41 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Aug 20 00:56:10 2022
Response via : Initial Calibration

