




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081922\
Data File : VW024286.D
Acq On : 19 Aug 2022 12:39
Operator : SY/VA
Sample : N4267-03
Misc : 5.84g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0ZG9

Manual IntegrationsAPPROVED

Quant Time: Aug 20 00:57:15 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Aug 20 00:56:10 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/22/2022
Supervised By :Mahesh Dadoda 08/22/2022

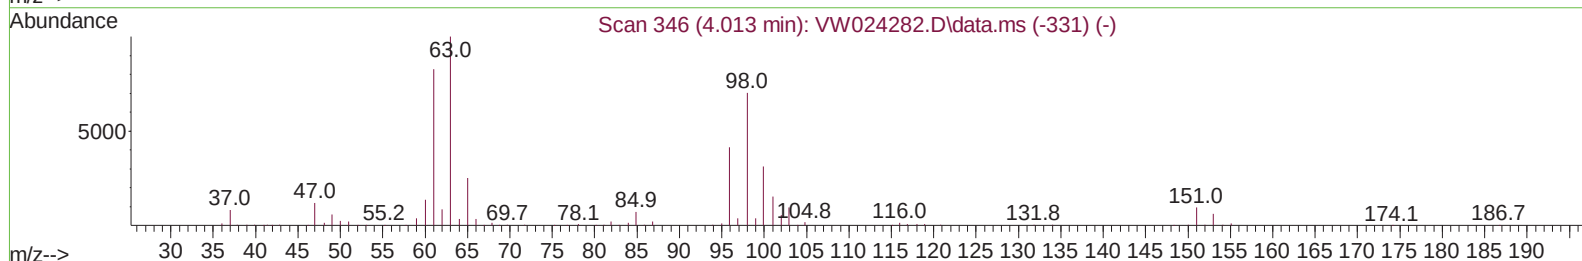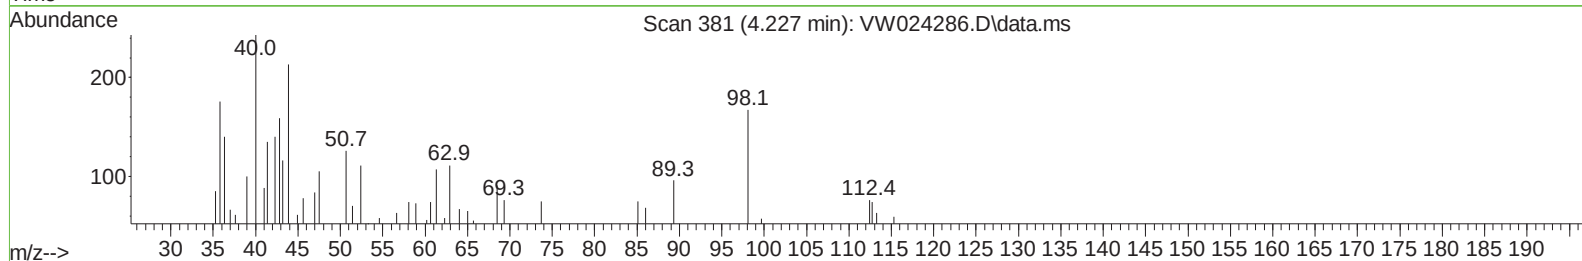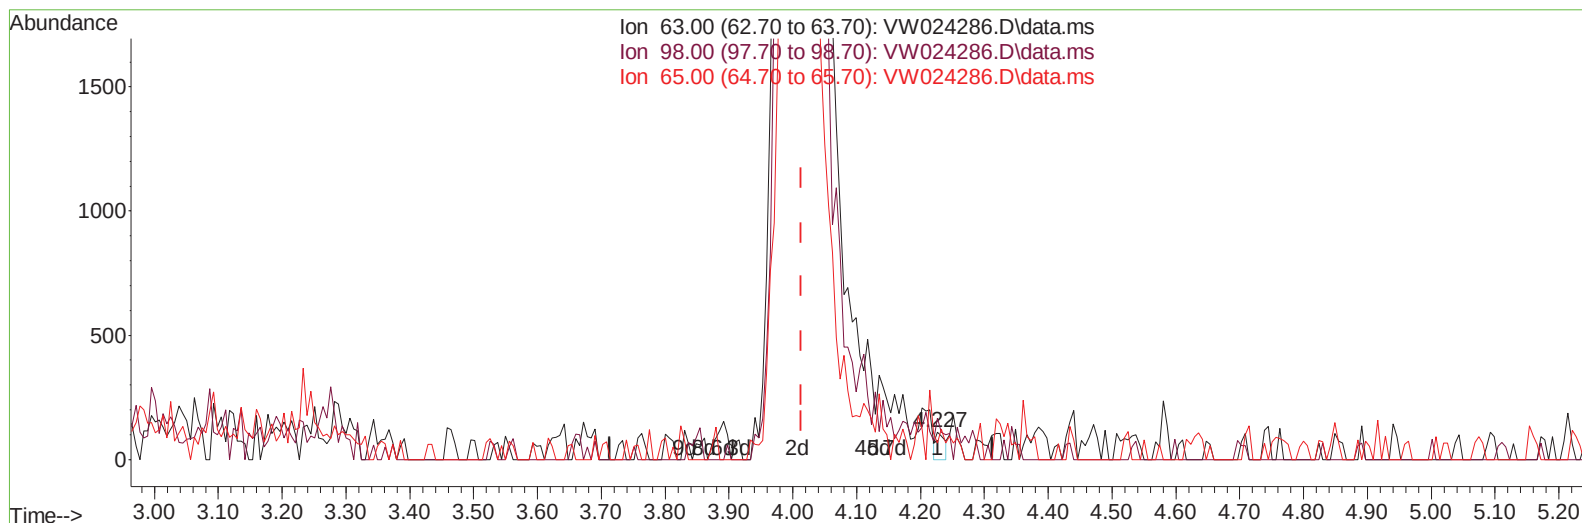

TIC: VW024286.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.227min (+ 0.214) 0.01 ug/L

response 102

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	75.50	53.92
65.00	23.50	21.57
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081922\
 Data File : VW024286.D
 Acq On : 19 Aug 2022 12:39
 Operator : SY/VA
 Sample : N4267-03
 Misc : 5.84g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0ZG9

Manual IntegrationsAPPROVED

Quant Time: Aug 20 00:57:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 20 00:56:10 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/22/2022
 Supervised By :Mahesh Dadoda 08/22/2022

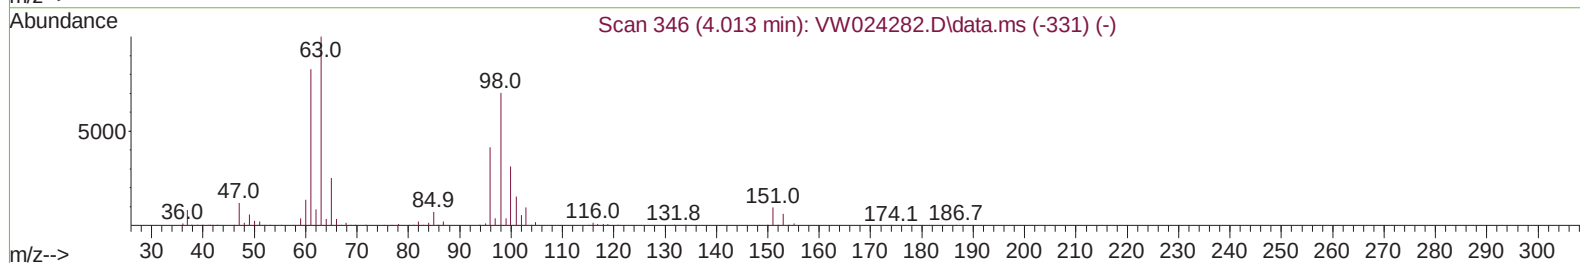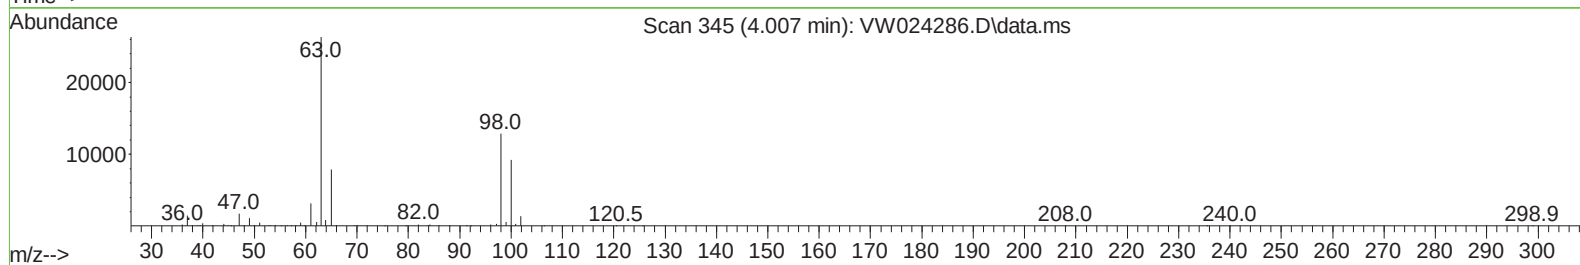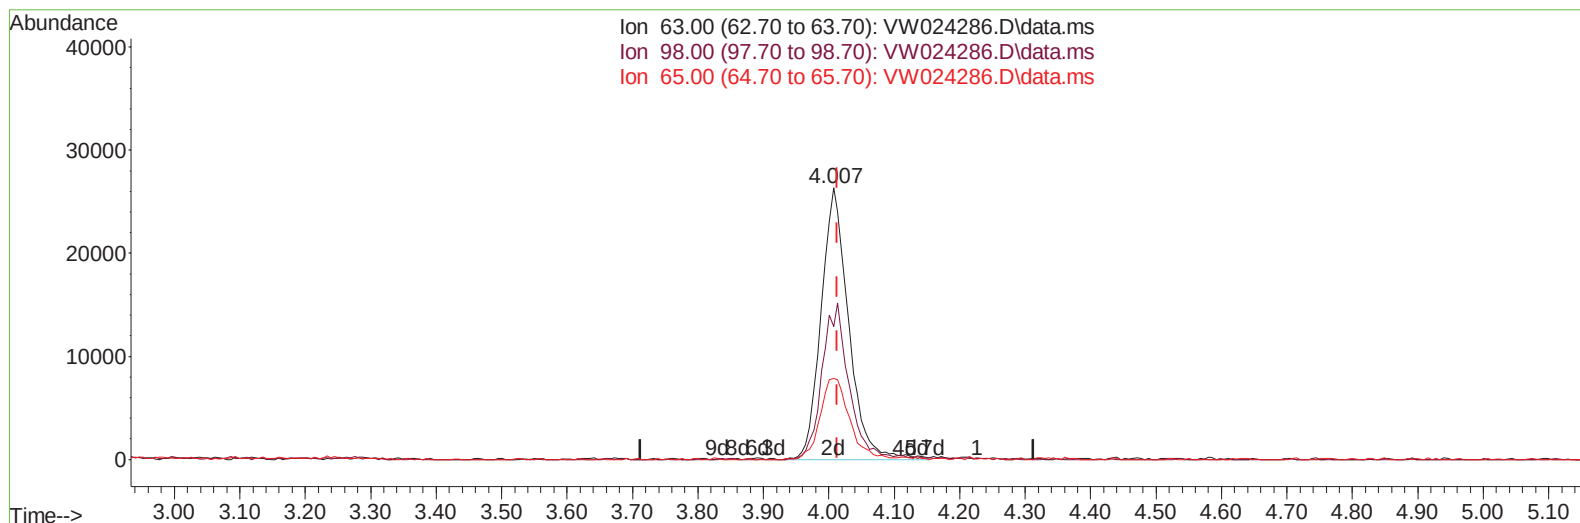

TIC: VW024286.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.007min (-0.006) 9.66 ug/L m

response 77056

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	75.50	0.07#
65.00	23.50	0.03#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081922\
 Data File : VW024286.D
 Acq On : 19 Aug 2022 12:39
 Operator : SY/VA
 Sample : N4267-03
 Misc : 5.84g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0ZG9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/22/2022
 Supervised By :Mahesh Dadoda 08/22/2022

Quant Time: Aug 20 00:57:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 20 00:56:10 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	334818	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	305381	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	127325	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	91271	13.041	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	52.160%	
7) Chloroethane-d5	2.873	69	73130	16.774	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	67.080%	
11) 1,1-Dichloroethene-d2	4.007	63	77056m	9.661	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	38.640%#	
21) 2-Butanone-d5	7.074	46	58772	45.138	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	90.280%	
24) Chloroform-d	7.647	84	178661	17.635	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	70.560%	
26) 1,2-Dichloroethane-d4	8.305	65	99482	17.687	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	70.760%	
32) Benzene-d6	8.269	84	308291	17.118	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	68.480%	
36) 1,2-Dichloropropane-d6	9.268	67	102151	19.210	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	76.840%	
41) Toluene-d8	10.323	98	262371	15.586	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	62.360%	
43) trans-1,3-Dichloroprop...	10.573	79	37422	16.067	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	64.280%	
47) 2-Hexanone-d5	10.921	63	45381	46.204	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	92.400%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	102672	19.901	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	79.600%	
66) 1,2-Dichlorobenzene-d4	13.853	152	86118	18.483	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	73.920%#	
Target Compounds						
					Qvalue	
13) Acetone	4.129	43	10112	10.549	ug/L	84
29) Cyclohexane	7.946	56	4074	0.651	ug/L	99
35) Methylcyclohexane	9.329	83	23042	3.082	ug/L #	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081922\
Data File : VW024286.D
Acq On : 19 Aug 2022 12:39
Operator : SY/VA
Sample : N4267-03
Misc : 5.84g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0ZG9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/22/2022
Supervised By :Mahesh Dadoda 08/22/2022

Quant Time: Aug 20 00:57:15 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Aug 20 00:56:10 2022
Response via : Initial Calibration

