




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081924\
Data File : VW029950.D
Acq On : 19 Aug 2024 15:21
Operator : SY/MD
Sample : P3626-15
Misc : 5.61g/10mL/MSVOA_W/SOIL/A
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCYE1

Manual IntegrationsAPPROVED

Quant Time: Aug 20 02:40:30 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Aug 20 02:38:01 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/20/2024
Supervised By :Semsettin Yesilyurt 08/20/2024

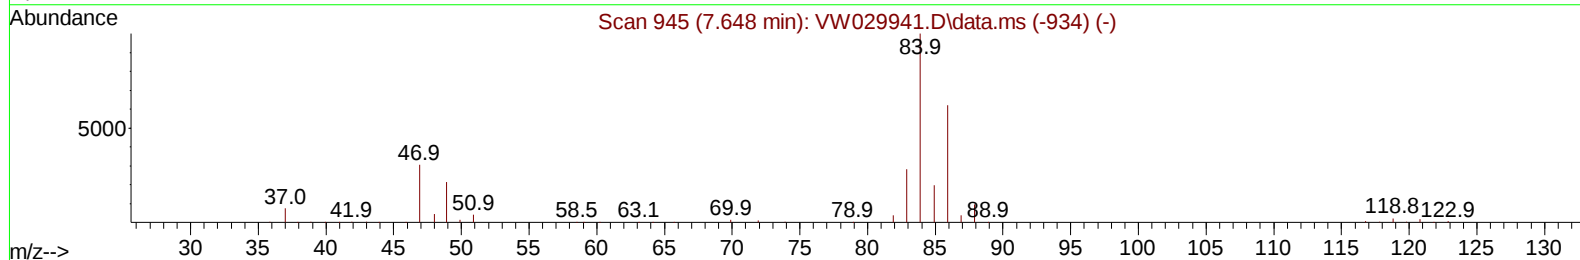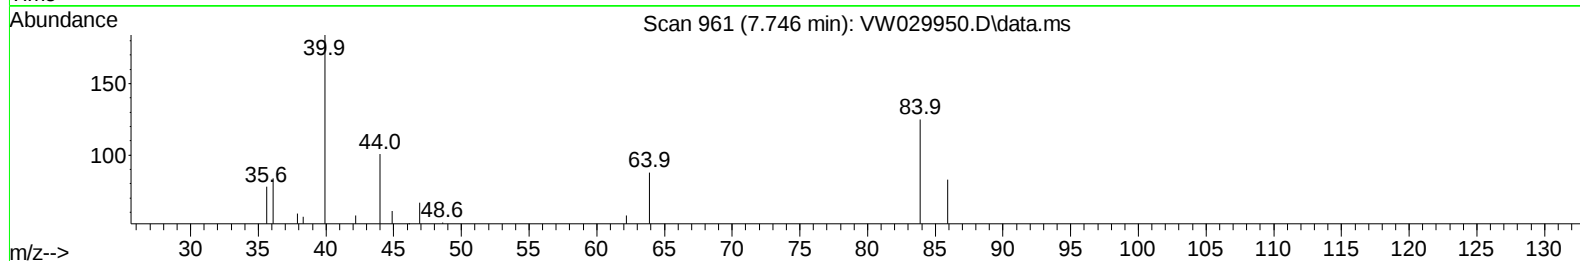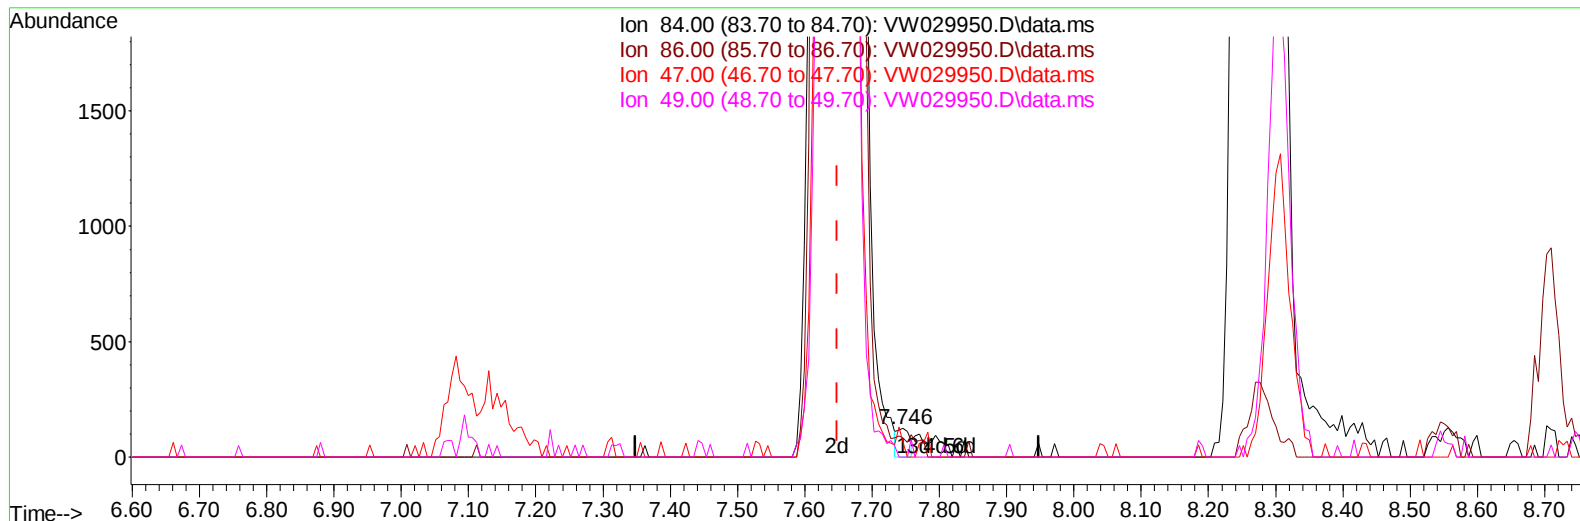

TIC: VW029950.D\data.ms

(24) Chloroform-d (S)

7.746min (+ 0.098) 0.02 ug/L

response 157

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.90	75.80
47.00	57.60	45.86
49.00	31.80	25.48




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081924\
 Data File : VW029950.D
 Acq On : 19 Aug 2024 15:21
 Operator : SY/MD
 Sample : P3626-15
 Misc : 5.61g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCYE1

Manual IntegrationsAPPROVED

Quant Time: Aug 20 02:40:30 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 20 02:38:01 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/20/2024
 Supervised By :Semsettin Yesilyurt 08/20/2024

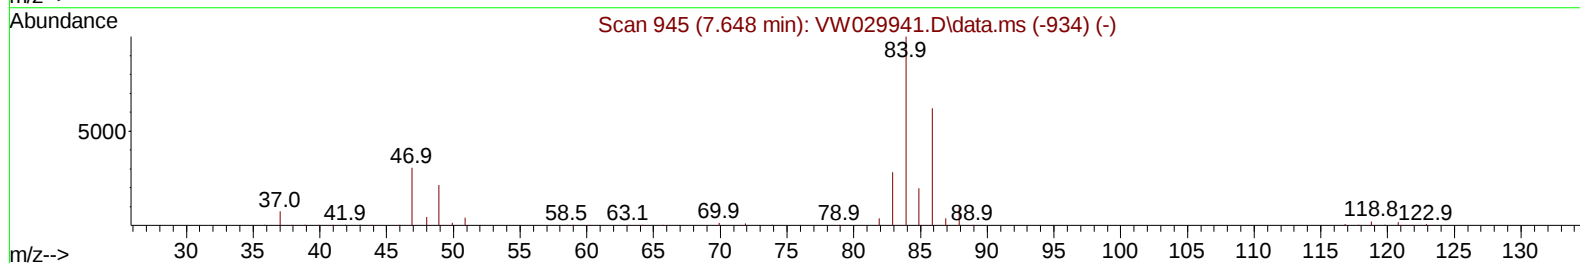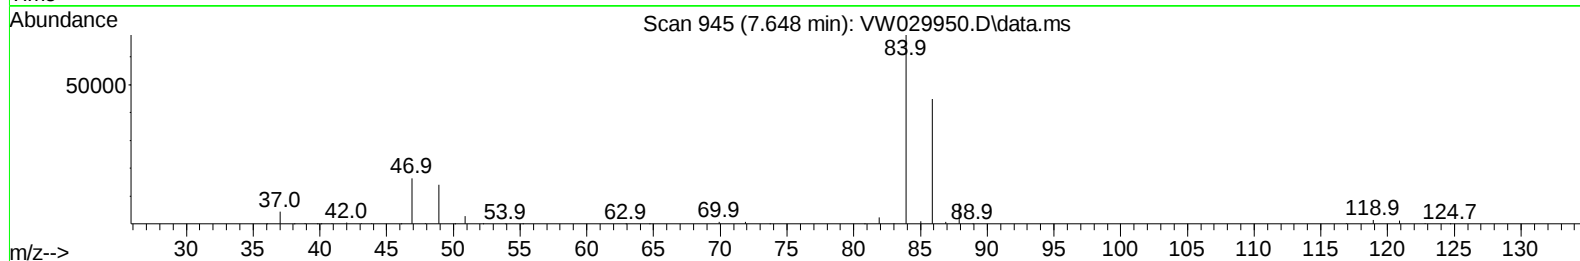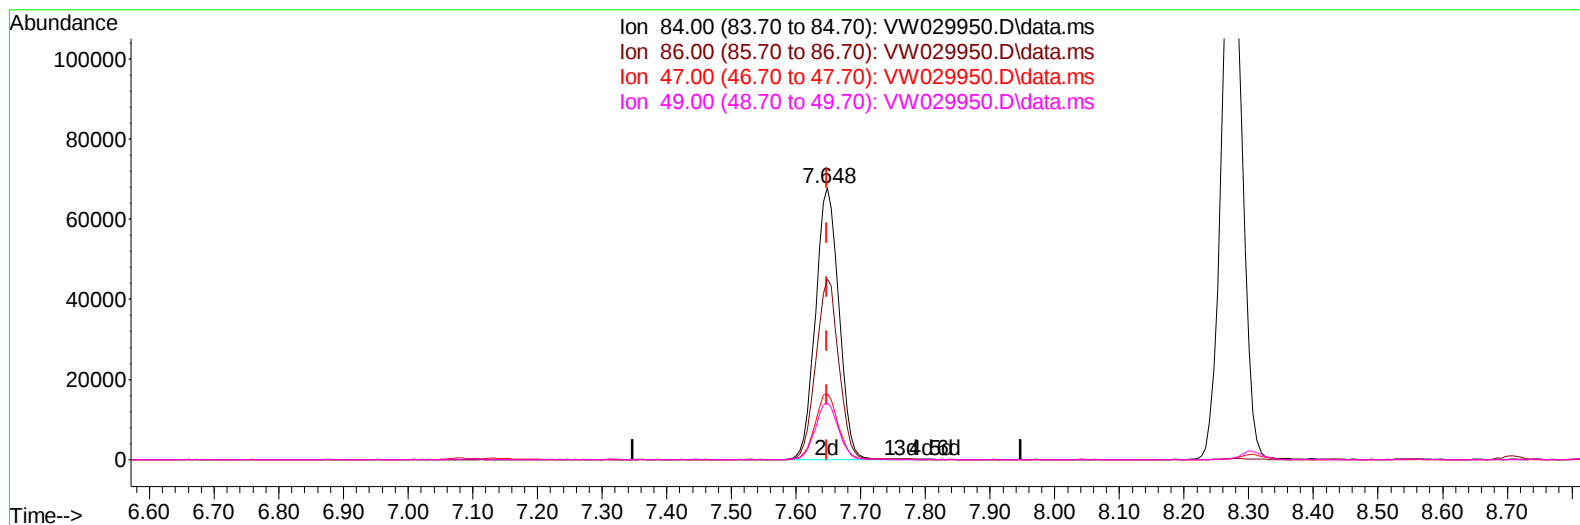

TIC: VW029950.D\data.ms

(24) Chloroform-d (S)

7.648min (+ 0.000) 18.67 ug/L m

response 171126

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.90	0.07#
47.00	57.60	0.04#
49.00	31.80	0.02#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081924\
 Data File : VW029950.D
 Acq On : 19 Aug 2024 15:21
 Operator : SY/MD
 Sample : P3626-15
 Misc : 5.61g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCYE1

Manual IntegrationsAPPROVED

Quant Time: Aug 20 02:40:30 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 20 02:38:01 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/20/2024
 Supervised By :Semsettin Yesilyurt 08/20/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		354120	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		318656	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		124205	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		71298	14.182	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	56.720%	
7) Chloroethane-d5	2.899	69		65111	18.141	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	72.560%	
11) 1,1-Dichloroethene-d2	4.021	65		31348	13.660	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	54.640%	
21) 2-Butanone-d5	7.081	46		40420	29.334	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	58.660%	
24) Chloroform-d	7.648	84		171126m	18.668	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	74.680%	
26) 1,2-Dichloroethane-d4	8.307	65		98487	18.862	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	75.440%	
32) Benzene-d6	8.276	84		314132	18.245	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	72.960%	
36) 1,2-Dichloropropane-d6	9.270	67		102102	18.572	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	74.280%	
41) Toluene-d8	10.319	98		277832	18.148	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	72.600%	
43) trans-1,3-Dichloroprop...	10.575	79		38151	17.150	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	68.600%	
47) 2-Hexanone-d5	10.922	63		31362	34.596	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	69.200%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		83736	20.513	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	82.040%	
66) 1,2-Dichlorobenzene-d4	13.848	152		77202	20.018	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	80.080%	
Target Compounds							
13) Acetone	4.137	43		88846	51.884	ug/L	96
55) Styrene	12.178	104		6600	0.447	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081924\
Data File : VW029950.D
Acq On : 19 Aug 2024 15:21
Operator : SY/MD
Sample : P3626-15
Misc : 5.61g/10mL/MSVOA_W/SOIL/A
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCYE1

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 08/20/2024
Supervised By :Semsettin Yesilyurt 08/20/2024

Quant Time: Aug 20 02:40:30 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Aug 20 02:38:01 2024
Response via : Initial Calibration

