

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082024\
 Data File : VW029971.D
 Acq On : 20 Aug 2024 20:07
 Operator : SY/MD
 Sample : P3675-07
 Misc : 5.63g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Aug 21 00:49:32 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 21 00:44:34 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	331947	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	308687	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	114161	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	67836	14.395	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	57.560%		
7) Chloroethane-d5	2.899	69	63982	19.017	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	76.080%		
11) 1,1-Dichloroethene-d2	4.021	65	31149	14.480	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	57.920%		
21) 2-Butanone-d5	7.087	46	33948	26.283	ug/L	0.01
Spiked Amount 50.000	Range 20 - 135		Recovery =	52.560%		
24) Chloroform-d	7.648	84	170264	19.814	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	79.240%		
26) 1,2-Dichloroethane-d4	8.307	65	94365	19.280	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	77.120%		
32) Benzene-d6	8.276	84	308397	18.490	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	73.960%		
36) 1,2-Dichloropropane-d6	9.276	67	98732	18.539	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	74.160%		
41) Toluene-d8	10.325	98	275476	18.575	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	74.320%		
43) trans-1,3-Dichloroprop...	10.575	79	36439	16.909	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	67.640%		
47) 2-Hexanone-d5	10.922	63	27221	30.998	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	62.000%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	74852	18.929	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	75.720%		
66) 1,2-Dichlorobenzene-d4	13.854	152	71674	20.220	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	80.880%		
Target Compounds					Qvalue	
13) Acetone	4.155	43	23861	14.865	ug/L	91
39) cis-1,3-Dichloropropene	10.032	75	3000	0.355	ug/L #	41


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082024\
Data File : VW029971.D
Acq On : 20 Aug 2024 20:07
Operator : SY/MD
Sample : P3675-07
Misc : 5.63g/10mL/MSVOA_W/SOIL/A
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Aug 21 00:49:32 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Aug 21 00:44:34 2024
Response via : Initial Calibration

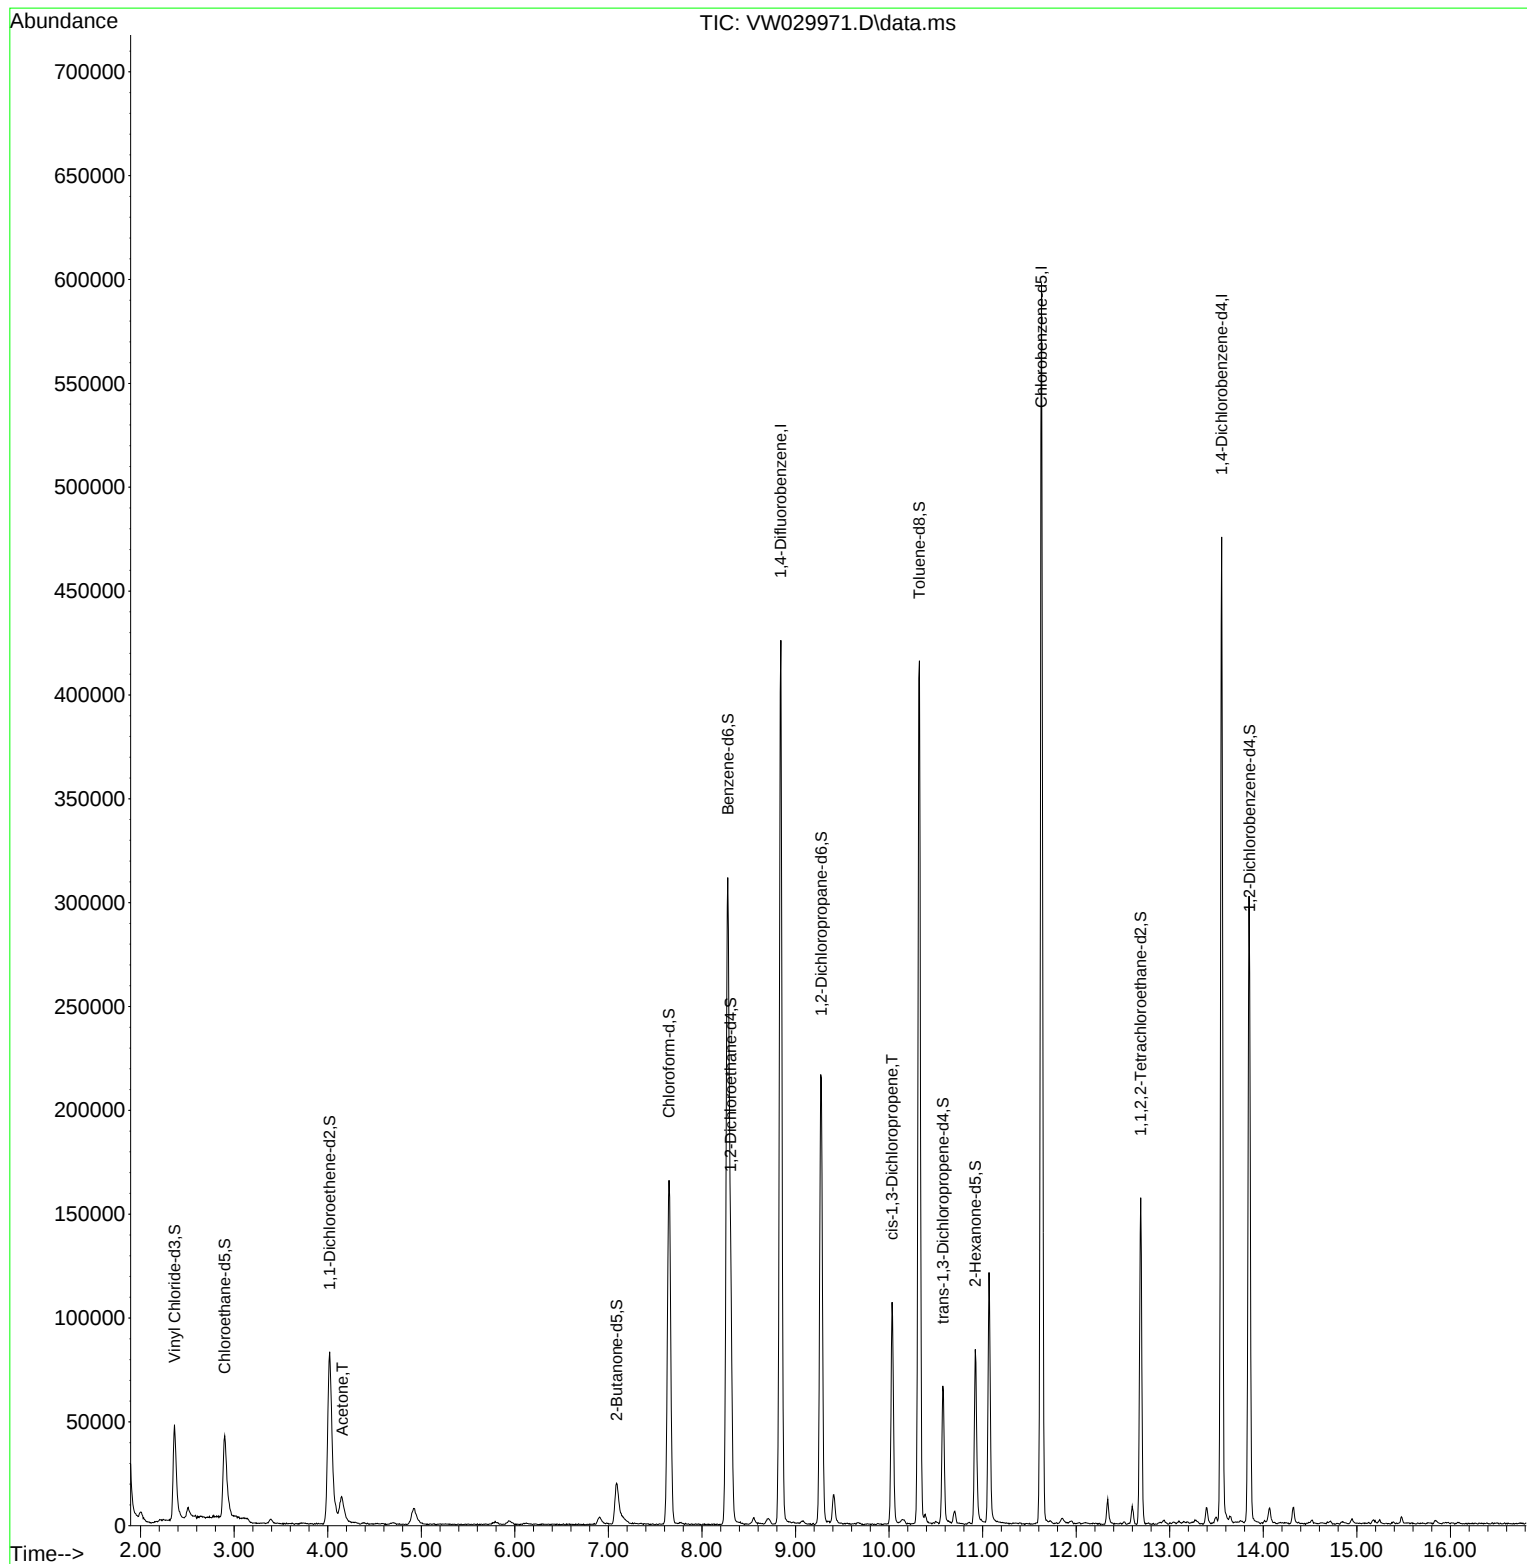



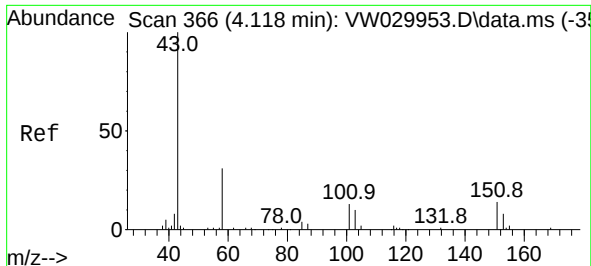


#13
Acetone
Concen: 14.865 ug/L
RT: 4.155 min Scan# 31
Delta R.T. 0.037 min
Lab File: VW029971.D
Acq: 20 Aug 2024 20:07

Instrument :
MSVOA_W
ClientSampleId :

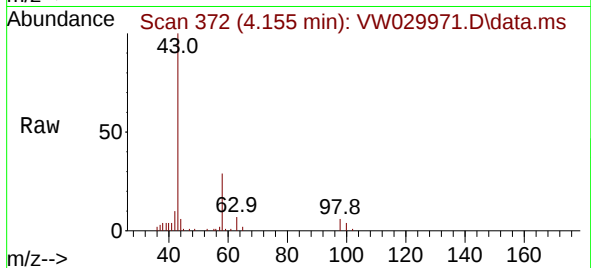

Tgt Ion: 43 Resp: 23861
Ion Ratio Lower Upper
43 100
58 33.4 0.0 57.6

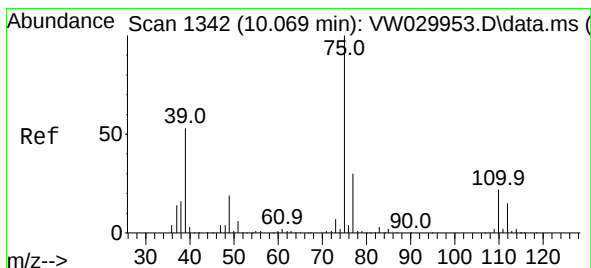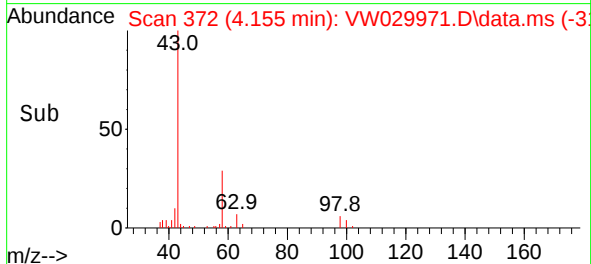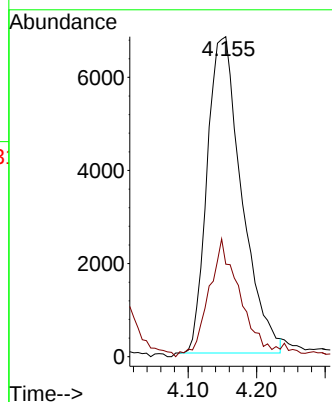

#39
cis-1,3-Dichloropropene
Concen: 0.355 ug/L
RT: 10.032 min Scan# 1336
Delta R.T. -0.037 min
Lab File: VW029971.D
Acq: 20 Aug 2024 20:07

Tgt Ion: 75 Resp: 3000
Ion Ratio Lower Upper
75 100
77 61.6 20.8 38.6#

