

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082024\
 Data File : VW029960.D
 Acq On : 20 Aug 2024 15:44
 Operator : SY/MD
 Sample : P3626-18
 Misc : 4.41g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCXZ7

Quant Time: Aug 21 00:46:59 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 21 00:44:34 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	313555	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	259942	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	89759	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	64008	14.379	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	57.520%
7) Chloroethane-d5	2.899	69	57336	18.041	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	72.160%
11) 1,1-Dichloroethene-d2	4.027	65	28606	14.078	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	56.320%
21) 2-Butanone-d5	7.075	46	37694	30.895	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	61.780%
24) Chloroform-d	7.648	84	148393	18.282	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	73.120%
26) 1,2-Dichloroethane-d4	8.307	65	83479	18.056	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	72.240%
32) Benzene-d6	8.276	84	263036	18.728	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	74.920%
36) 1,2-Dichloropropane-d6	9.270	67	84922	18.936	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	75.760%
41) Toluene-d8	10.325	98	230001	18.417	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	73.680%
43) trans-1,3-Dichloroprop...	10.575	79	32287	17.792	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	71.160%
47) 2-Hexanone-d5	10.922	63	27871	37.690	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	75.380%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	68931	20.700	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	82.800%
66) 1,2-Dichlorobenzene-d4	13.848	152	52457	18.821	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	75.280%
Target Compounds						
					Qvalue	
13) Acetone	4.118	43	41999	27.699	ug/L	96
15) Methyl Acetate	4.685	43	1920	0.760	ug/L	# 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082024\
Data File : VW029960.D
Acq On : 20 Aug 2024 15:44
Operator : SY/MD
Sample : P3626-18
Misc : 4.41g/10mL/MSVOA_W/SOIL/A
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCXZ7

Quant Time: Aug 21 00:46:59 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Aug 21 00:44:34 2024
Response via : Initial Calibration




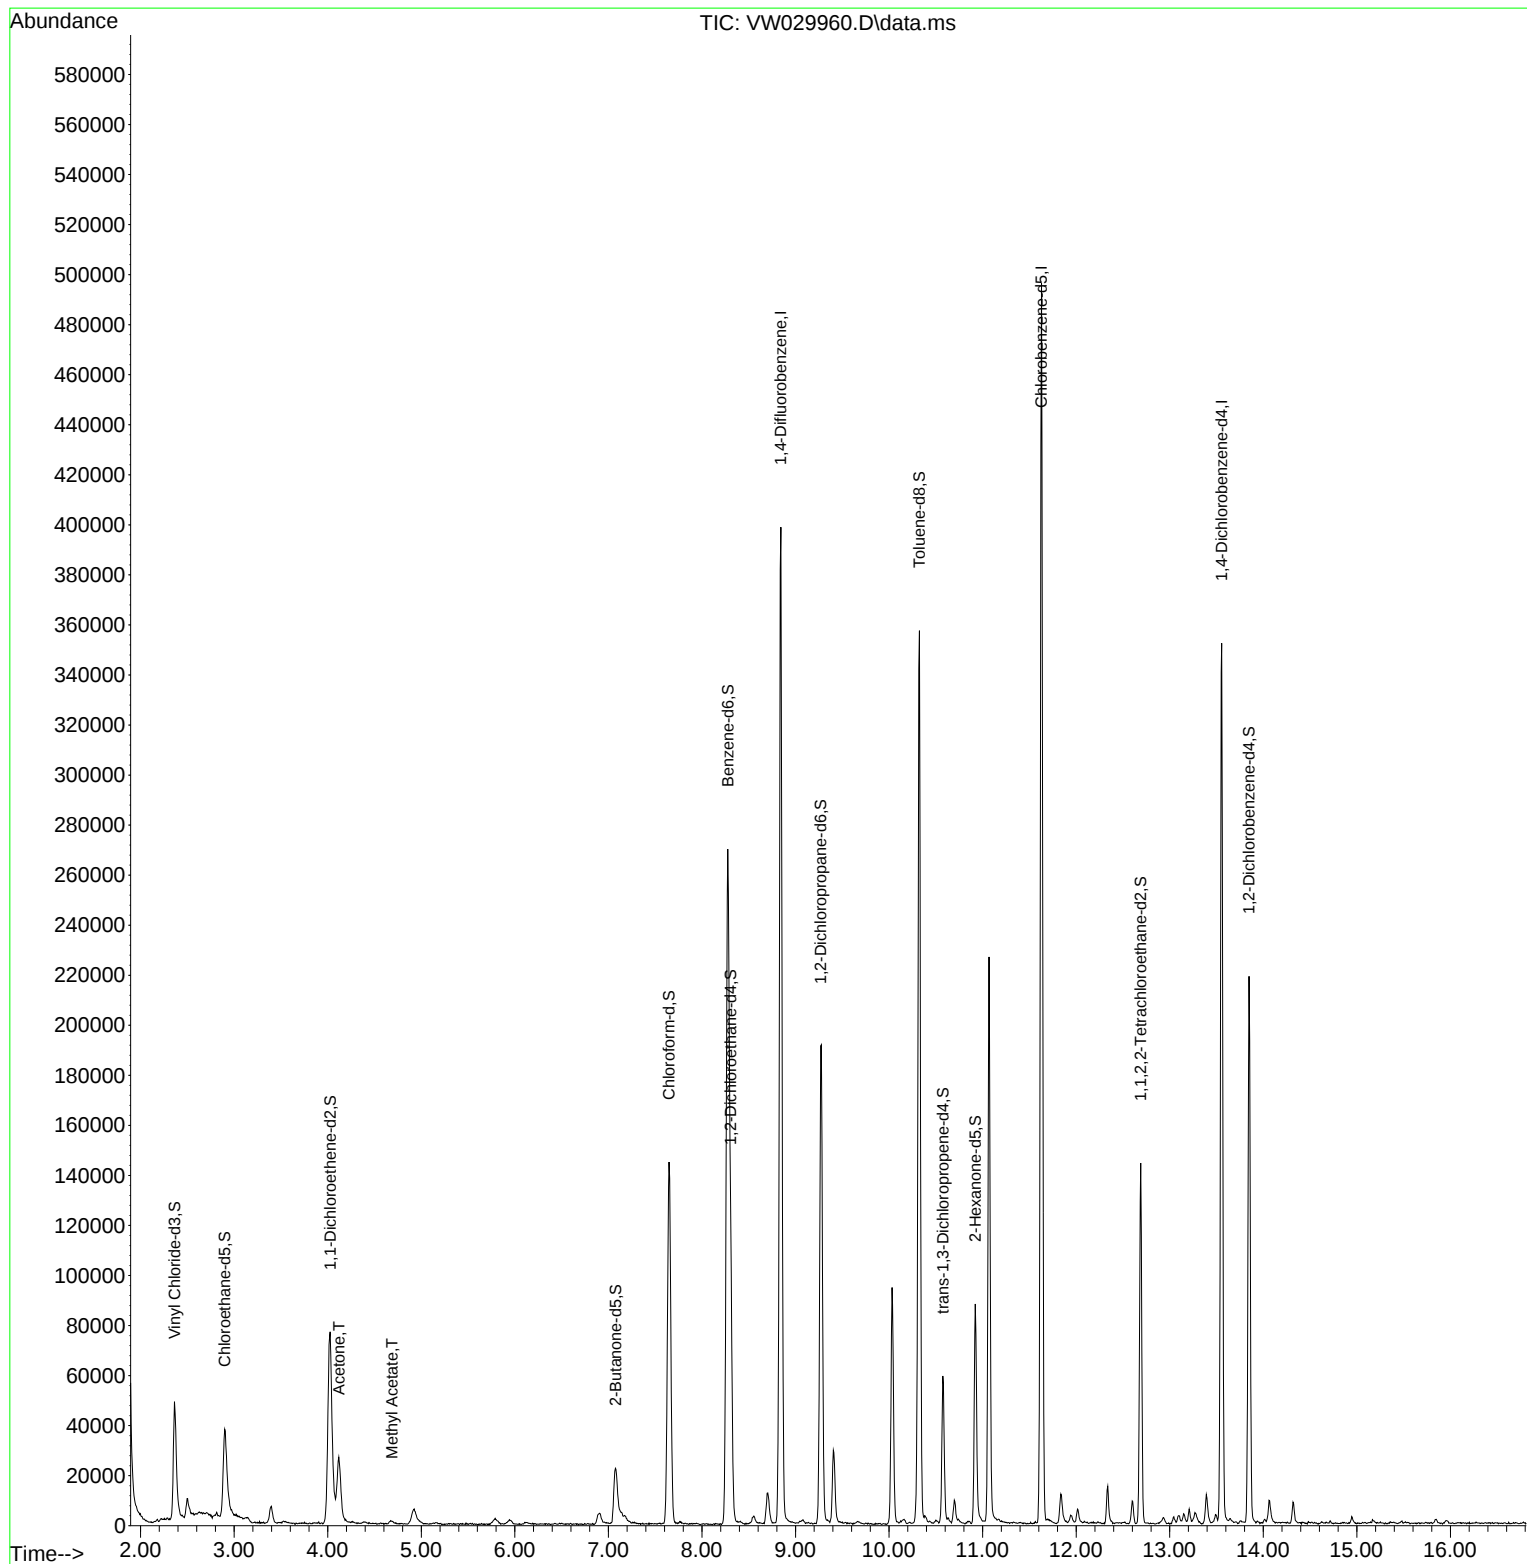


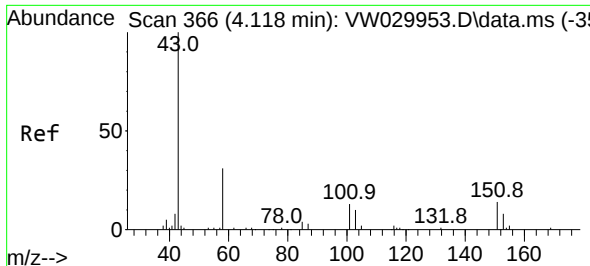

#13
Acetone
Concen: 27.699 ug/L
RT: 4.118 min Scan# 366
Delta R.T. 0.000 min
Lab File: VW029960.D
Acq: 20 Aug 2024 15:44

Instrument :
MSVOA_W
ClientSampleId :
DCXZ7

Tgt Ion: 43 Resp: 41999
Ion Ratio Lower Upper
43 100
58 31.0 0.0 57.6

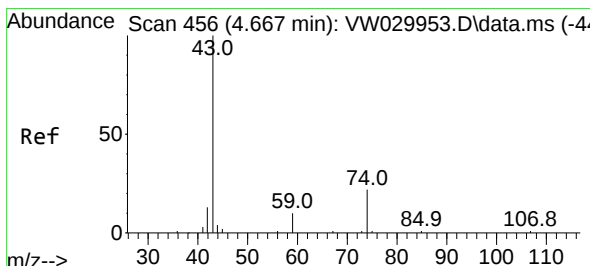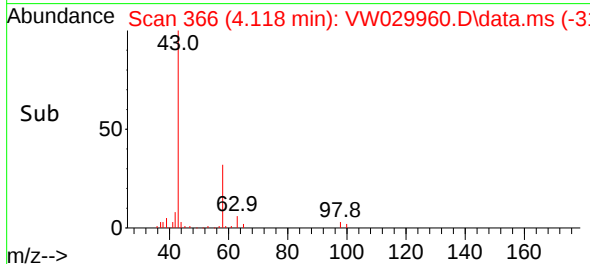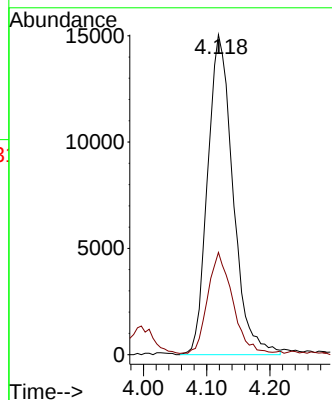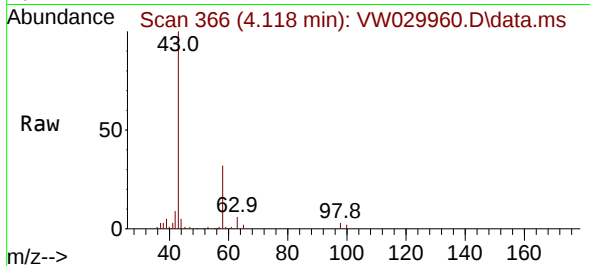

#15
Methyl Acetate
Concen: 0.760 ug/L
RT: 4.685 min Scan# 459
Delta R.T. 0.018 min
Lab File: VW029960.D
Acq: 20 Aug 2024 15:44

Tgt Ion: 43 Resp: 1920
Ion Ratio Lower Upper
43 100
74 15.4 16.5 24.7#

