

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082024\
 Data File : VW029972.D
 Acq On : 20 Aug 2024 20:31
 Operator : SY/MD
 Sample : P3675-08
 Misc : 6.14g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCYE3

Quant Time: Aug 21 00:49:44 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 21 00:44:34 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	276813	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	233813	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	73091	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	61873	15.744	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	62.960%		
7) Chloroethane-d5	2.899	69	55852	19.907	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	79.640%		
11) 1,1-Dichloroethene-d2	4.027	65	26826	14.954	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	59.800%		
21) 2-Butanone-d5	7.087	46	36649	34.025	ug/L	0.01
Spiked Amount 50.000	Range 20 - 135		Recovery =	68.060%		
24) Chloroform-d	7.648	84	147322	20.559	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	82.240%		
26) 1,2-Dichloroethane-d4	8.307	65	86061	21.086	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	84.360%		
32) Benzene-d6	8.276	84	258993	20.501	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	82.000%		
36) 1,2-Dichloropropane-d6	9.270	67	85192	21.119	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	84.480%		
41) Toluene-d8	10.319	98	218152	19.420	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	77.680%		
43) trans-1,3-Dichloroprop...	10.575	79	31405	19.240	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	76.960%		
47) 2-Hexanone-d5	10.922	63	28460	42.787	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	85.580%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	72214	24.110	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	96.440%		
66) 1,2-Dichlorobenzene-d4	13.848	152	50803	22.385	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	89.520%		
Target Compounds					Qvalue	
13) Acetone	4.149	43	20964	15.661	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082024\
Data File : VW029972.D
Acq On : 20 Aug 2024 20:31
Operator : SY/MD
Sample : P3675-08
Misc : 6.14g/10mL/MSVOA_W/SOIL/A
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCYE3

Quant Time: Aug 21 00:49:44 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Aug 21 00:44:34 2024
Response via : Initial Calibration

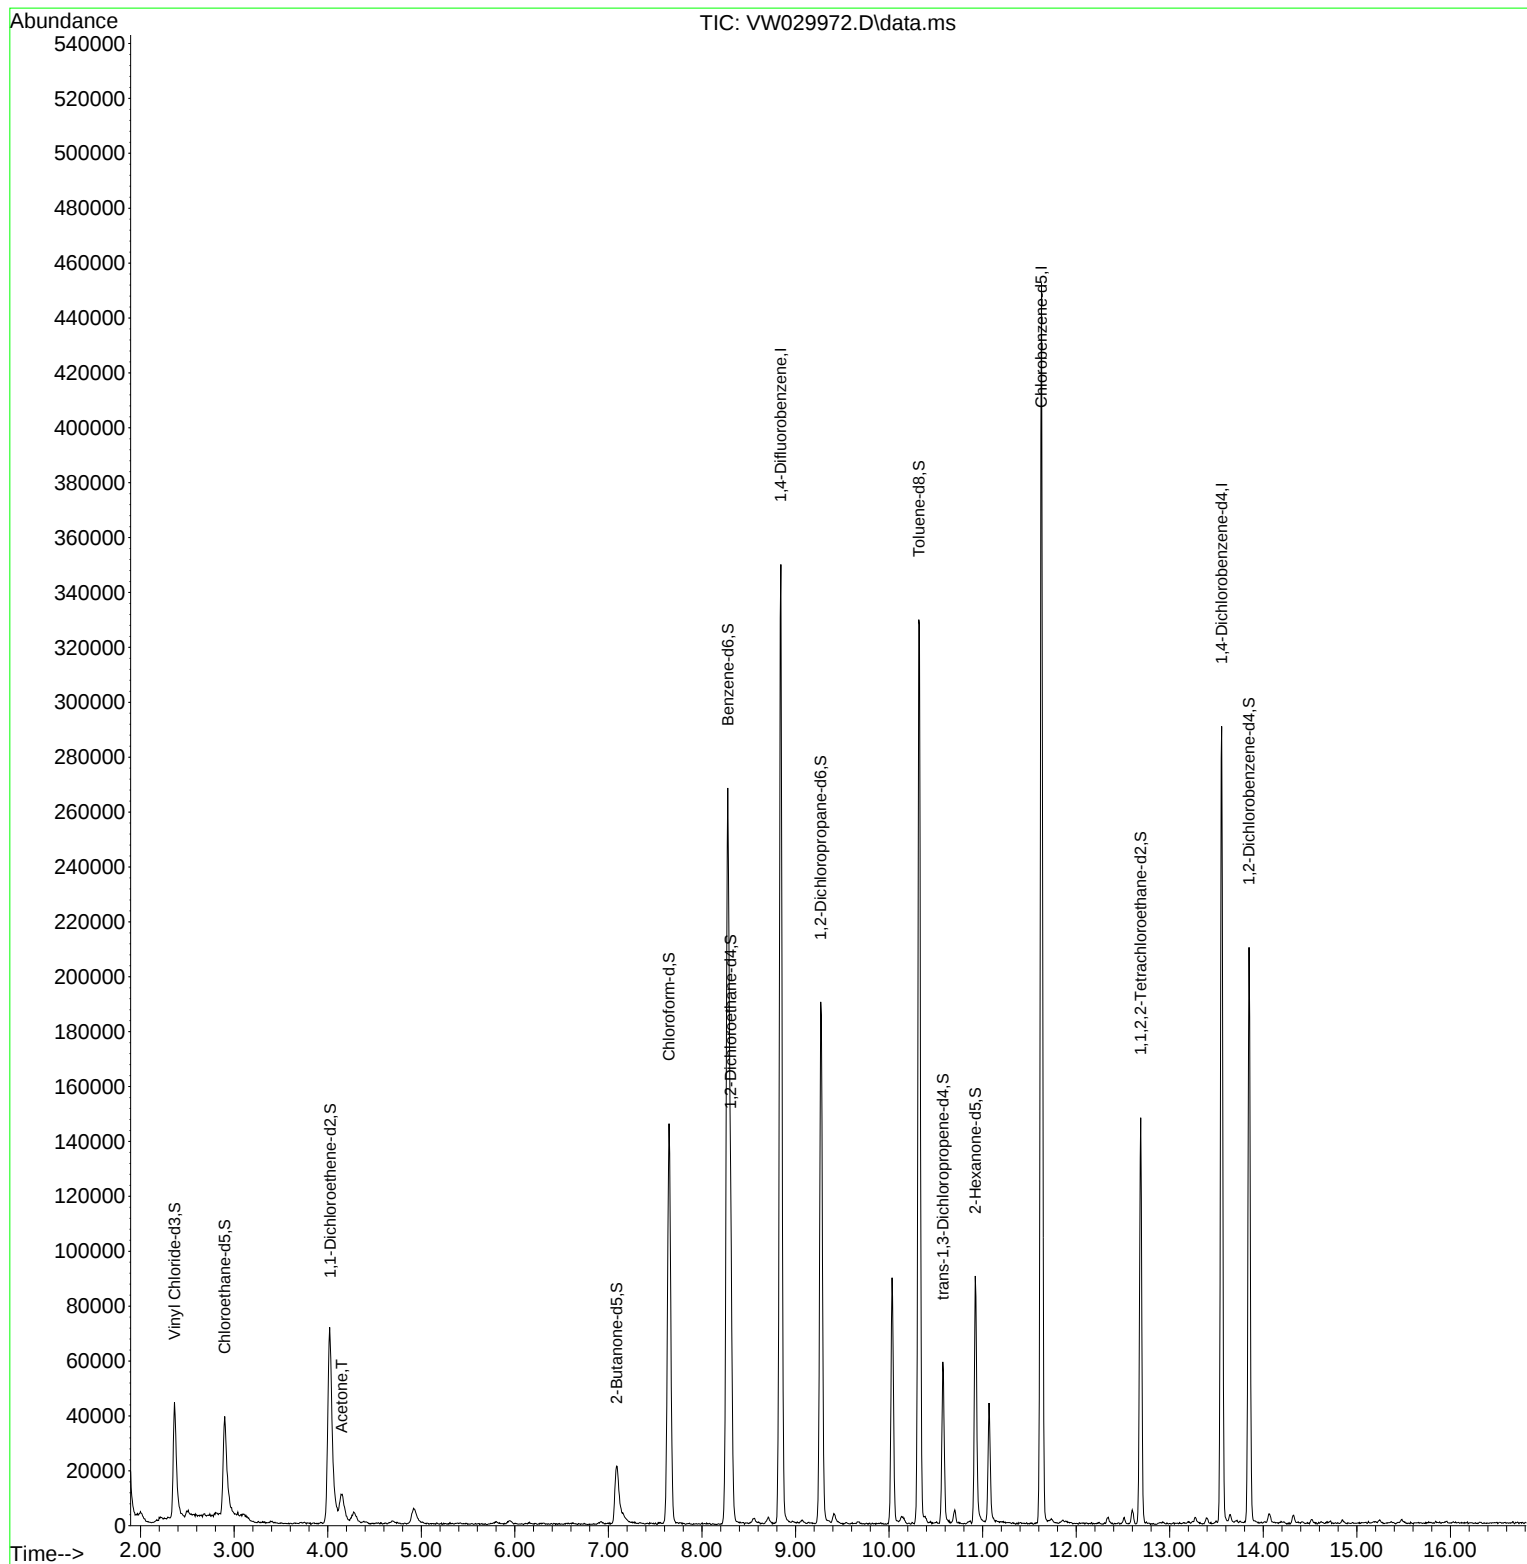

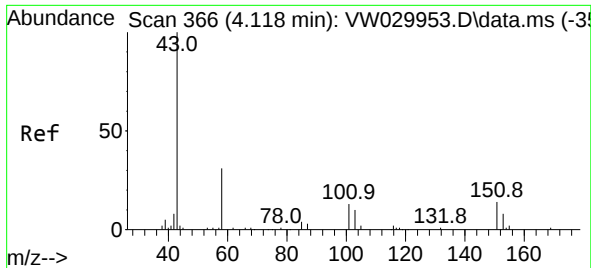

#13

Acetone

Concen: 15.661 ug/L

RT: 4.149 min Scan# 31

Delta R.T. 0.030 min

Lab File: VW029972.D


Acq: 20 Aug 2024 20:31

Instrument :

MSVOA_W

ClientSampleId :

DCYE3

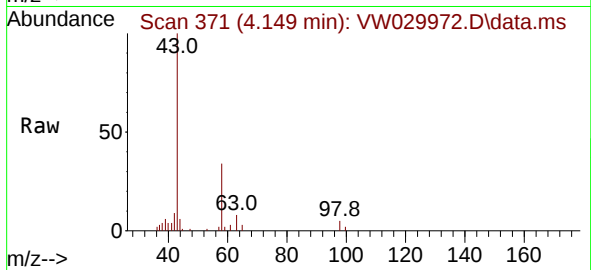

Tgt Ion: 43 Resp: 20964

Ion Ratio Lower Upper

43 100

58 32.3 0.0 57.6

