

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082224\
 Data File : VW029982.D
 Acq On : 22 Aug 2024 13:02
 Operator : SY/MD
 Sample : P3673-03
 Misc : 5.03g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCYD0

Quant Time: Aug 23 01:50:32 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 23 01:48:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	383744	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	335151	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.555	152	133247	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.362	65	79348	14.565	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	58.240%
7) Chloroethane-d5	2.899	69	67629	17.388	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	69.560%
11) 1,1-Dichloroethene-d2	4.021	65	36216	14.563	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	58.240%
21) 2-Butanone-d5	7.093	46	46589	31.201	ug/L	0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	62.400%
24) Chloroform-d	7.648	84	193841	19.513	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	78.040%
26) 1,2-Dichloroethane-d4	8.306	65	105650	18.672	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	74.680%
32) Benzene-d6	8.276	84	348740	19.258	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	77.040%
36) 1,2-Dichloropropane-d6	9.270	67	111237	19.238	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	76.960%
41) Toluene-d8	10.324	98	315304	19.582	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	78.320%
43) trans-1,3-Dichloroprop...	10.574	79	43499	18.591	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	74.360%
47) 2-Hexanone-d5	10.922	63	37967	39.821	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	79.640%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	95005	22.128	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	88.520%
66) 1,2-Dichlorobenzene-d4	13.848	152	94398	22.816	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	91.280%
Target Compounds					Qvalue	
13) Acetone	4.155	43	99520	53.631	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082224\
Data File : VW029982.D
Acq On : 22 Aug 2024 13:02
Operator : SY/MD
Sample : P3673-03
Misc : 5.03g/10mL/MSVOA_W/SOIL/A
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCYD0

Quant Time: Aug 23 01:50:32 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 23 01:48:12 2024
Response via : Initial Calibration

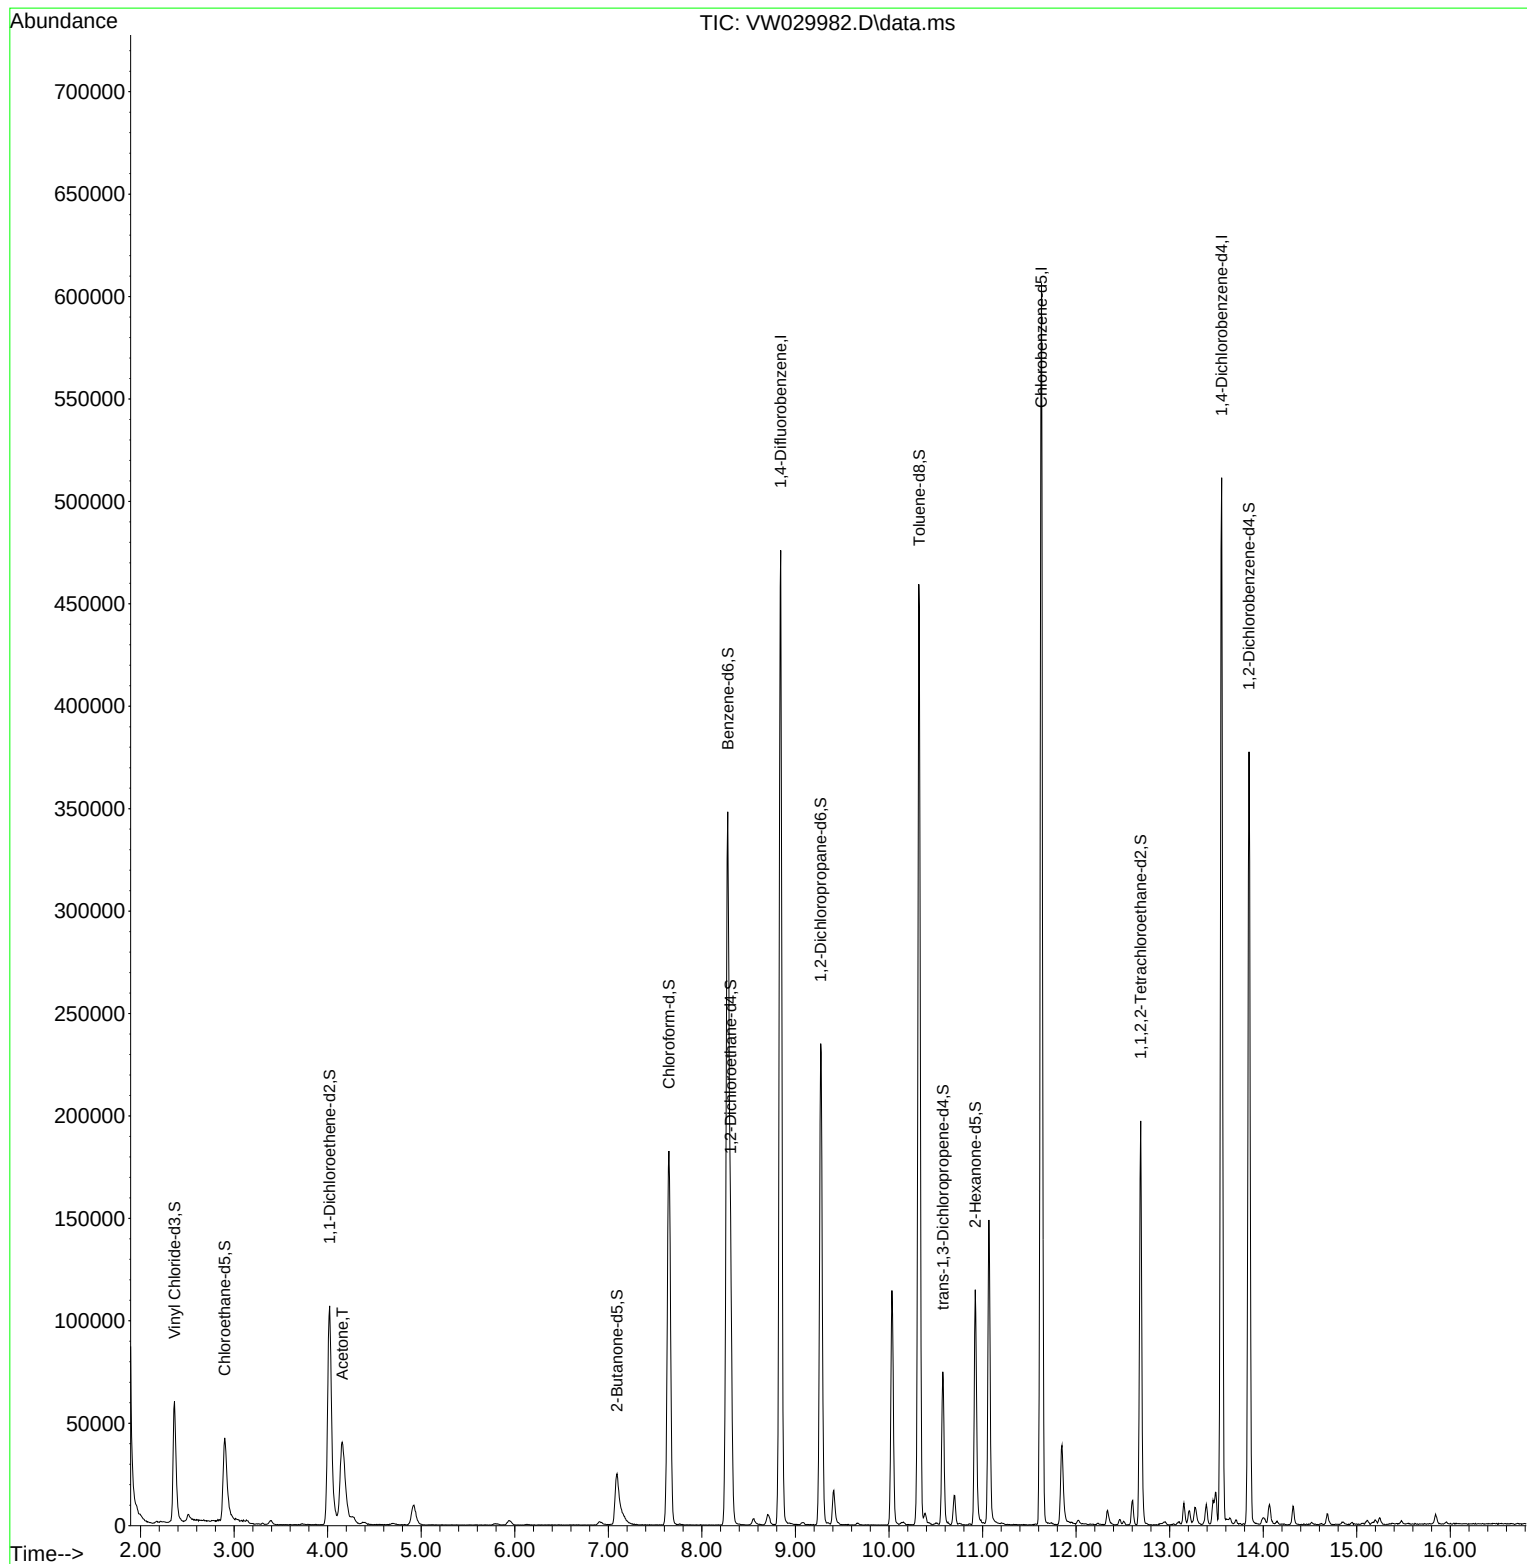

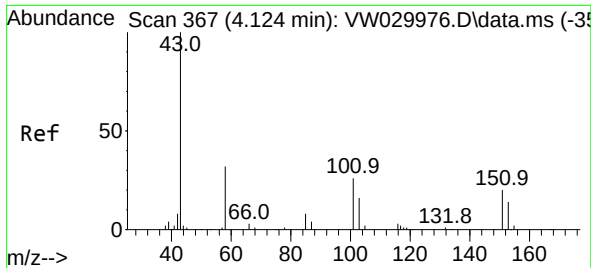

#13
 Acetone
 Concen: 53.631 ug/L
 RT: 4.155 min Scan# 31
 Delta R.T. 0.030 min
 Lab File: VW029982.D
 Acq: 22 Aug 2024 13:02

Instrument :
 MSVOA_W
 ClientSampleId :
 DCYD0

Tgt Ion: 43 Resp: 99520
 Ion Ratio Lower Upper
 43 100
 58 32.4 0.0 57.6

