

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082224\
 Data File : VW029990.D
 Acq On : 22 Aug 2024 16:13
 Operator : SY/MD
 Sample : P3673-12
 Misc : 4.83g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCYC3

Quant Time: Aug 23 01:52:26 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 23 01:48:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	184081	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	174055	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	68518	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.357	65	39109	14.965	ug/L	-0.01
Spiked Amount	25.000	Range 30 - 150	Recovery	=	59.880%	
7) Chloroethane-d5	2.899	69	33025	17.701	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	70.800%	
11) 1,1-Dichloroethene-d2	4.015	65	18349	15.381	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery	=	61.520%	
21) 2-Butanone-d5	7.081	46	21075	29.423	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	58.840%	
24) Chloroform-d	7.648	84	87670	18.398	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	=	73.600%	
26) 1,2-Dichloroethane-d4	8.307	65	48981	18.046	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	=	72.200%	
32) Benzene-d6	8.276	84	156358	16.626	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	=	66.520%	
36) 1,2-Dichloropropane-d6	9.270	67	51242	17.064	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	=	68.240%#	
41) Toluene-d8	10.325	98	132930	15.897	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	=	63.600%	
43) trans-1,3-Dichloroprop...	10.575	79	18487	15.214	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	=	60.840%	
47) 2-Hexanone-d5	10.922	63	16056	32.426	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	64.860%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	45655	20.476	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	=	81.920%	
66) 1,2-Dichlorobenzene-d4	13.848	152	41976	19.730	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	=	78.920%	
Target Compounds						
13) Acetone	4.125	43	25262	28.379	ug/L	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082224\
Data File : VW029990.D
Acq On : 22 Aug 2024 16:13
Operator : SY/MD
Sample : P3673-12
Misc : 4.83g/10mL/MSVOA_W/SOIL/A
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCYC3

Quant Time: Aug 23 01:52:26 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 23 01:48:12 2024
Response via : Initial Calibration

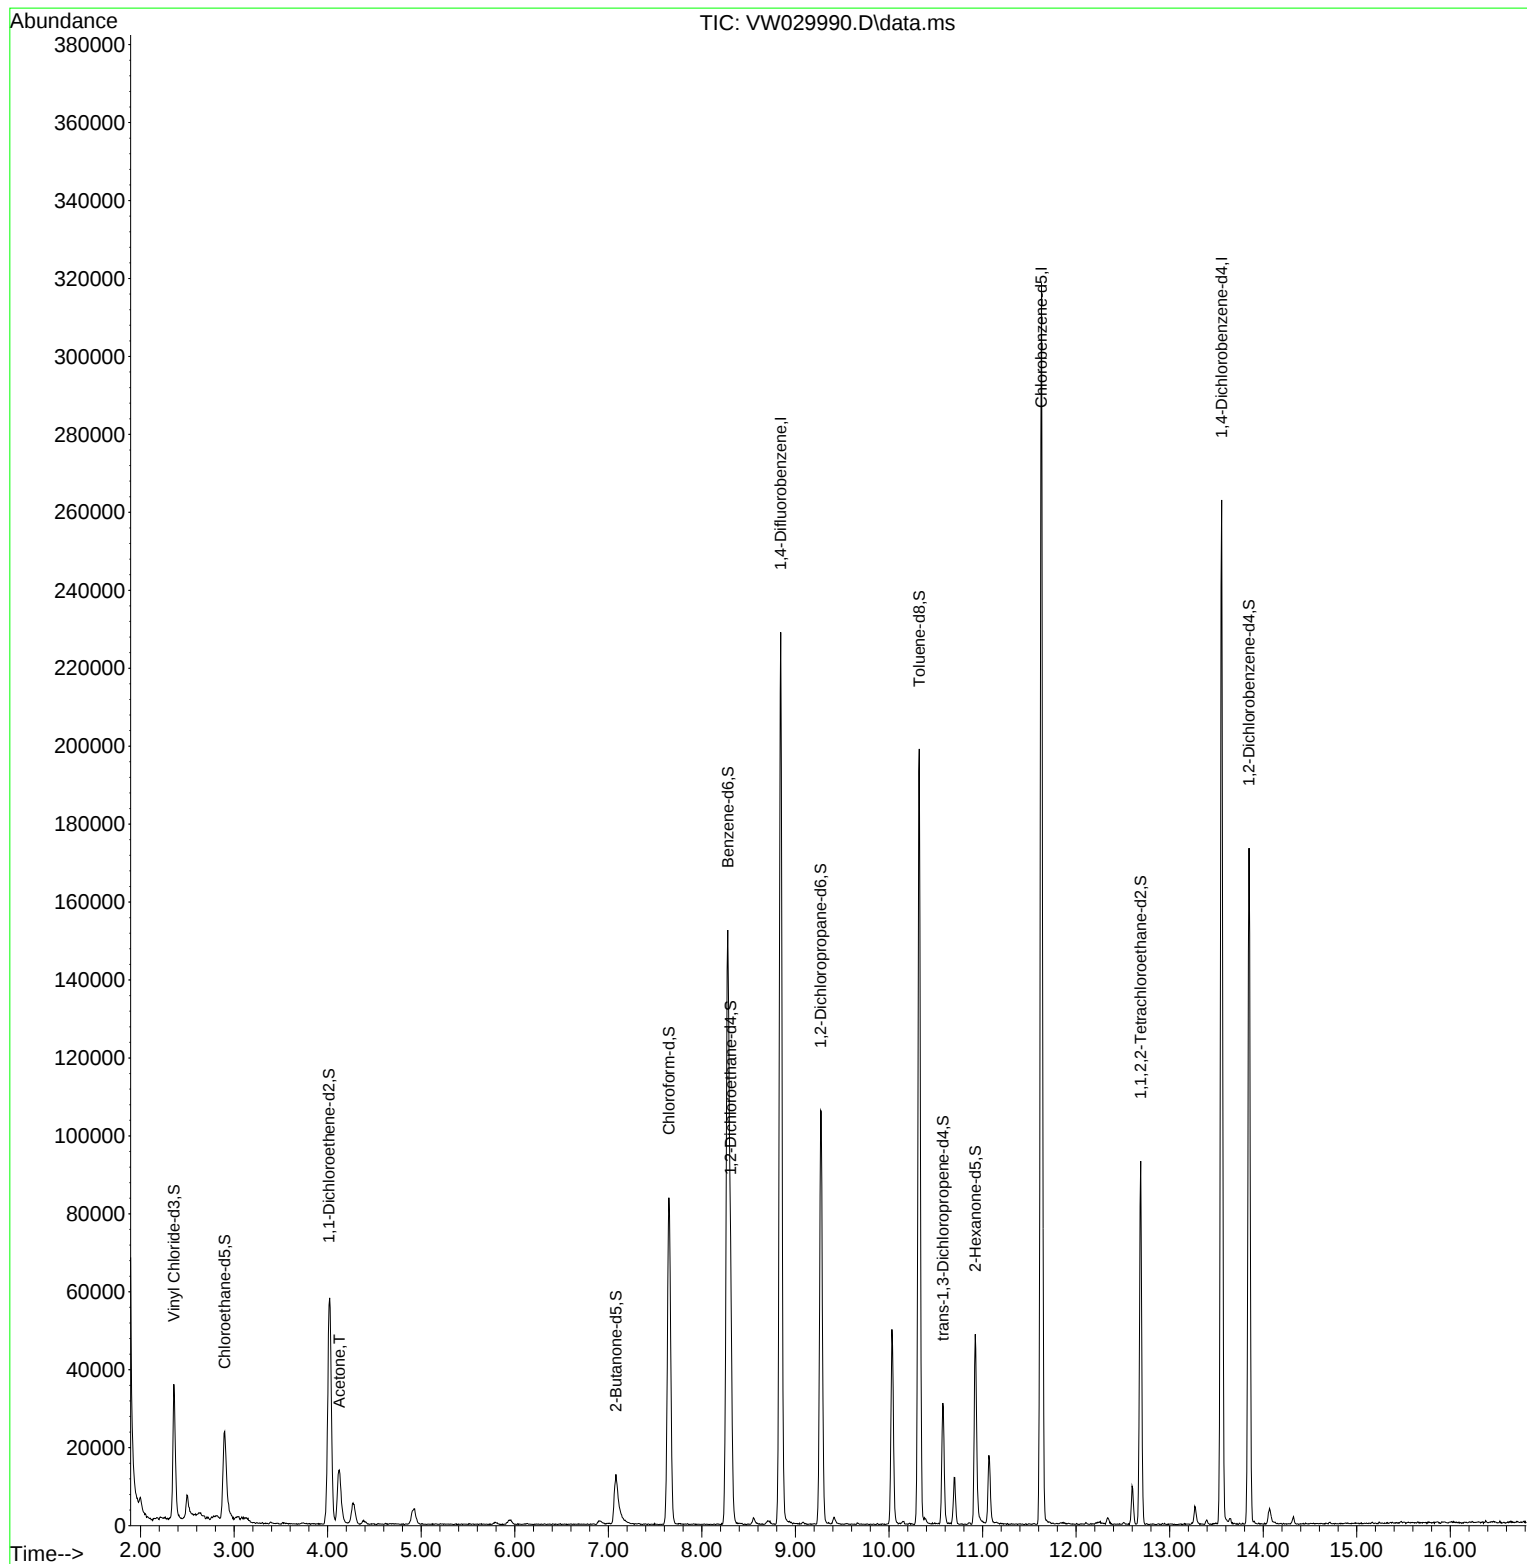

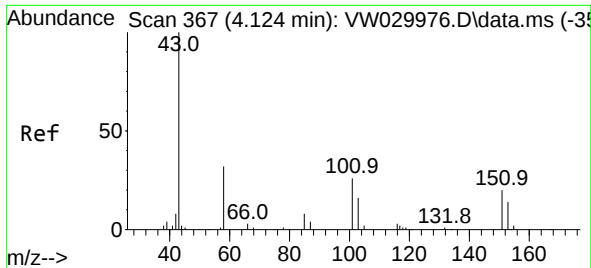

#13
 Acetone
 Concen: 28.379 ug/L
 RT: 4.125 min Scan# 30
 Delta R.T. 0.000 min
 Lab File: VW029990.D
 Acq: 22 Aug 2024 16:13

Instrument :
 MSVOA_W
 ClientSampleId :
 DCYC3

Tgt Ion: 43 Resp: 25262
 Ion Ratio Lower Upper
 43 100
 58 31.6 0.0 57.6

