

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082224\
 Data File : VW029992.D
 Acq On : 22 Aug 2024 17:01
 Operator : SY/MD
 Sample : P3673-15
 Misc : 4.65g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCXX6

Quant Time: Aug 23 01:52:57 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 23 01:48:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	412061	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	368602	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	140440	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	69941	11.956	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	47.840%		
7) Chloroethane-d5	2.899	69	63196	15.131	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	60.520%		
11) 1,1-Dichloroethene-d2	4.021	65	32519	12.178	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	48.720%		
21) 2-Butanone-d5	7.075	46	49088	30.616	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	61.240%		
24) Chloroform-d	7.648	84	188116	17.636	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	70.560%		
26) 1,2-Dichloroethane-d4	8.307	65	103149	16.977	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	67.920%#		
32) Benzene-d6	8.276	84	331405	16.640	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	66.560%		
36) 1,2-Dichloropropane-d6	9.276	67	108590	17.076	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	68.320%#		
41) Toluene-d8	10.325	98	296378	16.736	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	66.960%		
43) trans-1,3-Dichloroprop...	10.575	79	41294	16.047	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	64.200%		
47) 2-Hexanone-d5	10.922	63	38873	37.071	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	74.140%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	94297	19.970	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	79.880%		
66) 1,2-Dichlorobenzene-d4	13.848	152	87177	19.991	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	79.960%		
Target Compounds					Qvalue	
13) Acetone	4.124	43	10597	5.318	ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082224\
Data File : VW029992.D
Acq On : 22 Aug 2024 17:01
Operator : SY/MD
Sample : P3673-15
Misc : 4.65g/10mL/MSVOA_W/SOIL/A
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCXX6

Quant Time: Aug 23 01:52:57 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 23 01:48:12 2024
Response via : Initial Calibration

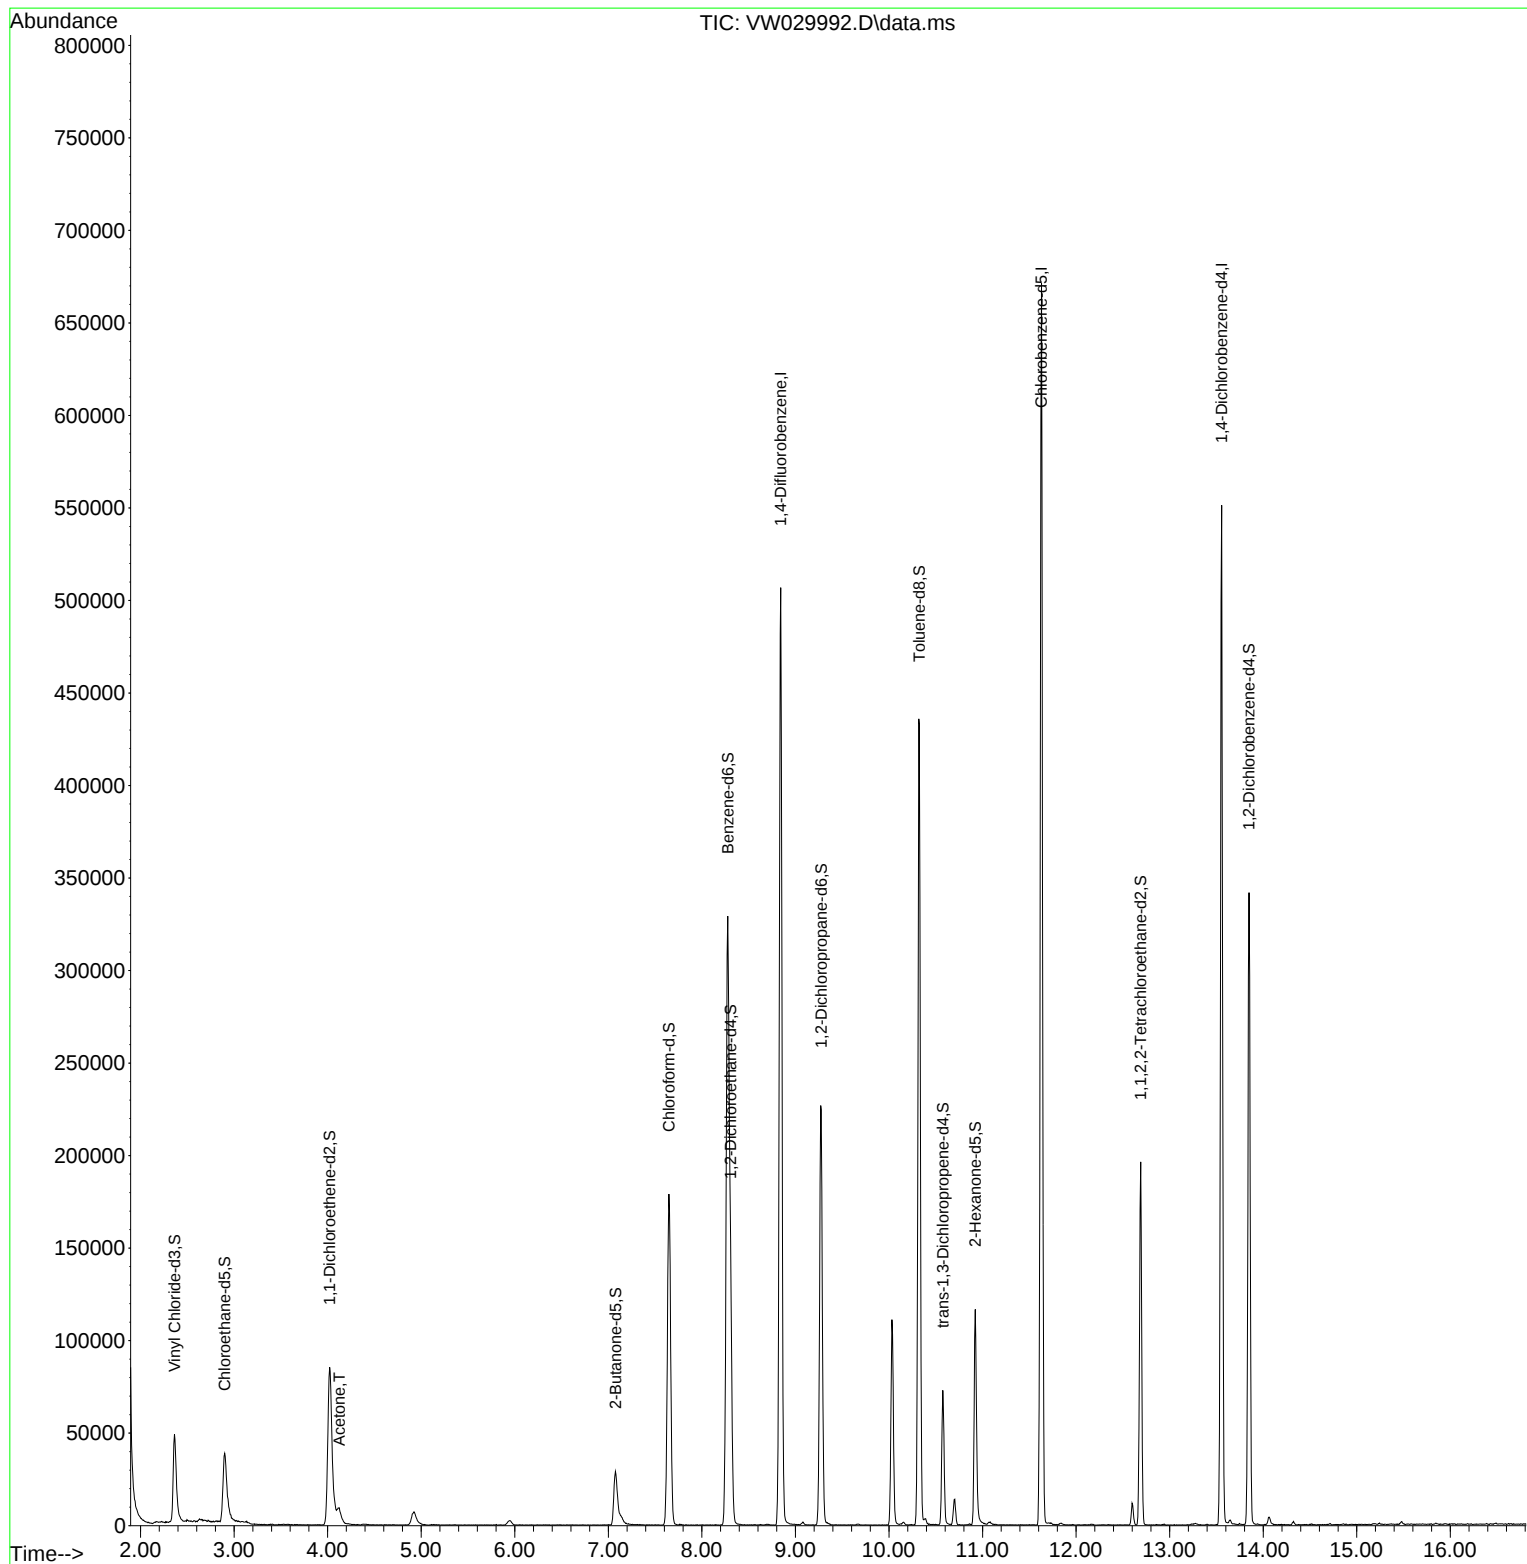

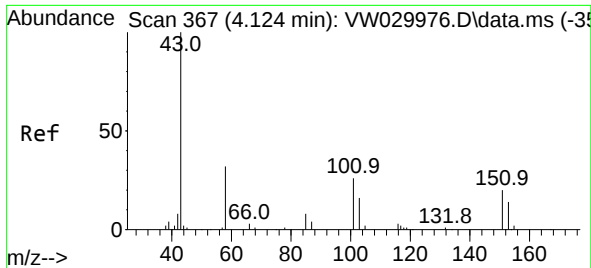

#13
 Acetone
 Concen: 5.318 ug/L
 RT: 4.124 min Scan# 367
 Delta R.T. 0.000 min
 Lab File: VW029992.D
 Acq: 22 Aug 2024 17:01

Instrument :
 MSVOA_W
 ClientSampleId :
 DCXX6

Tgt Ion: 43 Resp: 10597
 Ion Ratio Lower Upper
 43 100
 58 35.8 0.0 57.6

