

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082322\
 Data File : VW024303.D
 Acq On : 23 Aug 2022 15:22
 Operator : SY/VA
 Sample : N4168-15
 Misc : 5.02g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Quant Time: Aug 24 01:07:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 24 01:06:02 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	259436	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117	257610	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	122690	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.342	65	112313	20.711	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.840%
7) Chloroethane-d5	2.873	69	79279	23.468	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.880%
11) 1,1-Dichloroethene-d2	4.007	63	100717	16.297	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	65.200%
21) 2-Butanone-d5	7.079	46	65226	64.651	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	129.300%
24) Chloroform-d	7.646	84	201609	25.683	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	102.720%
26) 1,2-Dichloroethane-d4	8.299	65	118570	27.206	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	108.840%
32) Benzene-d6	8.274	84	358596	23.603	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	94.400%
36) 1,2-Dichloropropane-d6	9.274	67	113806	25.371	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	101.480%
41) Toluene-d8	10.323	98	314330	22.135	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	88.520%
43) trans-1,3-Dichloroprop...	10.579	79	47747	24.302	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	97.200%
47) 2-Hexanone-d5	10.920	63	49677	59.957	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	119.920%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	119845	27.537	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	110.160%
66) 1,2-Dichlorobenzene-d4	13.853	152	127949	28.498	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	114.000%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.030	75	4385	0.792	ug/L	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082322\
Data File : VW024303.D
Acq On : 23 Aug 2022 15:22
Operator : SY/VA
Sample : N4168-15
Misc : 5.02g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Quant Time: Aug 24 01:07:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Aug 24 01:06:02 2022
Response via : Initial Calibration

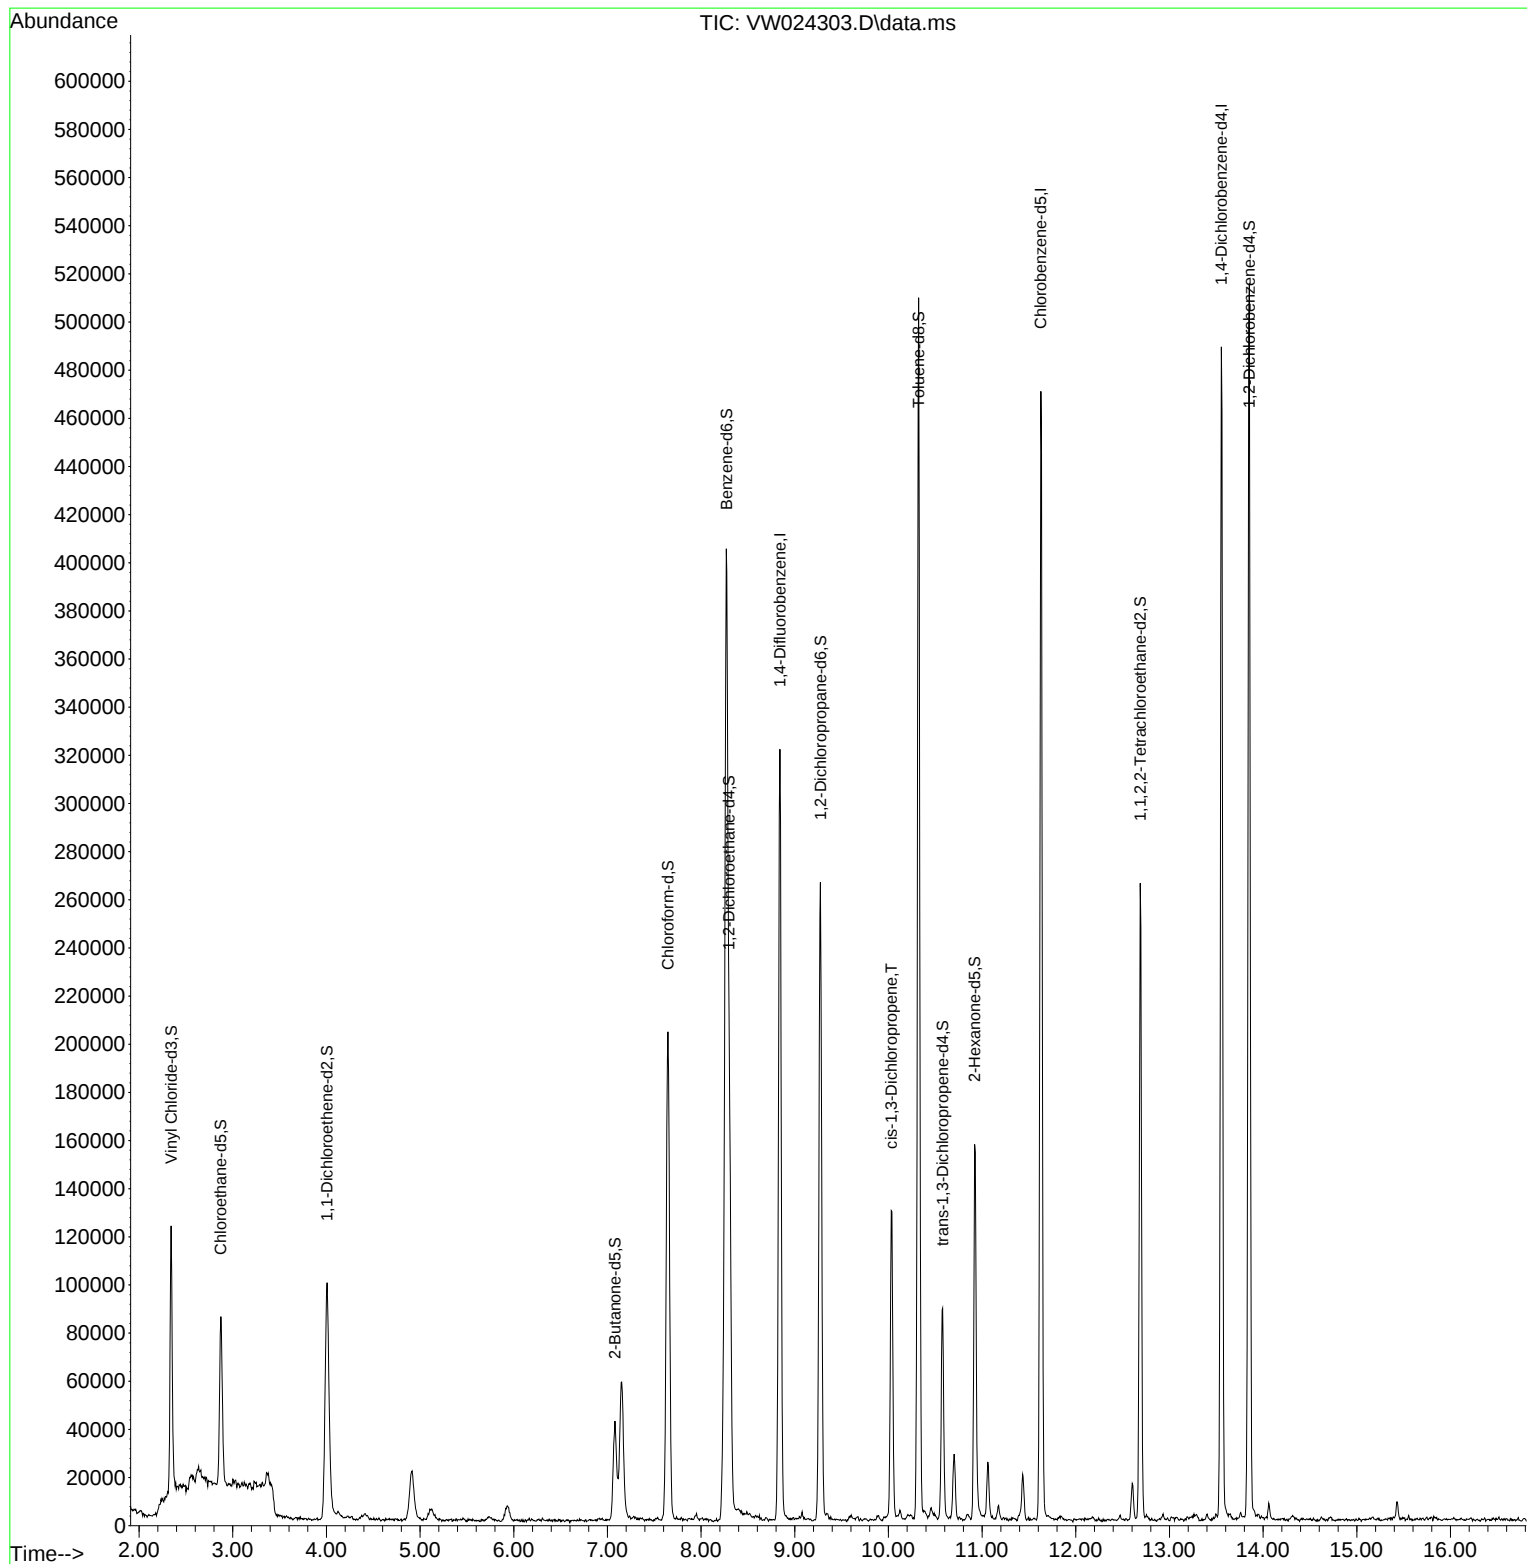

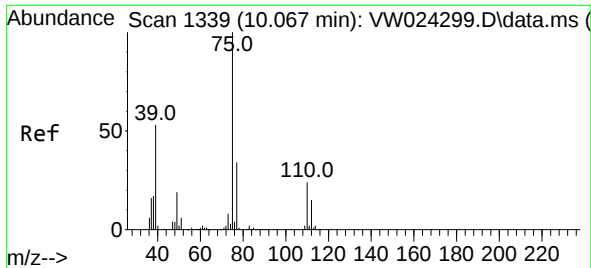

#39
 cis-1,3-Dichloropropene
 Concen: 0.792 ug/L
 RT: 10.030 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW024303.D
 Acq: 23 Aug 2022 15:22

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Tgt Ion: 75 Resp: 4385
 Ion Ratio Lower Upper
 75 100
 77 41.6 23.4 43.6

