

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082324\
 Data File : VW030003.D
 Acq On : 23 Aug 2024 12:19
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Aug 24 05:02:11 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 24 05:00:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	238262	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	234179	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	106966	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	55715	16.471	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	65.880%
7) Chloroethane-d5	3.009	69	314	0.130	ug/L	0.10
Spiked Amount	25.000	Range	30 - 150	Recovery	=	0.520%#
11) 1,1-Dichloroethene-d2	4.021	65	26586	17.218	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	68.880%
21) 2-Butanone-d5	7.087	46	29265	31.566	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	63.140%
24) Chloroform-d	7.654	84	143863	23.325	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.280%
26) 1,2-Dichloroethane-d4	8.307	65	78240	22.271	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	89.080%
32) Benzene-d6	8.276	84	263065	20.791	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	83.160%
36) 1,2-Dichloropropane-d6	9.276	67	83132	20.576	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	82.320%
41) Toluene-d8	10.325	98	232296	20.647	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	82.600%
43) trans-1,3-Dichloroprop...	10.581	79	31279	19.133	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	76.520%
47) 2-Hexanone-d5	10.922	63	21293	31.962	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	63.920%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	66753	22.251	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	89.000%
66) 1,2-Dichlorobenzene-d4	13.848	152	82672	24.891	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	99.560%
Target Compounds						
					Qvalue	
16) Methylene chloride	4.929	84	18558	3.726	ug/L	81
39) cis-1,3-Dichloropropene	10.032	75	2657	0.415	ug/L #	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082324\
Data File : VW030003.D
Acq On : 23 Aug 2024 12:19
Operator : SY/MD
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Aug 24 05:02:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Aug 24 05:00:17 2024
Response via : Initial Calibration

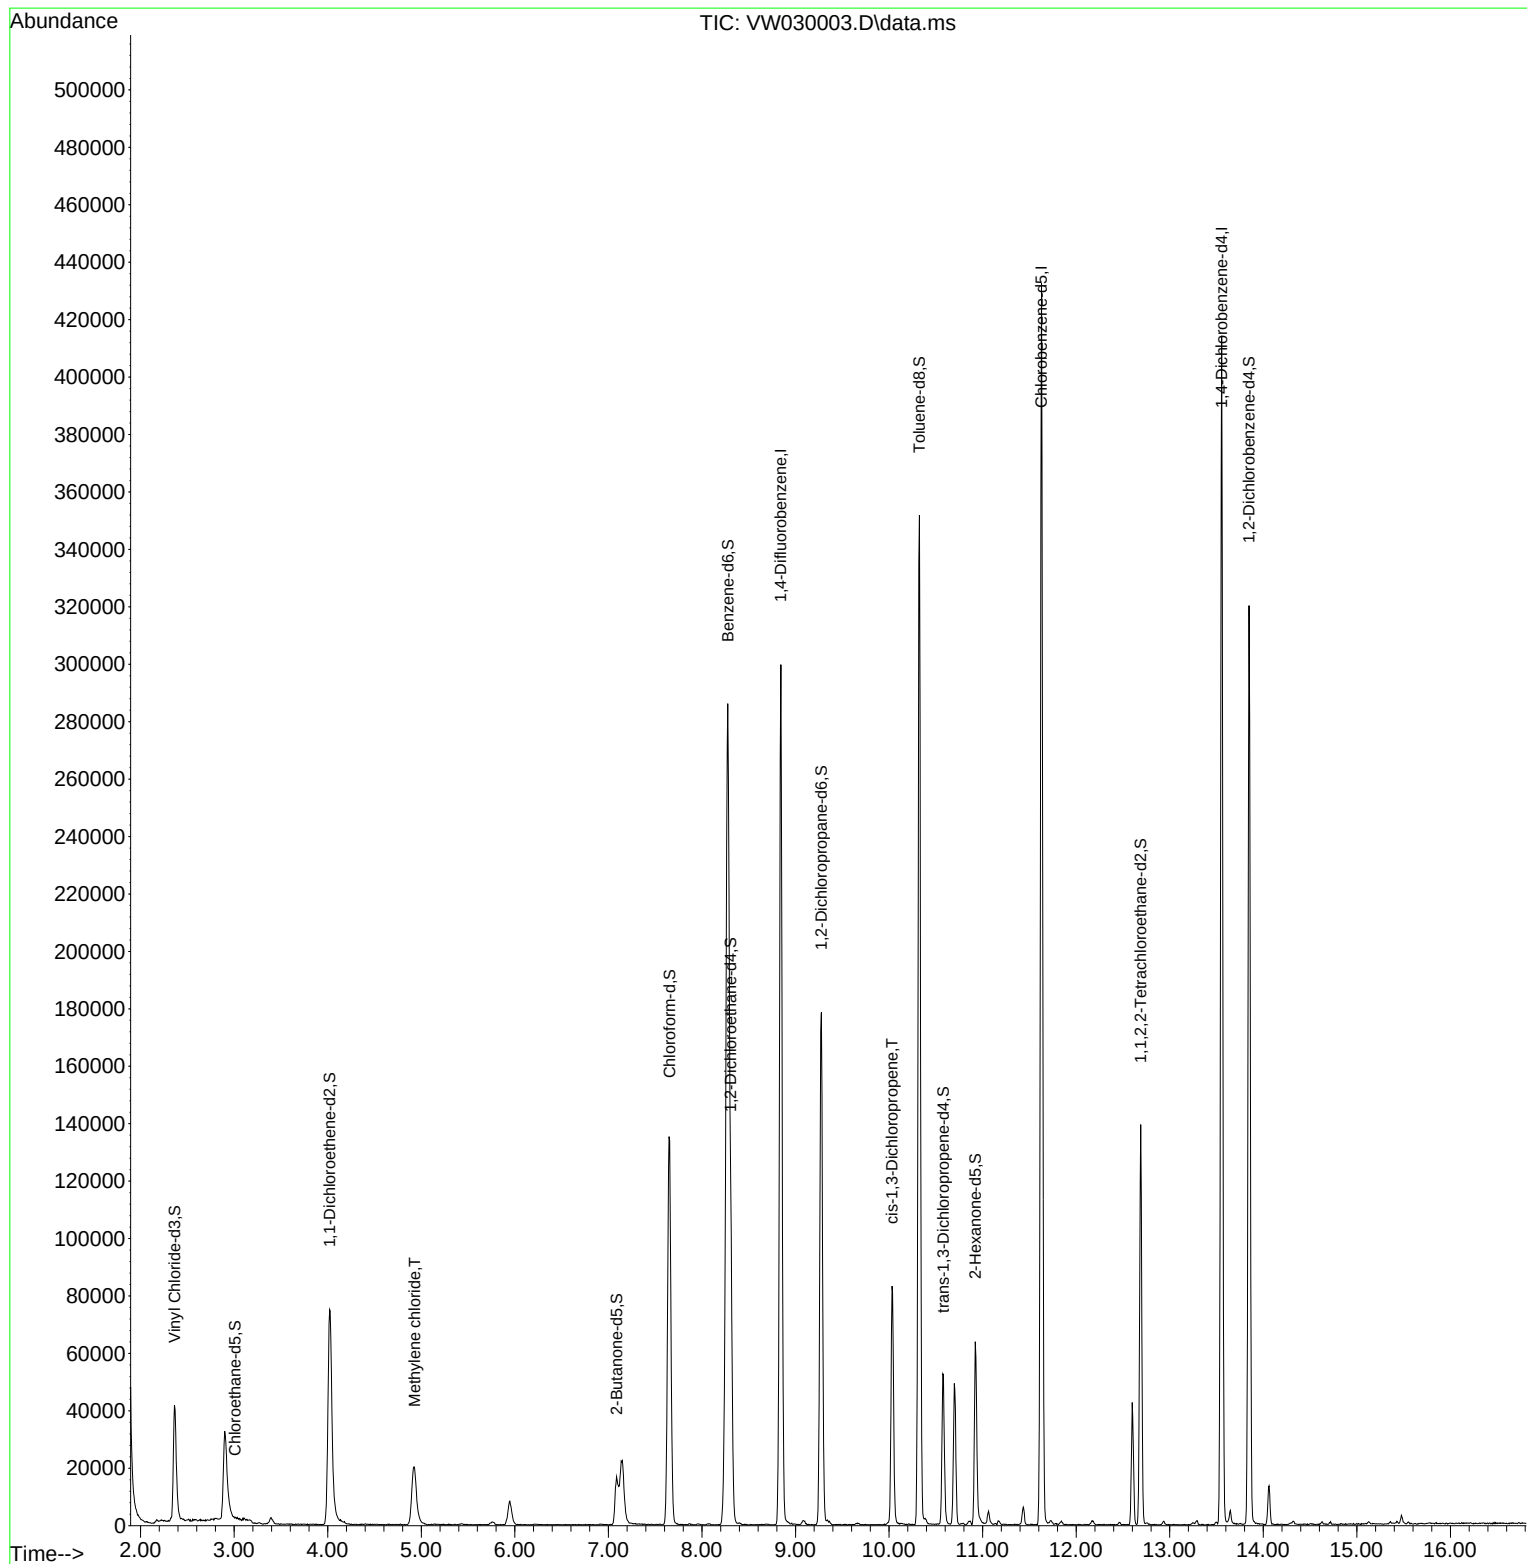



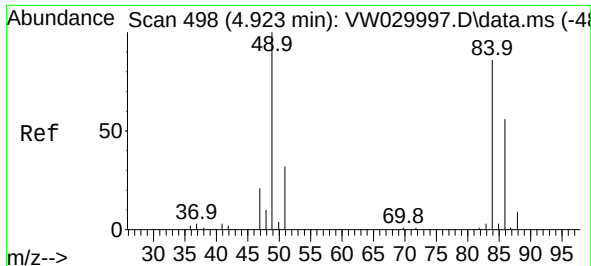


#16
Methylene chloride
Concen: 3.726 ug/L
RT: 4.929 min Scan# 499
Delta R.T. 0.006 min
Lab File: VW030003.D
Acq: 23 Aug 2024 12:19

Instrument :
MSVOA_W
ClientSampleId :

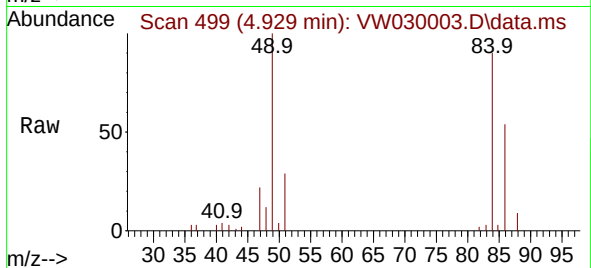

Tgt Ion: 84 Resp: 18558
Ion Ratio Lower Upper
84 100
86 60.0 44.7 82.9
49 111.2 99.0 184.0

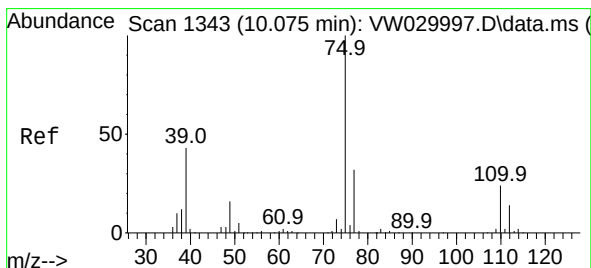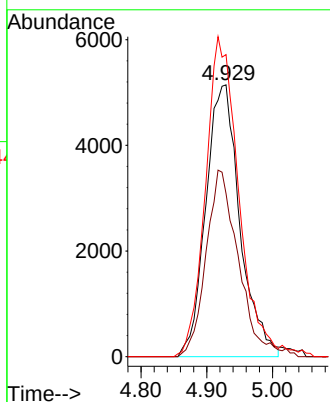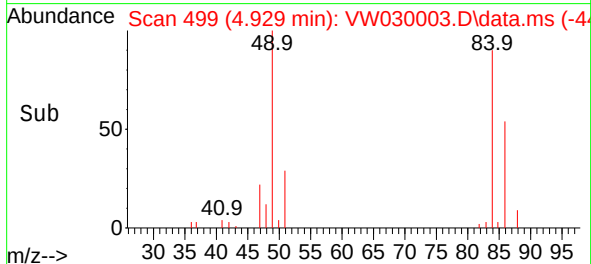

#39
cis-1,3-Dichloropropene
Concen: 0.415 ug/L
RT: 10.032 min Scan# 1336
Delta R.T. -0.043 min
Lab File: VW030003.D
Acq: 23 Aug 2024 12:19

Tgt Ion: 75 Resp: 2657
Ion Ratio Lower Upper
75 100
77 50.1 20.8 38.6#

