

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082324\
 Data File : VW030015.D
 Acq On : 23 Aug 2024 17:06
 Operator : SY/MD
 Sample : P3721-04
 Misc : 5.57g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCYD8

Quant Time: Aug 24 05:05:11 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 24 05:00:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	394012	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	315919	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	111851	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	65758	11.756	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	47.040%		
7) Chloroethane-d5	2.899	69	58560	14.664	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	58.640%		
11) 1,1-Dichloroethene-d2	4.027	65	33548	13.139	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	52.560%		
21) 2-Butanone-d5	7.075	46	62502	40.767	ug/L	-0.01
Spiked Amount 50.000	Range 20 - 135		Recovery =	81.540%		
24) Chloroform-d	7.648	84	179439	17.593	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	70.360%		
26) 1,2-Dichloroethane-d4	8.307	65	105792	18.210	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	72.840%		
32) Benzene-d6	8.276	84	322414	18.888	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	75.560%		
36) 1,2-Dichloropropane-d6	9.270	67	104728	19.215	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	76.840%		
41) Toluene-d8	10.325	98	283660	18.689	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	74.760%		
43) trans-1,3-Dichloroprop...	10.581	79	43505	19.726	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	78.920%		
47) 2-Hexanone-d5	10.922	63	51051	56.803	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	113.600%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	96124	23.752	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	95.000%		
66) 1,2-Dichlorobenzene-d4	13.848	152	70136	20.194	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	80.760%		
Target Compounds					Qvalue	
13) Acetone	4.118	43	76203	39.995	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082324\
Data File : VW030015.D
Acq On : 23 Aug 2024 17:06
Operator : SY/MD
Sample : P3721-04
Misc : 5.57g/10mL/MSVOA_W/SOIL/A
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCYD8

Quant Time: Aug 24 05:05:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Aug 24 05:00:17 2024
Response via : Initial Calibration

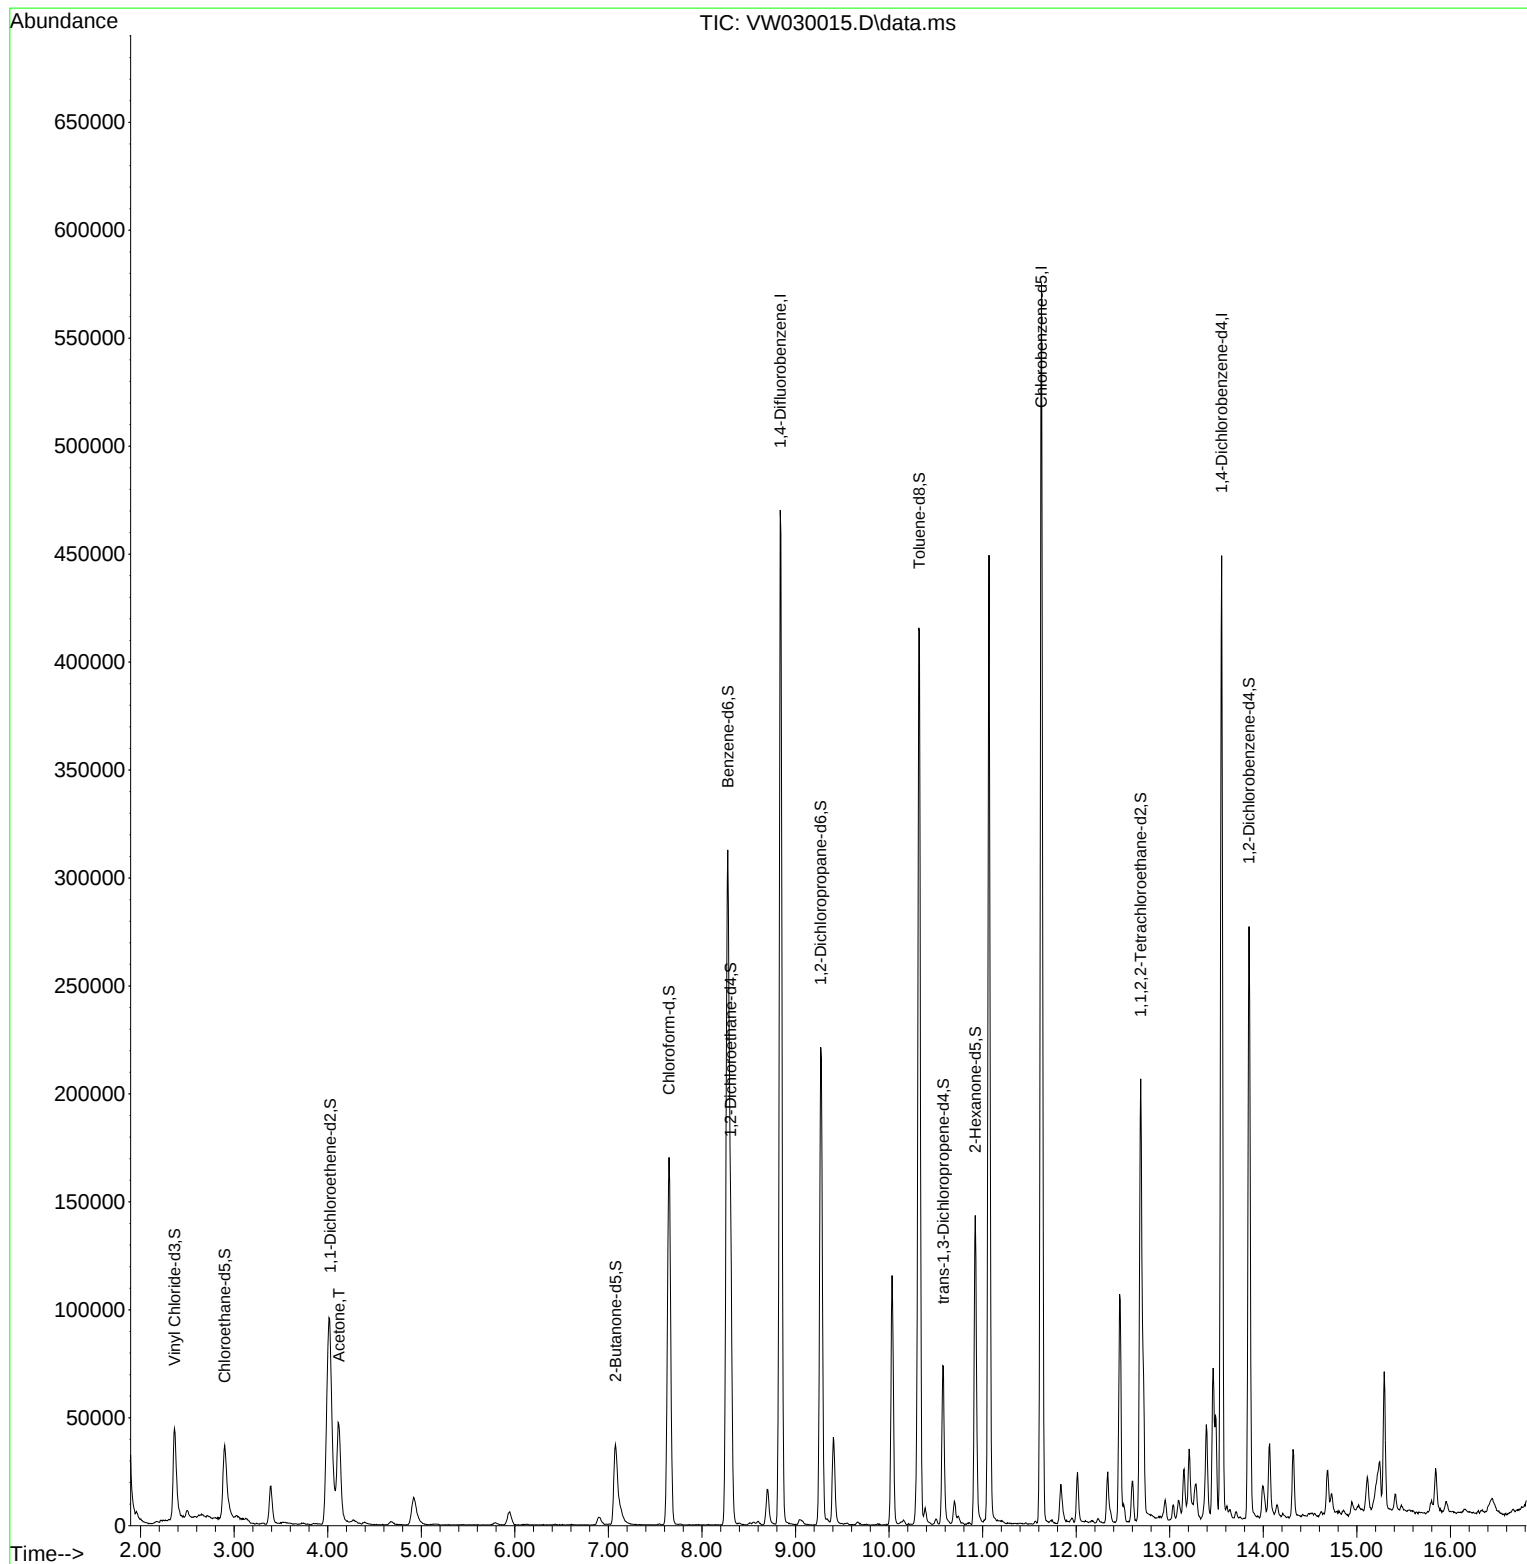

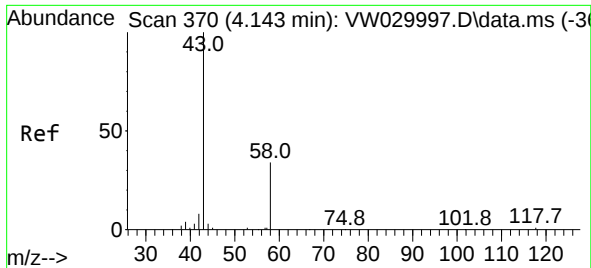

#13
 Acetone
 Concen: 39.995 ug/L
 RT: 4.118 min Scan# 30
 Delta R.T. -0.024 min
 Lab File: VW030015.D
 Acq: 23 Aug 2024 17:06

Instrument :
 MSVOA_W
 ClientSampleId :
 DCYD8

Tgt Ion: 43 Resp: 76203
 Ion Ratio Lower Upper
 43 100
 58 32.0 0.0 57.6

