

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082523\
 Data File : VW026910.D
 Acq On : 25 Aug 2023 22:15
 Operator : SY/MD
 Sample : 04157-24
 Misc : 5.85g/10mL/MSVOA_W/SOIL
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Aug 28 01:04:55 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 26 05:14:45 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	7420	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	5878	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	2659	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.259	65	158	1.295	ug/L	-0.11
Spiked Amount	25.000	Range	30 - 150	Recovery	=	5.200%#
7) Chloroethane-d5	2.899	69	2004	22.094	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.360%
11) 1,1-Dichloroethene-d2	4.021	65	240	4.001	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	16.000%#
21) 2-Butanone-d5	6.947	46	266	7.587	ug/L	-0.13
Spiked Amount	50.000	Range	20 - 135	Recovery	=	15.180%#
24) Chloroform-d	7.642	84	5550	22.286	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.160%
26) 1,2-Dichloroethane-d4	8.404	65	149	1.084	ug/L	0.10
Spiked Amount	25.000	Range	70 - 130	Recovery	=	4.320%#
32) Benzene-d6	8.276	84	9312	22.986	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	91.960%
36) 1,2-Dichloropropane-d6	9.270	67	3367	26.683	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	106.720%
41) Toluene-d8	10.331	98	6621	19.040	ug/L	0.01
Spiked Amount	25.000	Range	30 - 130	Recovery	=	76.160%
43) trans-1,3-Dichloroprop...	10.672	79	162	3.109	ug/L	0.10
Spiked Amount	25.000	Range	30 - 135	Recovery	=	12.440%#
47) 2-Hexanone-d5	10.910	63	74	5.581	ug/L	-0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	11.160%#
56) 1,1,2,2-Tetrachloroeth...	12.690	84	2476	24.846	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	99.400%
66) 1,2-Dichlorobenzene-d4	13.854	152	2021	21.235	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	84.960%
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	2.265	85	147	1.457	ug/L	93
3) Chloromethane	2.125	50	136	0.986	ug/L	85
6) Bromomethane	2.741	94	59	0.768	ug/L	80
9) Trichlorofluoromethane	3.198	101	104	0.961	ug/L	91
13) Acetone	4.143	43	531	15.233	ug/L	84
15) Methyl Acetate	4.679	43	130	1.862	ug/L	99
16) Methylene chloride	4.960	84	255	1.777	ug/L	91
17) trans-1,2-Dichloroethene	5.405	96	107	0.874	ug/L #	45
19) 1,1-Dichloroethane	6.234	63	168	0.667	ug/L #	7
22) 2-Butanone	7.258	43	158	3.076	ug/L	89
23) Bromochloromethane	7.624	128	63	1.109	ug/L #	1
29) Cyclohexane	7.959	56	129	0.710	ug/L #	50
30) 1,1,1-Trichloroethane	7.862	97	127	0.828	ug/L #	34
35) Methylcyclohexane	9.349	83	172	0.922	ug/L #	70
37) 1,2-Dichloropropane	9.367	63	117	0.998	ug/L #	88
38) Bromodichloromethane	9.624	83	190	1.381	ug/L #	24
39) cis-1,3-Dichloropropene	10.062	75	118	0.700	ug/L	85
40) 4-Methyl-2-pentanone	10.221	43	360	4.720	ug/L #	77
44) trans-1,3-Dichloropropene	10.447	75	130	0.895	ug/L	92

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082523\
 Data File : VW026910.D
 Acq On : 25 Aug 2023 22:15
 Operator : SY/MD
 Sample : 04157-24
 Misc : 5.85g/10mL/MSVOA_W/SOIL
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Aug 28 01:04:55 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 26 05:14:45 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


45) 1,1,2-Trichloroethane	10.800	97	81	1.010	ug/L #	68
46) Tetrachloroethene	10.861	164	102	1.288	ug/L #	72
48) 2-Hexanone	10.959	43	280	5.396	ug/L #	62
50) 1,2-Dibromoethane	11.251	107	105	1.396	ug/L #	61
57) 1,1,2,2-Tetrachloroethane	12.727	83	153	1.507	ug/L #	10
59) Bromoform	12.501	173	53	1.272	ug/L #	39
61) 1,2,3-Trichloropropane	12.763	75	245	3.799	ug/L #	63
63) 1,2,4-Trimethylbenzene	13.251	105	176	0.575	ug/L	100
64) 1,3-Dichlorobenzene	13.495	146	103	0.599	ug/L #	14
65) 1,4-Dichlorobenzene	13.574	146	219	1.221	ug/L #	81
67) 1,2-Dichlorobenzene	13.873	146	105	0.672	ug/L #	6
69) 1,3,5-Trichlorobenzene	14.610	180	75	0.646	ug/L #	29
71) Naphthalene	15.373	128	253	1.347	ug/L #	38
72) 1,2,3-Trichlorobenzene	15.555	180	88	0.991	ug/L #	24


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082523\
Data File : VW026910.D
Acq On : 25 Aug 2023 22:15
Operator : SY/MD
Sample : 04157-24
Misc : 5.85g/10mL/MSVOA_W/SOIL
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Aug 28 01:04:55 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Aug 26 05:14:45 2023
Response via : Initial Calibration




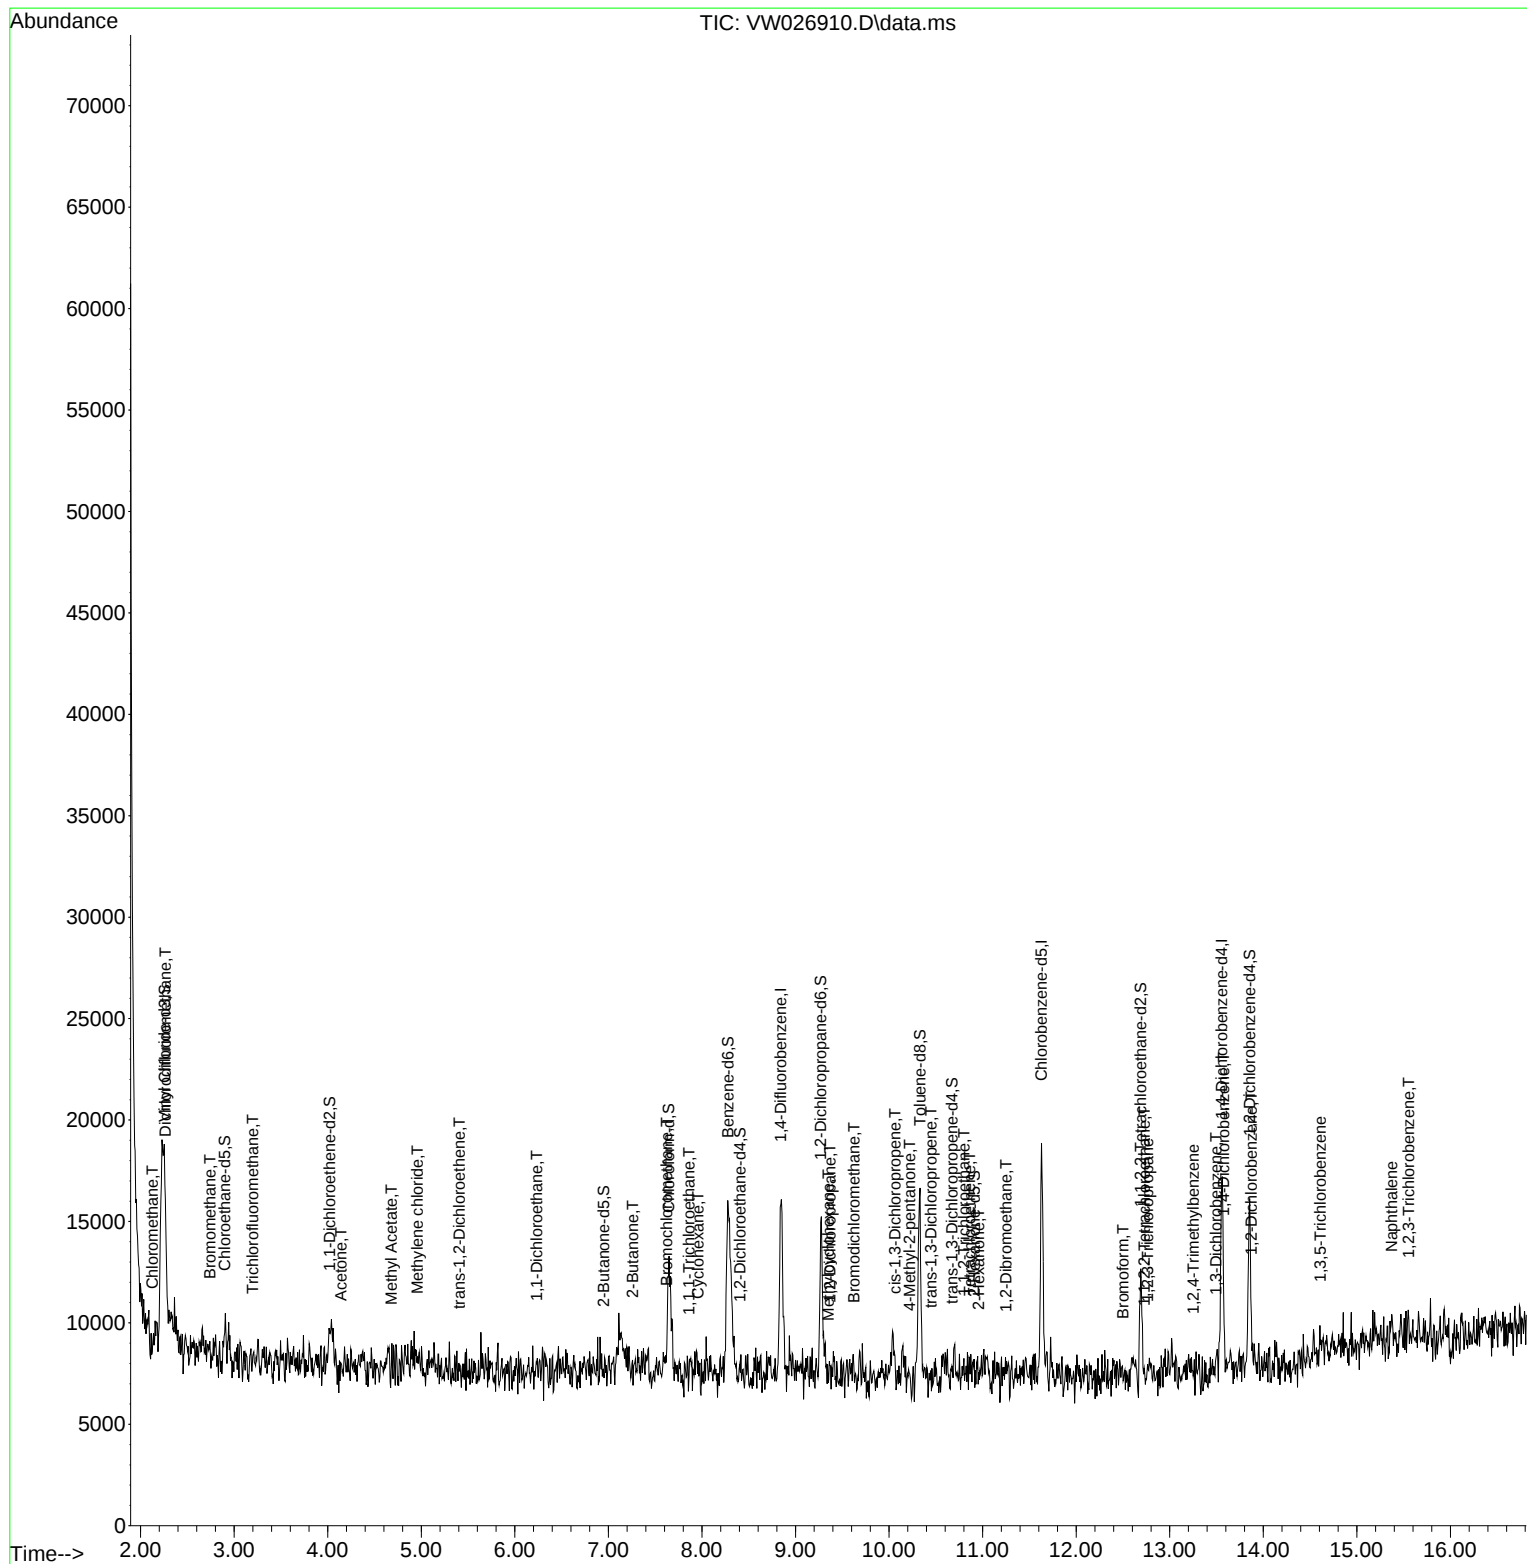




#2
Dichlorodifluoromethane
Concen: 1.457 ug/L
RT: 2.265 min Scan# 61
Delta R.T. 0.250 min
Lab File: VW026910.D
Acq: 25 Aug 2023 22:15




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion: 85 Resp: 147
Ion Ratio Lower Upper
85 100
87 27.9 19.5 29.3



#3
Chloromethane
Concen: 0.986 ug/L
RT: 2.125 min Scan# 39
Delta R.T. -0.104 min
Lab File: VW026910.D
Acq: 25 Aug 2023 22:15

Tgt Ion: 50 Resp: 136
Ion Ratio Lower Upper
50 100
52 41.3 23.0 42.8


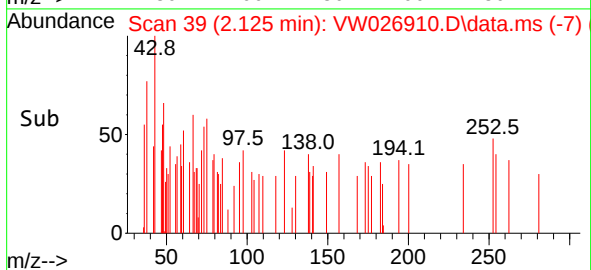






#6
Bromomethane
Concen: 0.768 ug/L
RT: 2.741 min Scan# 147
Delta R.T. -0.043 min
Lab File: VW026910.D
Acq: 25 Aug 2023 22:15




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion: 94 Resp: 59
Ion Ratio Lower Upper
94 100
96 73.8 64.8 120.3



#9
Trichlorofluoromethane
Concen: 0.961 ug/L
RT: 3.198 min Scan# 215
Delta R.T. -0.067 min
Lab File: VW026910.D
Acq: 25 Aug 2023 22:15

Tgt Ion: 101 Resp: 104
Ion Ratio Lower Upper
101 100
103 72.1 51.9 77.9









#13
Acetone
Concen: 15.233 ug/L
RT: 4.143 min Scan# 31
Delta R.T. 0.018 min
Lab File: VW026910.D
Acq: 25 Aug 2023 22:15




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion: 43 Resp: 531
Ion Ratio Lower Upper
43 100
58 37.1 0.0 57.4

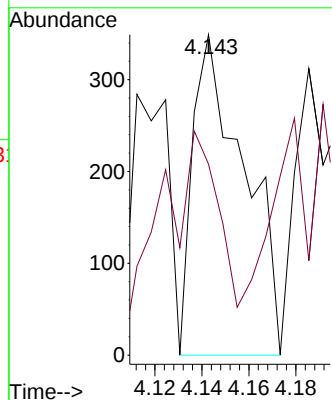

#15
Methyl Acetate
Concen: 1.862 ug/L
RT: 4.679 min Scan# 458
Delta R.T. 0.006 min
Lab File: VW026910.D
Acq: 25 Aug 2023 22:15

Tgt Ion: 43 Resp: 130
Ion Ratio Lower Upper
43 100
74 20.0 16.4 24.6


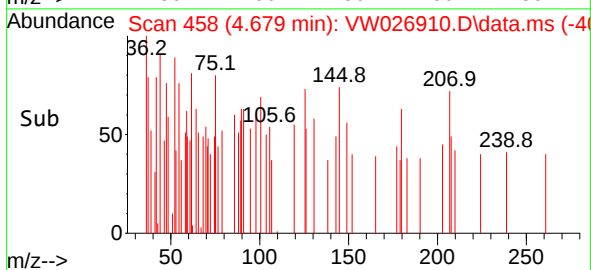
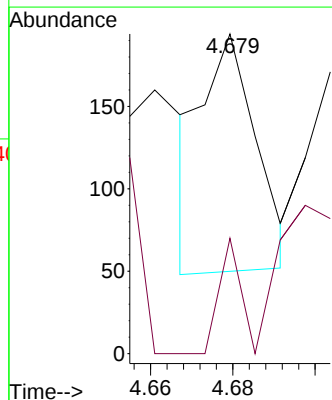





#16
Methylene chloride
Concen: 1.777 ug/L
RT: 4.960 min Scan# 504
Delta R.T. 0.037 min
Lab File: VW026910.D
Acq: 25 Aug 2023 22:15




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion: 84 Resp: 255
Ion Ratio Lower Upper
84 100
86 46.4 43.5 80.9
49 133.2 96.0 178.2

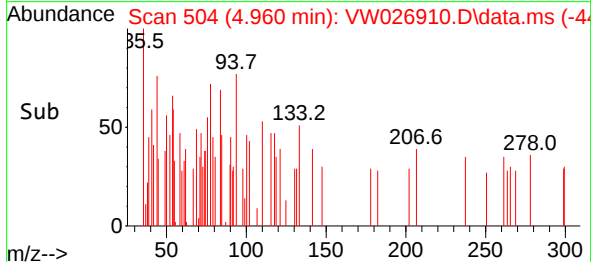

#17
trans-1,2-Dichloroethene
Concen: 0.874 ug/L
RT: 5.405 min Scan# 577
Delta R.T. -0.018 min
Lab File: VW026910.D
Acq: 25 Aug 2023 22:15

Tgt Ion: 96 Resp: 107
Ion Ratio Lower Upper
96 100
61 67.8 109.4 203.2#
98 44.4 43.6 81.0

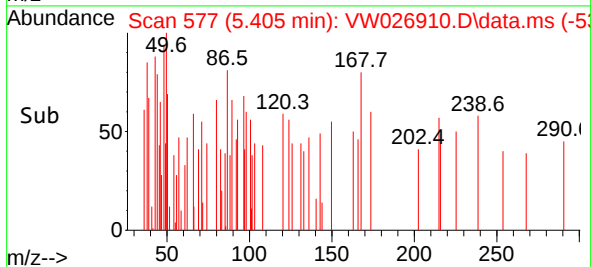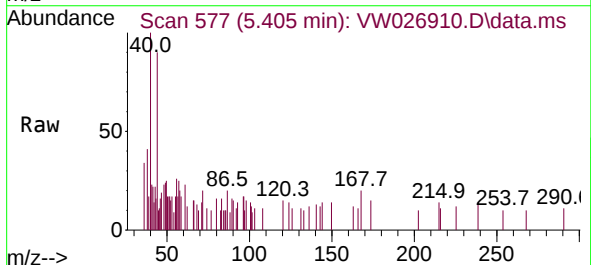



#19

1,1-Dichloroethane

Concen: 0.667 ug/L

RT: 6.234 min Scan# 710

Delta R.T. 0.018 min

Lab File: VW026910.D





Acq: 25 Aug 2023 22:15

Instrument :

MSVOA_W

ClientSampleId :

Tgt Ion: 63	Resp: 168
Ion Ratio	Lower Upper
63	100
65	87.2 21.8 40.6#
83	40.9 9.0 16.6#

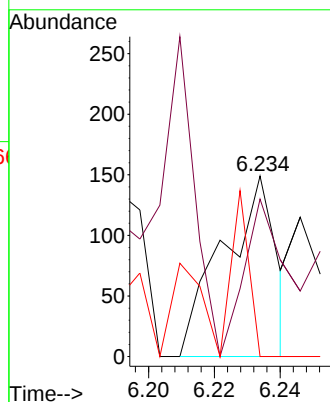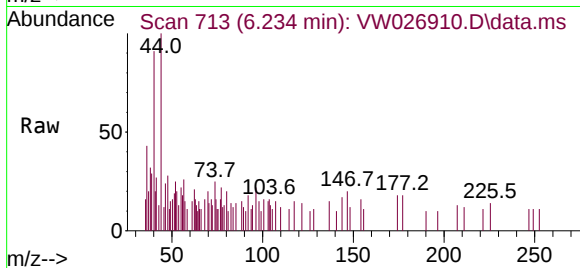

#22

2-Butanone

Concen: 3.076 ug/L




RT: 7.258 min Scan# 881


Delta R.T. 0.085 min

Lab File: VW026910.D

Acq: 25 Aug 2023 22:15


Tgt Ion: 43	Resp: 158
Ion Ratio	Lower Upper
43	100
72	18.4 11.8 35.4

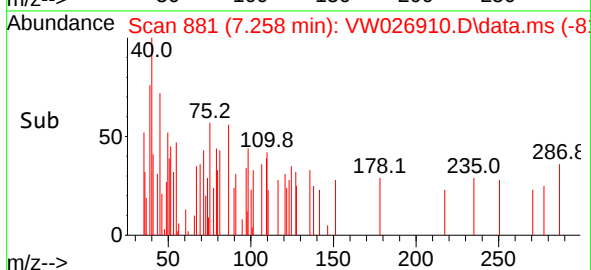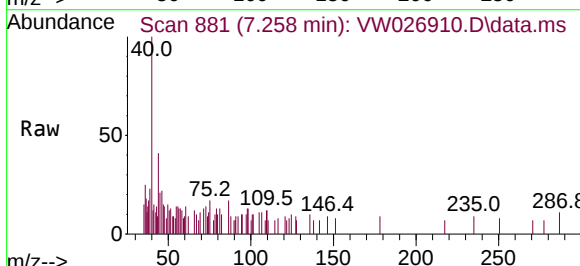



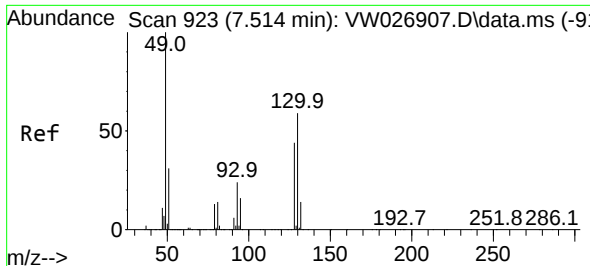


#23
Bromochloromethane
Concen: 1.109 ug/L
RT: 7.624 min Scan# 941
Delta R.T. 0.110 min
Lab File: VW026910.D
Acq: 25 Aug 2023 22:15

Instrument :
MSVOA_W
ClientSampleId :



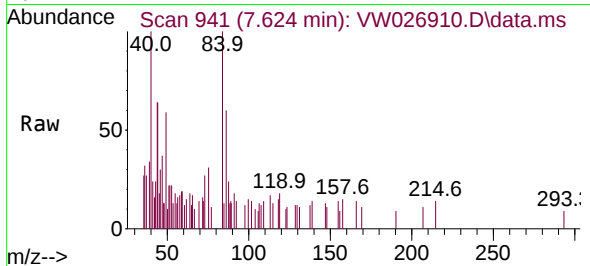



Tgt Ion:128 Resp: 63
Ion Ratio Lower Upper
128 100
49 500.0 143.1 265.7#
130 0.0 91.8 170.4#
51 381.3 53.0 79.4#

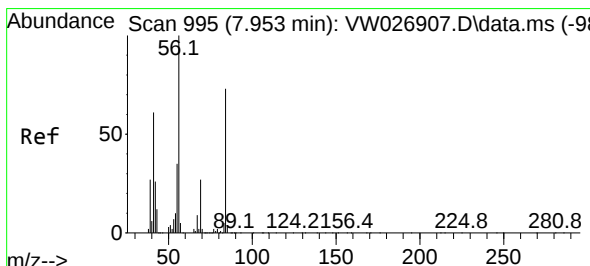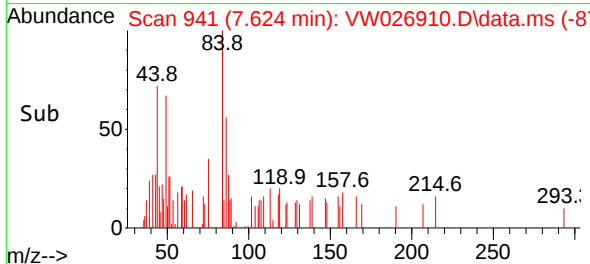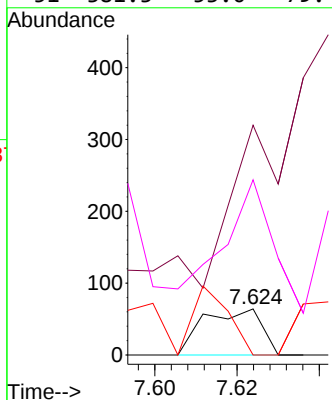

#29
Cyclohexane
Concen: 0.710 ug/L
RT: 7.959 min Scan# 996
Delta R.T. 0.006 min
Lab File: VW026910.D
Acq: 25 Aug 2023 22:15

Tgt Ion: 56 Resp: 129
Ion Ratio Lower Upper
56 100
69 0.0 23.2 34.8#
84 35.7 62.7 94.1#

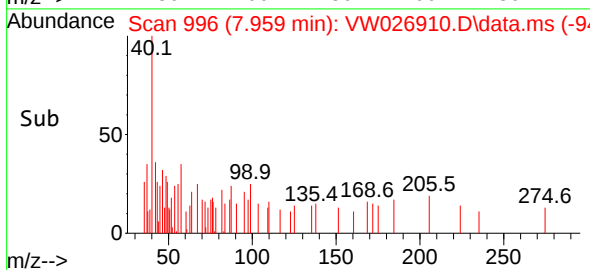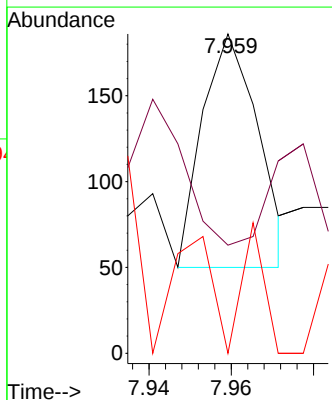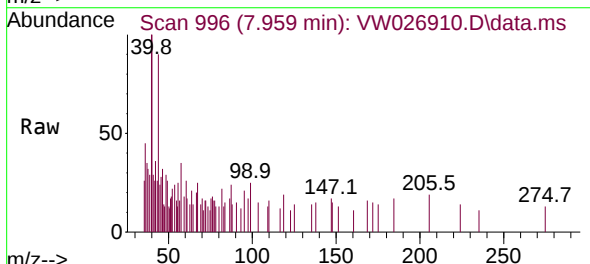



#30

1,1,1-Trichloroethane

Concen: 0.828 ug/L

RT: 7.862 min Scan# 91

Delta R.T. -0.012 min

Lab File: VW026910.D

Acq: 25 Aug 2023 22:15

Instrument :

MSVOA_W

ClientSampleId :





Tgt Ion: 97 Resp: 127

Ion Ratio Lower Upper

97 100

99 0.0 51.2 76.8#

61 17.3 39.2 58.8#

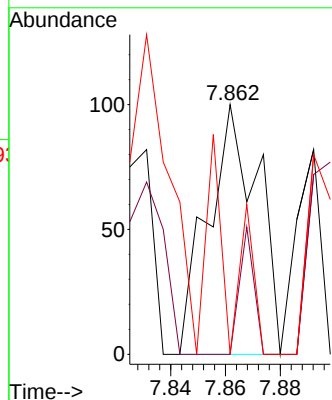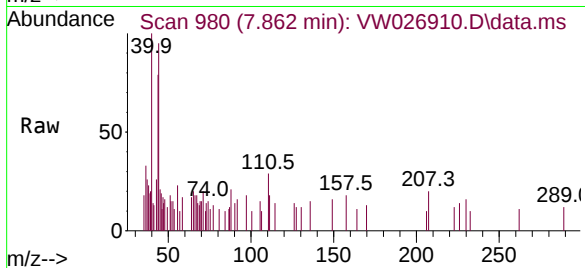

#35

Methylcyclohexane

Concen: 0.922 ug/L

RT: 9.349 min Scan# 1224

Delta R.T. 0.012 min

Lab File: VW026910.D

Acq: 25 Aug 2023 22:15




Tgt Ion: 83 Resp: 172


Ion Ratio Lower Upper

83 100

55 61.6 69.3 103.9#

98 22.7 37.4 56.0#

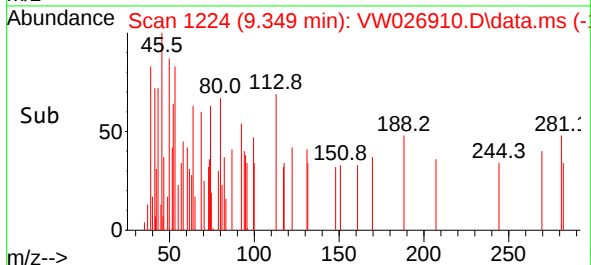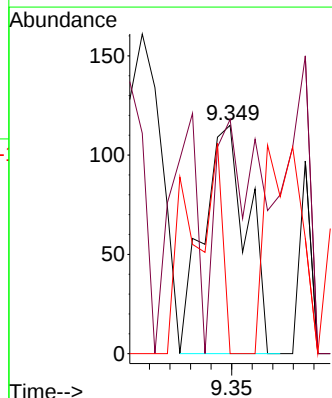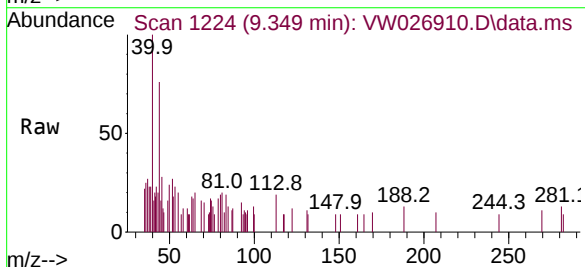

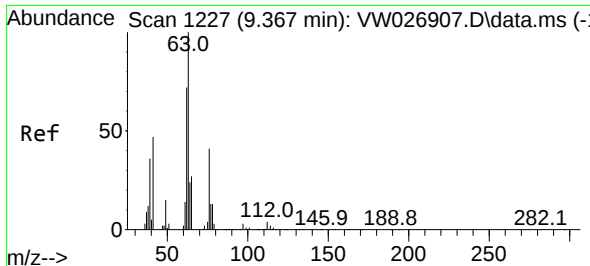

#37

1,2-Dichloropropane

Concen: 0.998 ug/L

RT: 9.367 min Scan# 117

Delta R.T. -0.000 min

Lab File: VW026910.D

Acq: 25 Aug 2023 22:15

Instrument :

MSVOA_W





ClientSampleId :

Tgt Ion: 63 Resp: 117

Ion Ratio Lower Upper

63 100

112 0.0 3.1 4.7#

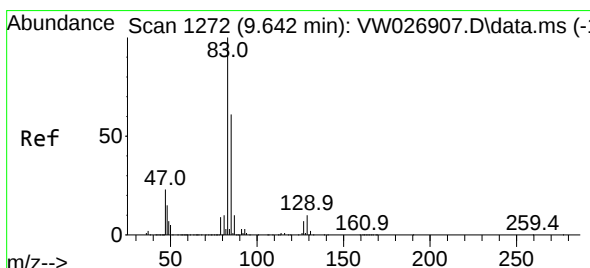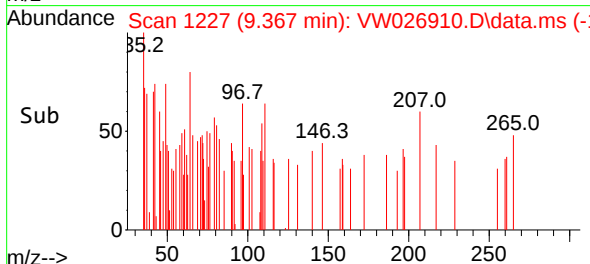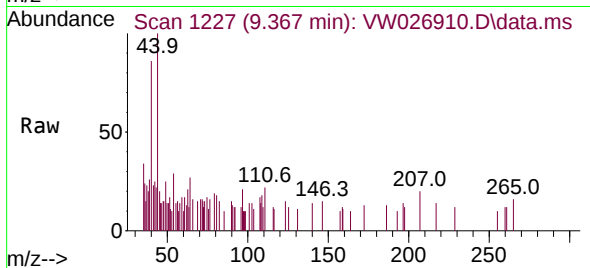

#38

Bromodichloromethane

Concen: 1.381 ug/L

RT: 9.624 min Scan# 1269

Delta R.T. -0.018 min

Lab File: VW026910.D

Acq: 25 Aug 2023 22:15




Tgt Ion: 83 Resp: 190


Ion Ratio Lower Upper

83 100

85 0.0 45.4 84.2#

127 0.0 6.2 9.2#

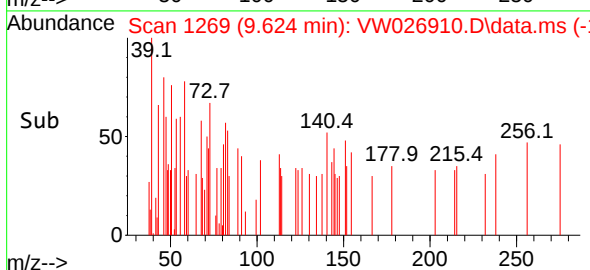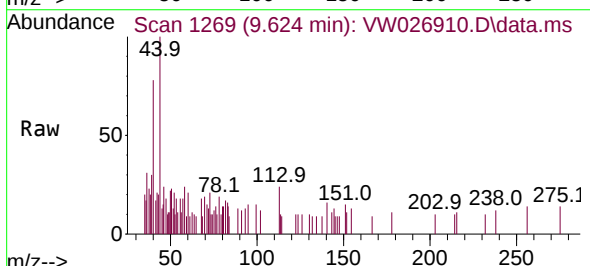



#39

cis-1,3-Dichloropropene

Concen: 0.700 ug/L

RT: 10.062 min Scan# 11

Delta R.T. -0.012 min

Lab File: VW026910.D

Acq: 25 Aug 2023 22:15

Instrument :

MSVOA_W





ClientSampleId :

Tgt Ion: 75 Resp: 118

Ion Ratio Lower Upper

75 100

77 41.2 22.8 42.4

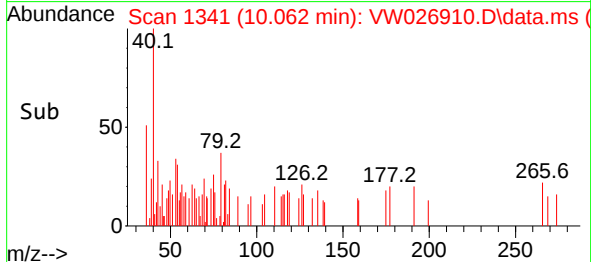

#40

4-Methyl-2-pentanone

Concen: 4.720 ug/L

RT: 10.221 min Scan# 1367

Delta R.T. 0.012 min

Lab File: VW026910.D

Acq: 25 Aug 2023 22:15




Tgt Ion: 43 Resp: 360


Ion Ratio Lower Upper

43 100

58 25.3 29.2 43.8#

100 0.0 10.7 16.1#

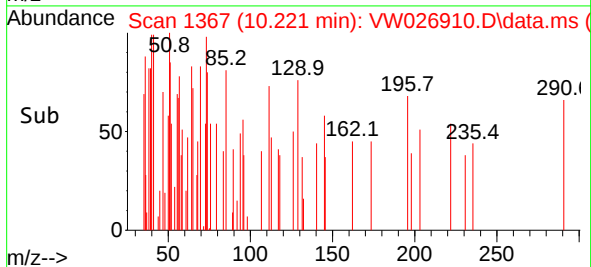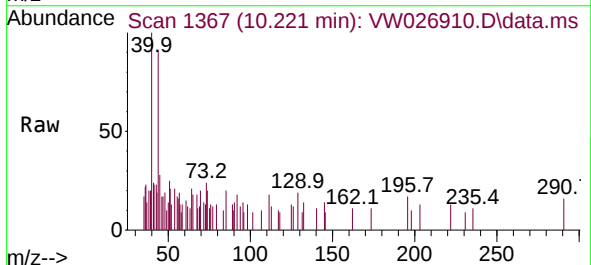



#44

trans-1,3-Dichloropropene

Concen: 0.895 ug/L

RT: 10.447 min Scan# 1404

Delta R.T. -0.159 min

Lab File: VW026910.D

Acq: 25 Aug 2023 22:15

Instrument :

MSVOA_W





ClientSampleId :

Tgt Ion: 75 Resp: 130

Ion Ratio Lower Upper

75 100

77 34.8 21.2 39.4

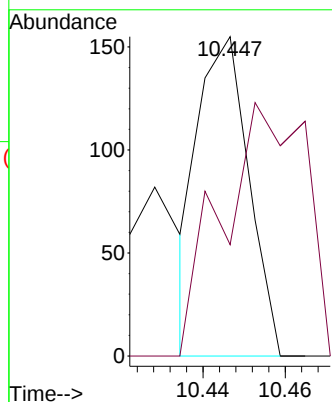

#45

1,1,2-Trichloroethane

Concen: 1.010 ug/L

RT: 10.800 min Scan# 1462

Delta R.T. 0.012 min

Lab File: VW026910.D

Acq: 25 Aug 2023 22:15

Tgt Ion: 97 Resp: 81




Ion Ratio Lower Upper


97 100

99 68.3 44.2 82.0

83 69.5 61.9 114.9


85 0.0 40.0 74.2#

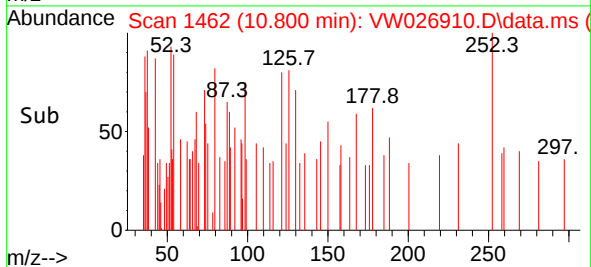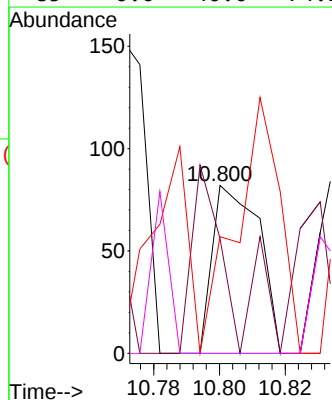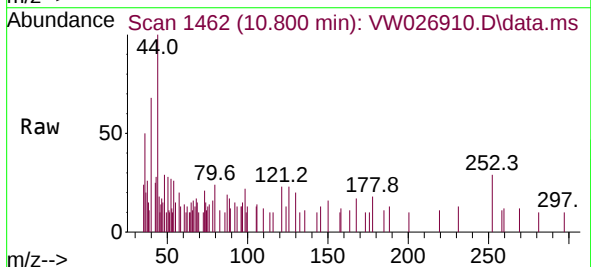






#46
Tetrachloroethene
Concen: 1.288 ug/L
RT: 10.861 min Scan# 1472
Delta R.T. -0.000 min
Lab File: VW026910.D
Acq: 25 Aug 2023 22:15

Instrument :
MSVOA_W
ClientSampleId :







Tgt Ion:	164	Resp:	102
Ion	Ratio	Lower	Upper
164	100		
129	44.4	68.1	126.5#
131	57.7	65.5	121.7#
166	126.8	89.1	165.5

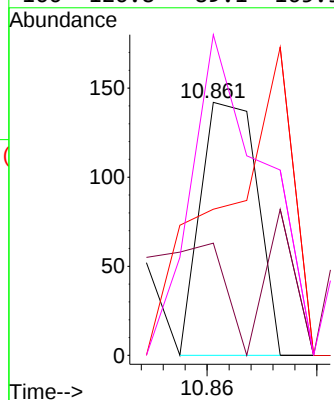

#48
2-Hexanone
Concen: 5.396 ug/L
RT: 10.959 min Scan# 1488
Delta R.T. -0.006 min
Lab File: VW026910.D
Acq: 25 Aug 2023 22:15

Tgt Ion:	43	Resp:	280
Ion	Ratio	Lower	Upper
43	100		
58	80.7	41.1	61.7#
57	32.9	14.3	21.5#
100	22.1	8.8	13.2#


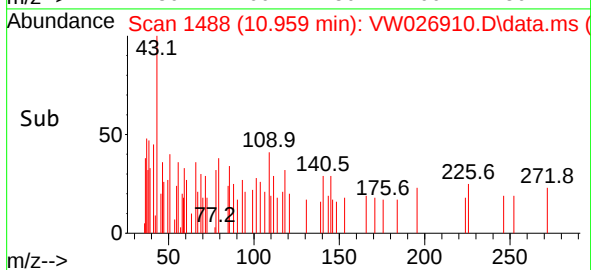
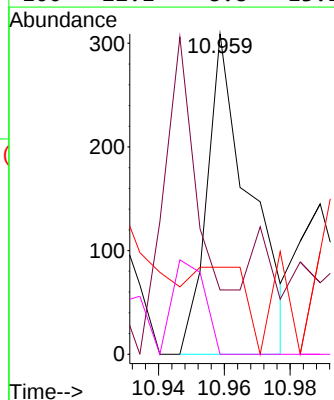





#50
1,2-Dibromoethane
Concen: 1.396 ug/L
RT: 11.251 min Scan# 11
Delta R.T. 0.018 min
Lab File: VW026910.D
Acq: 25 Aug 2023 22:15




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion:107 Resp: 105
Ion Ratio Lower Upper
107 100
109 65.9 68.8 127.8#
188 77.6 2.7 4.1#

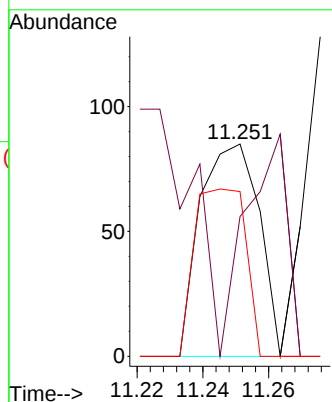

#57
1,1,2,2-Tetrachloroethane
Concen: 1.507 ug/L
RT: 12.727 min Scan# 1778
Delta R.T. 0.012 min
Lab File: VW026910.D
Acq: 25 Aug 2023 22:15


Tgt Ion: 83 Resp: 153
Ion Ratio Lower Upper
83 100
85 0.0 44.9 83.3#
131 63.0 7.4 11.0#

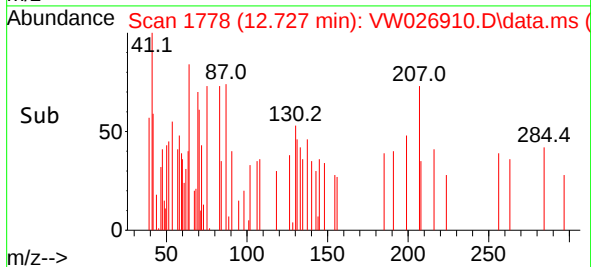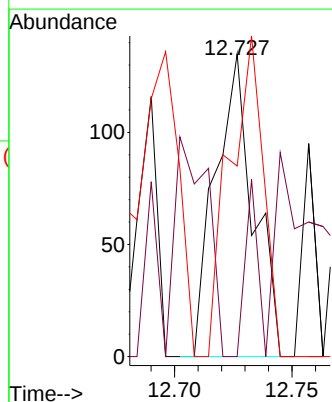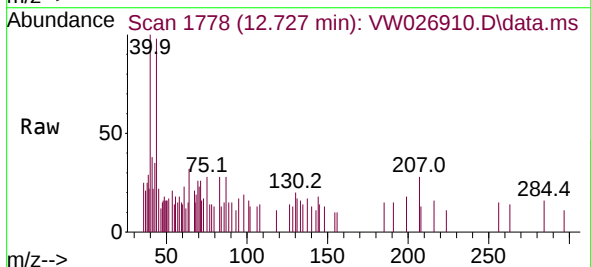






#59
Bromoform
Concen: 1.272 ug/L
RT: 12.501 min Scan# 1741
Delta R.T. 0.152 min
Lab File: VW026910.D
Acq: 25 Aug 2023 22:15

Instrument :
MSVOA_W
ClientSampleId :







Tgt Ion:173 Resp: 53
Ion Ratio Lower Upper
173 100
175 90.6 36.6 55.0#
254 0.0 7.8 11.6#

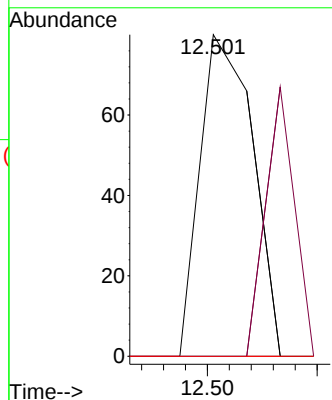

#61
1,2,3-Trichloropropane
Concen: 3.799 ug/L
RT: 12.763 min Scan# 1784
Delta R.T. -0.000 min
Lab File: VW026910.D
Acq: 25 Aug 2023 22:15

Tgt Ion: 75 Resp: 245
Ion Ratio Lower Upper
75 100
77 37.1 26.1 39.1
110 0.0 29.9 44.9#


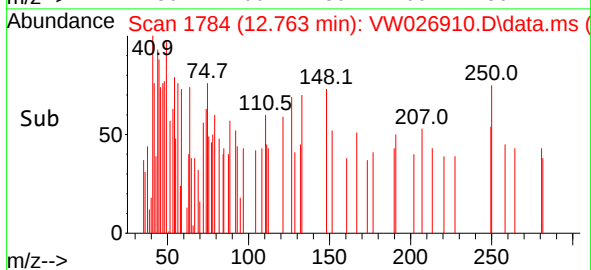
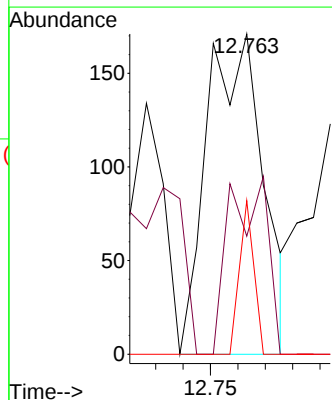





#63
1,2,4-Trimethylbenzene
Concen: 0.575 ug/L
RT: 13.251 min Scan# 1864
Delta R.T. 0.006 min
Lab File: VW026910.D
Acq: 25 Aug 2023 22:15




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion:105 Resp: 176
Ion Ratio Lower Upper
105 100
120 45.5 36.2 54.4

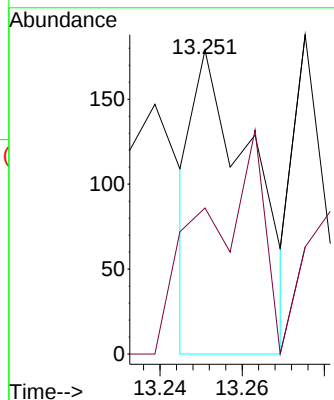

#64
1,3-Dichlorobenzene
Concen: 0.599 ug/L
RT: 13.495 min Scan# 1904
Delta R.T. -0.000 min
Lab File: VW026910.D
Acq: 25 Aug 2023 22:15

Tgt Ion:146 Resp: 103
Ion Ratio Lower Upper
146 100
111 103.7 29.1 54.1#
148 0.0 38.8 72.0#

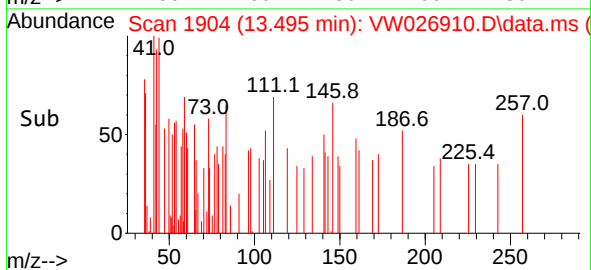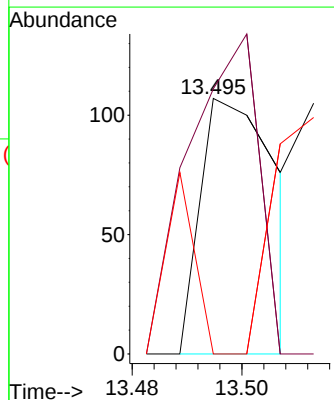



#65

1,4-Dichlorobenzene

Concen: 1.221 ug/L

RT: 13.574 min Scan# 1917

Delta R.T. -0.000 min

Lab File: VW026910.D

Acq: 25 Aug 2023 22:15

Instrument :

MSVOA_W

ClientSampleId :





Tgt Ion:146 Resp: 219

Ion Ratio Lower Upper

146 100

111 53.5 28.3 52.7#

148 49.0 44.2 82.2

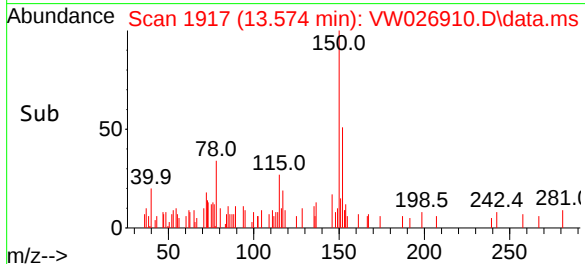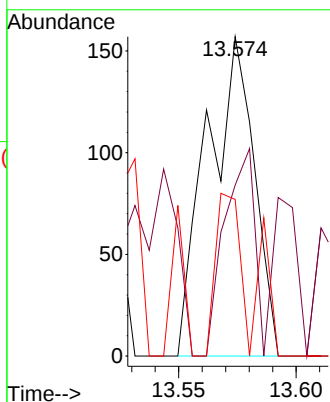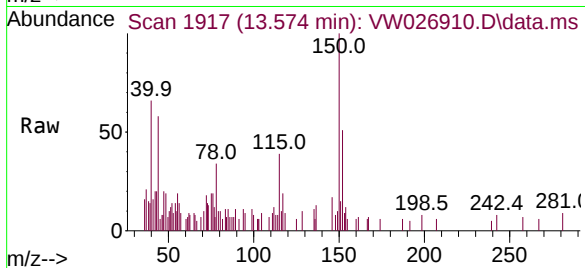

#67

1,2-Dichlorobenzene

Concen: 0.672 ug/L

RT: 13.873 min Scan# 1966

Delta R.T. 0.006 min

Lab File: VW026910.D

Acq: 25 Aug 2023 22:15




Tgt Ion:146 Resp: 105


Ion Ratio Lower Upper

146 100

111 114.5 34.6 52.0#

148 0.0 53.4 80.0#

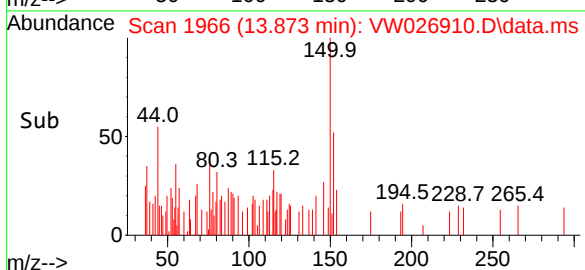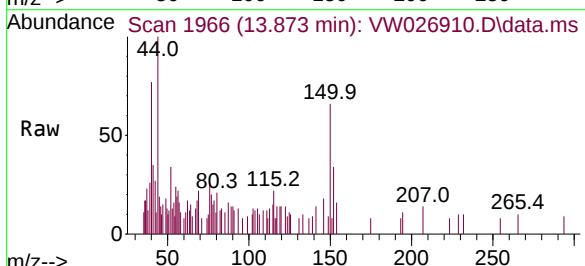



#69

1,3,5-Trichlorobenzene

Concen: 0.646 ug/L

RT: 14.610 min Scan# 2089

Delta R.T. -0.012 min


Lab File: VW026910.D

Acq: 25 Aug 2023 22:15

Instrument :

MSVOA_W

ClientSampleId :

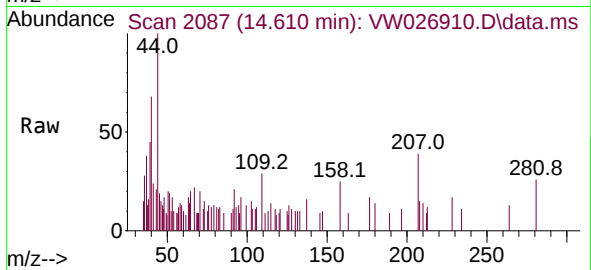

Tgt Ion:180 Resp: 75




Ion Ratio Lower Upper

180 100

182 0.0 75.2 112.8#

184 29.3 23.8 35.8

145 0.0 25.1 37.7#

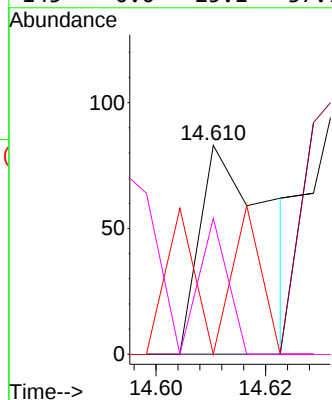

#71

Naphthalene

Concen: 1.347 ug/L

RT: 15.373 min Scan# 2212

Delta R.T. 0.012 min

Lab File: VW026910.D

Acq: 25 Aug 2023 22:15




Tgt Ion:128 Resp: 253


Ion Ratio Lower Upper

128 100

127 28.9 10.7 16.1#


129 45.5 9.0 13.4#

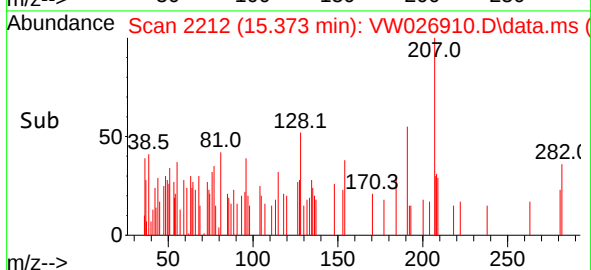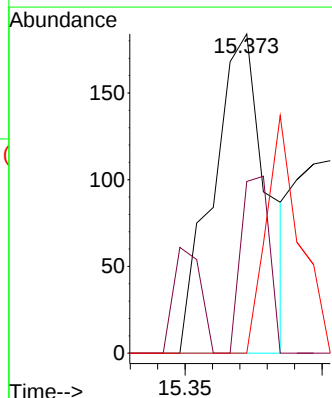



#72
 1,2,3-Trichlorobenzene
 Concen: 0.991 ug/L
 RT: 15.555 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: VW026910.D
 Acq: 25 Aug 2023 22:15

Instrument :
 MSVOA_W
 ClientSampleId :

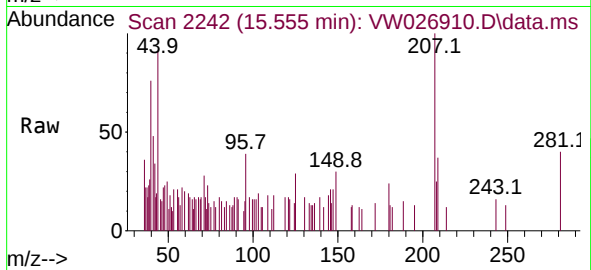

Tgt Ion:180 Resp: 88
 Ion Ratio Lower Upper
 180 100
 182 0.0 74.6 112.0#
 145 44.3 27.0 40.6#

