




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082523\
 Data File : VW026891.D
 Acq On : 25 Aug 2023 13:30
 Operator : SY/MD
 Sample : 04157-07
 Misc : 6.20g/10mL/MSVOA_W/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCHU3

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/28/2023
 Supervised By :Mahesh Dadoda 08/28/2023

Quant Time: Aug 26 01:46:17 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 26 01:43:45 2023
 Response via : Initial Calibration

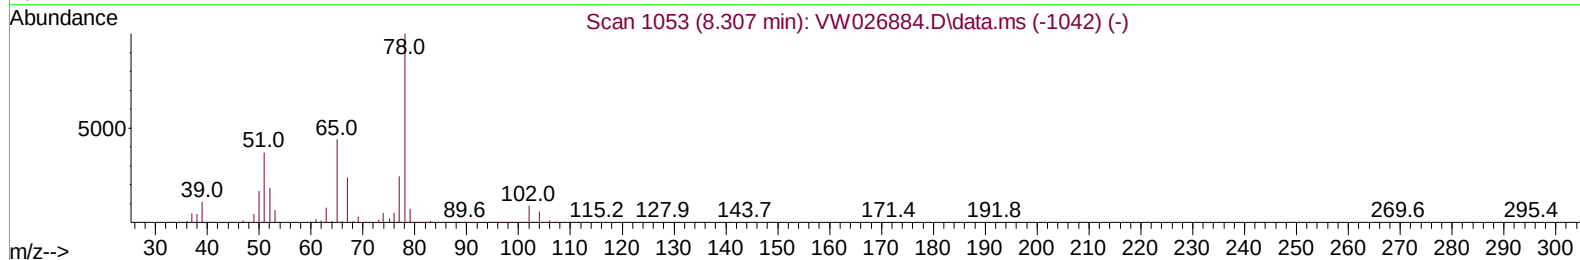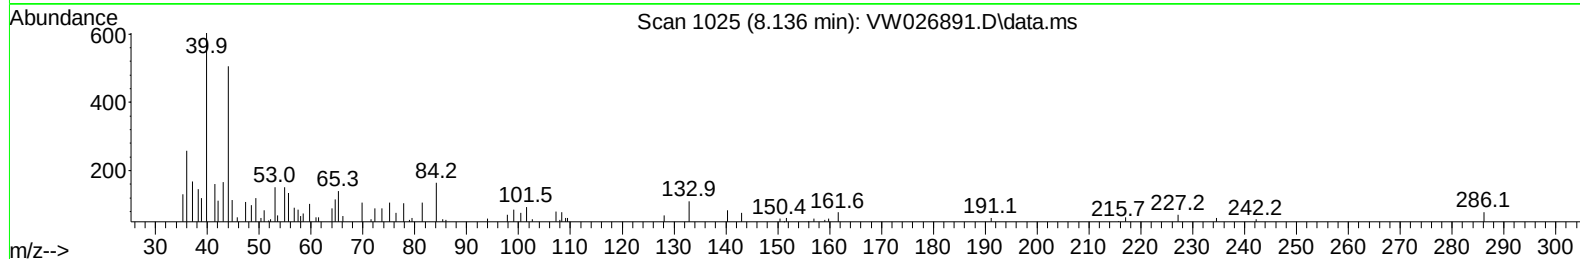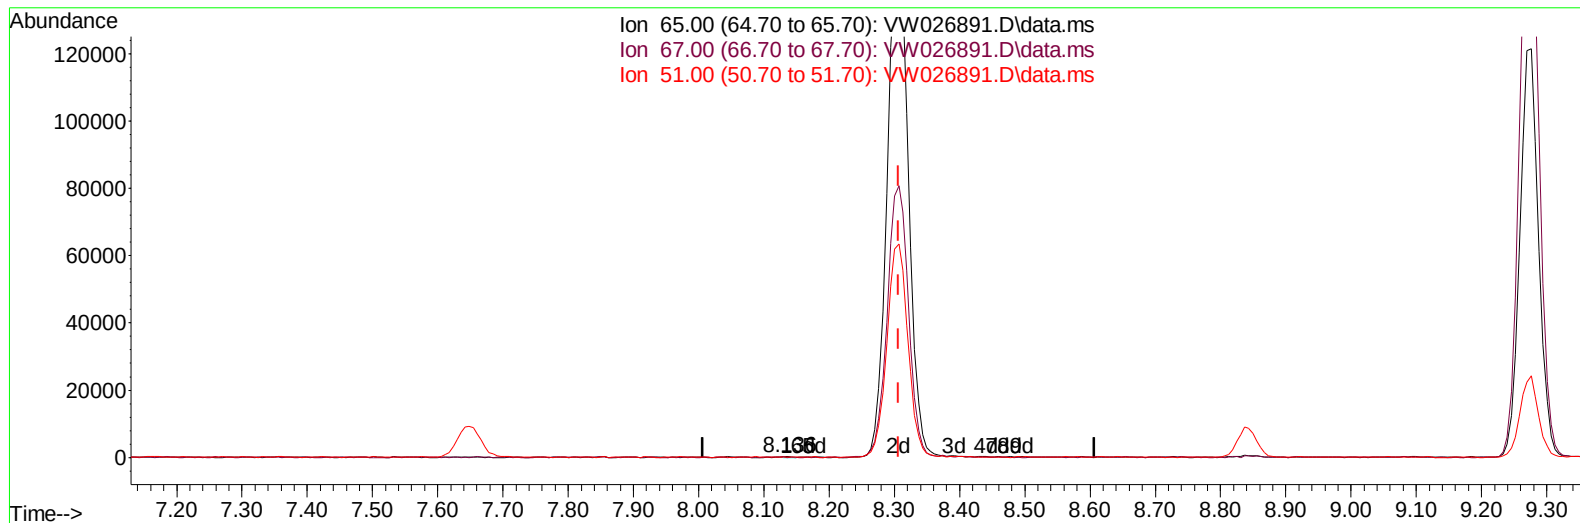

TIC: VW026891.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.136min (-0.171) 0.01 ug/L

response 119

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.60	51.26
51.00	112.90	87.39
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082523\
 Data File : VW026891.D
 Acq On : 25 Aug 2023 13:30
 Operator : SY/MD
 Sample : 04157-07
 Misc : 6.20g/10mL/MSVOA_W/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCHU3

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/28/2023
 Supervised By :Mahesh Dadoda 08/28/2023

Quant Time: Aug 26 01:46:17 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 26 01:43:45 2023
 Response via : Initial Calibration

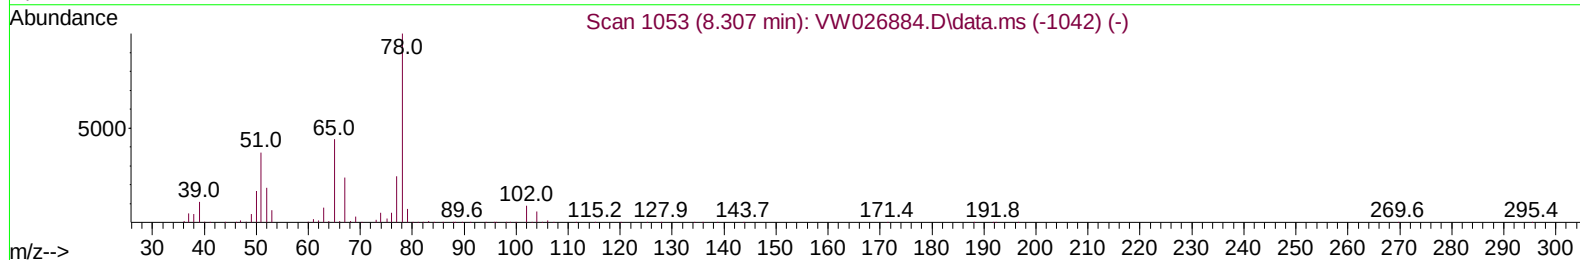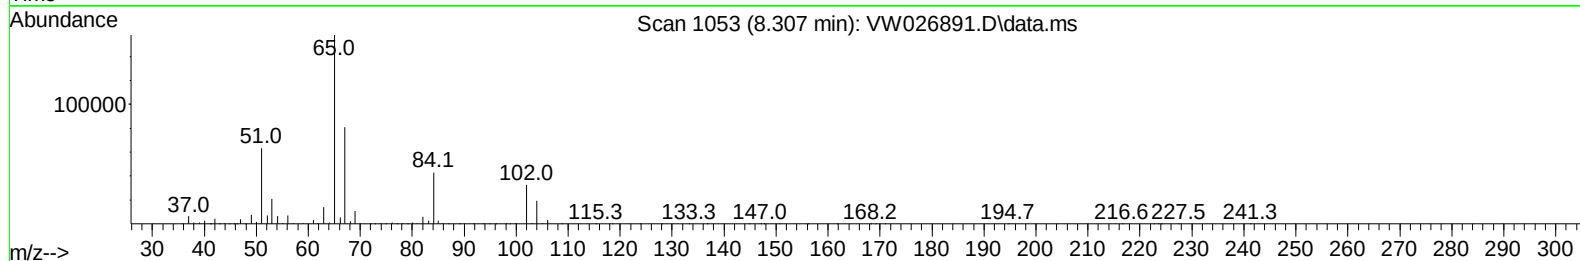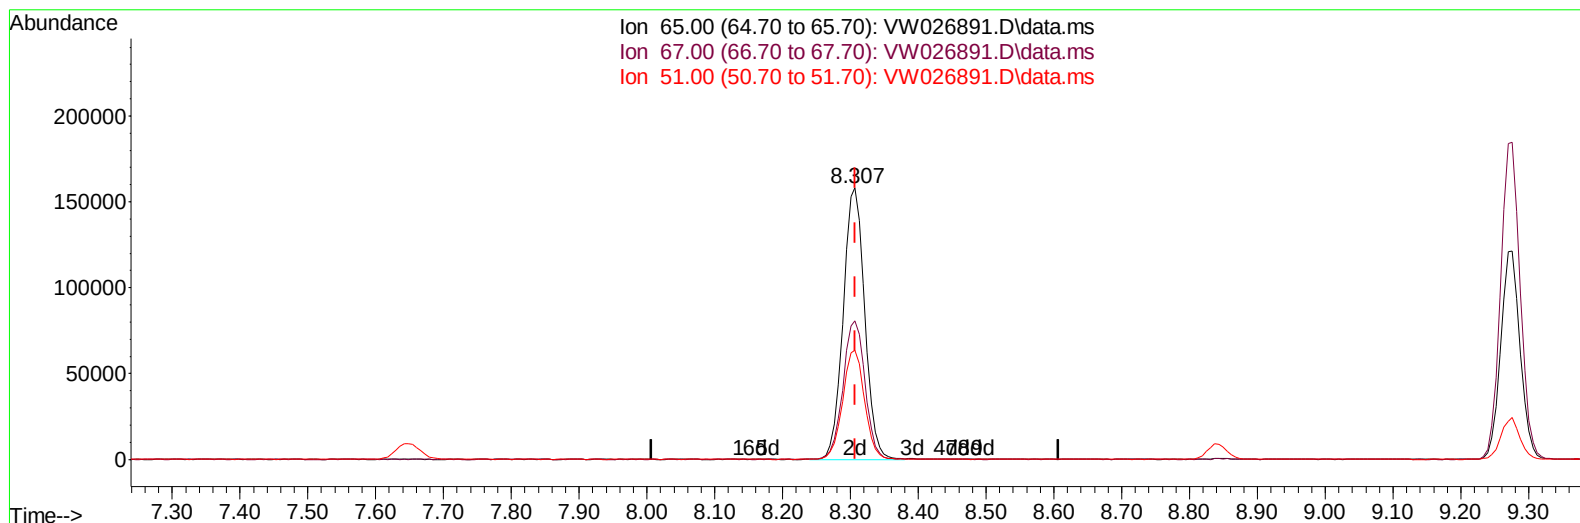

TIC: VW026891.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (-0.000) 23.45 ug/L m

response 349041

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.60	0.02#
51.00	112.90	0.03#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082523\
 Data File : VW026891.D
 Acq On : 25 Aug 2023 13:30
 Operator : SY/MD
 Sample : 04157-07
 Misc : 6.20g/10mL/MSVOA_W/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCHU3

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/28/2023
 Supervised By :Mahesh Dadoda 08/28/2023

Quant Time: Aug 26 01:46:17 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 26 01:43:45 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	803603	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	744852	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	352748	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	185943	14.076	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	56.320%	
7) Chloroethane-d5	2.899	69	164661	16.762	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	67.040%	
11) 1,1-Dichloroethene-d2	4.027	65	100960	15.539	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	62.160%	
21) 2-Butanone-d5	7.075	46	261259	68.808	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	137.620%#	
24) Chloroform-d	7.648	84	557750	20.680	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	82.720%	
26) 1,2-Dichloroethane-d4	8.307	65	349041m	23.451	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	93.800%	
32) Benzene-d6	8.276	84	1039723	20.254	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	81.000%	
36) 1,2-Dichloropropane-d6	9.276	67	371392	23.226	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	92.920%	
41) Toluene-d8	10.325	98	832888	18.901	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	75.600%	
43) trans-1,3-Dichloroprop...	10.574	79	139503	21.130	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	84.520%	
47) 2-Hexanone-d5	10.922	63	125296	74.572	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	149.140%#	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	375151	29.708	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	118.840%	
66) 1,2-Dichlorobenzene-d4	13.848	152	298620	23.652	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	94.600%	
Target Compounds						
16) Methylene chloride	4.923	84	50454	3.246	ug/L	96
19) 1,1-Dichloroethane	6.216	63	220729	8.091	ug/L	99
20) cis-1,2-Dichloroethene	7.167	96	22063	1.549	ug/L	96
46) Tetrachloroethene	10.861	164	30234	3.012	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082523\
Data File : VW026891.D
Acq On : 25 Aug 2023 13:30
Operator : SY/MD
Sample : 04157-07
Misc : 6.20g/10mL/MSVOA_W/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCHU3

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/28/2023
Supervised By :Mahesh Dadoda 08/28/2023

Quant Time: Aug 26 01:46:17 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Aug 26 01:43:45 2023
Response via : Initial Calibration

