




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082523\
 Data File : VW026900.D
 Acq On : 25 Aug 2023 17:07
 Operator : SY/MD
 Sample : 04157-17
 Misc : 5.78g/10mL/MSVOA_W/SOIL
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCHV6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/28/2023
 Supervised By :Mahesh Dadoda 08/28/2023

Quant Time: Aug 26 01:48:34 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 26 01:43:45 2023
 Response via : Initial Calibration

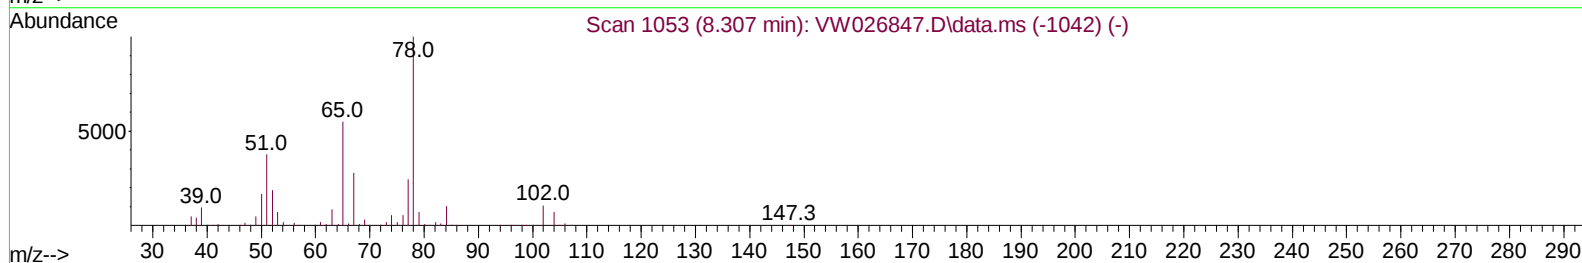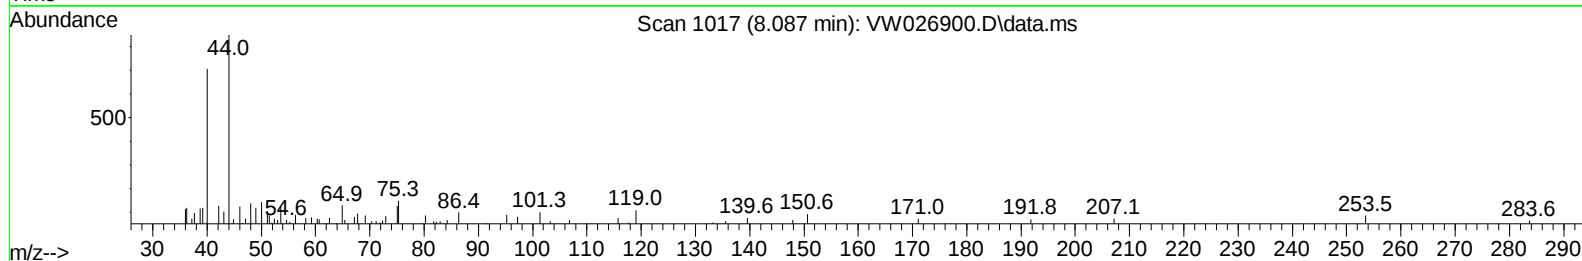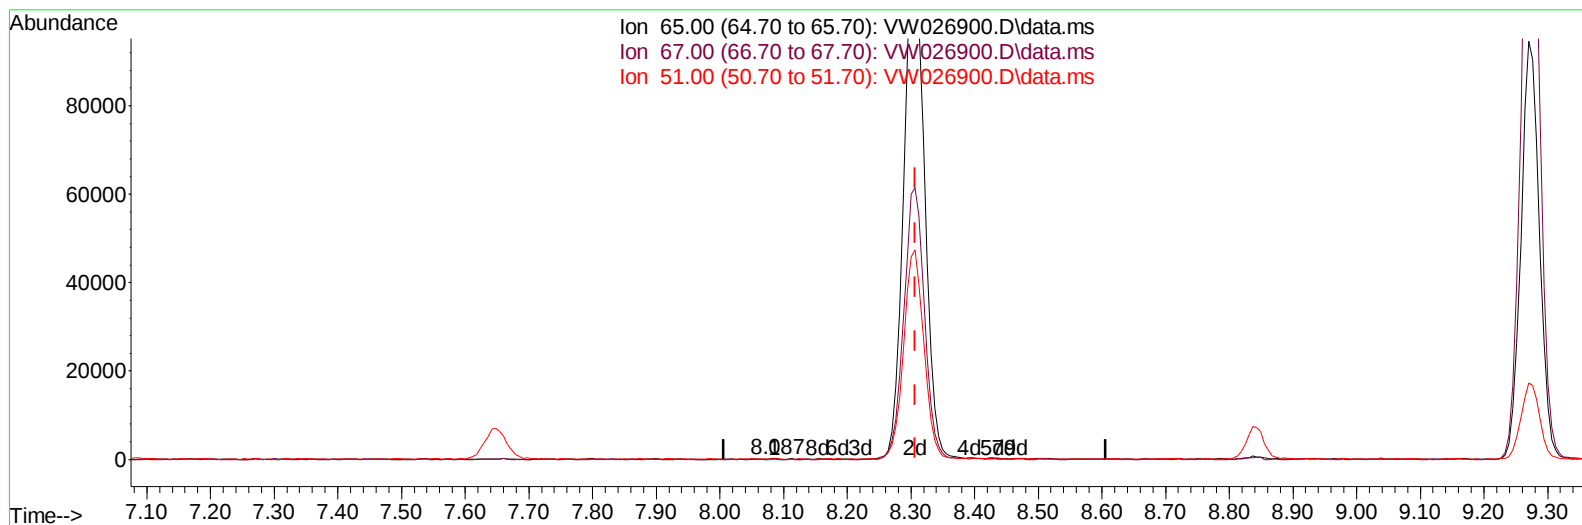

TIC: VW026900.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.087min (-0.219) 0.01 ug/L

response 183

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.60	61.75
51.00	112.90	128.42
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082523\
 Data File : VW026900.D
 Acq On : 25 Aug 2023 17:07
 Operator : SY/MD
 Sample : 04157-17
 Misc : 5.78g/10mL/MSVOA_W/SOIL
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCHV6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/28/2023
 Supervised By :Mahesh Dadoda 08/28/2023

Quant Time: Aug 26 01:48:34 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 26 01:43:45 2023
 Response via : Initial Calibration

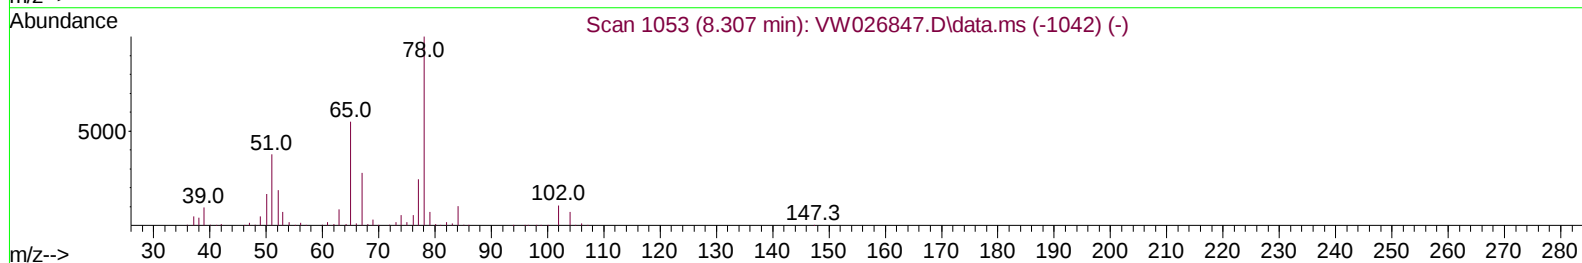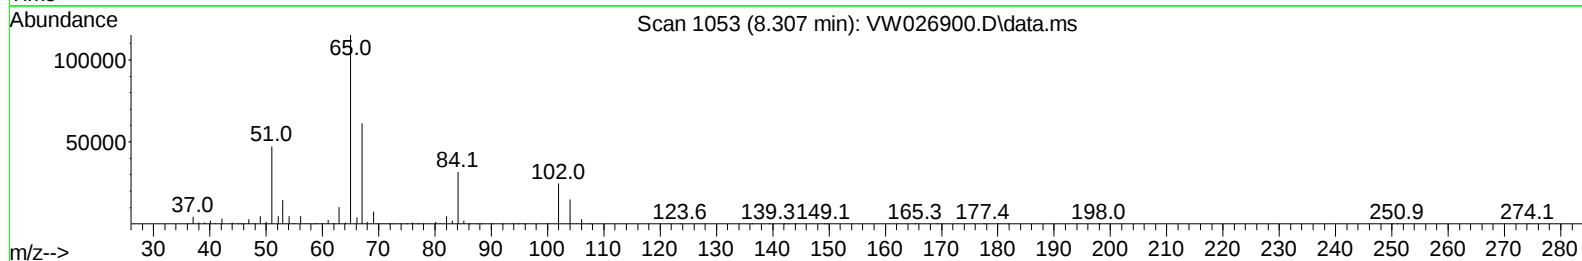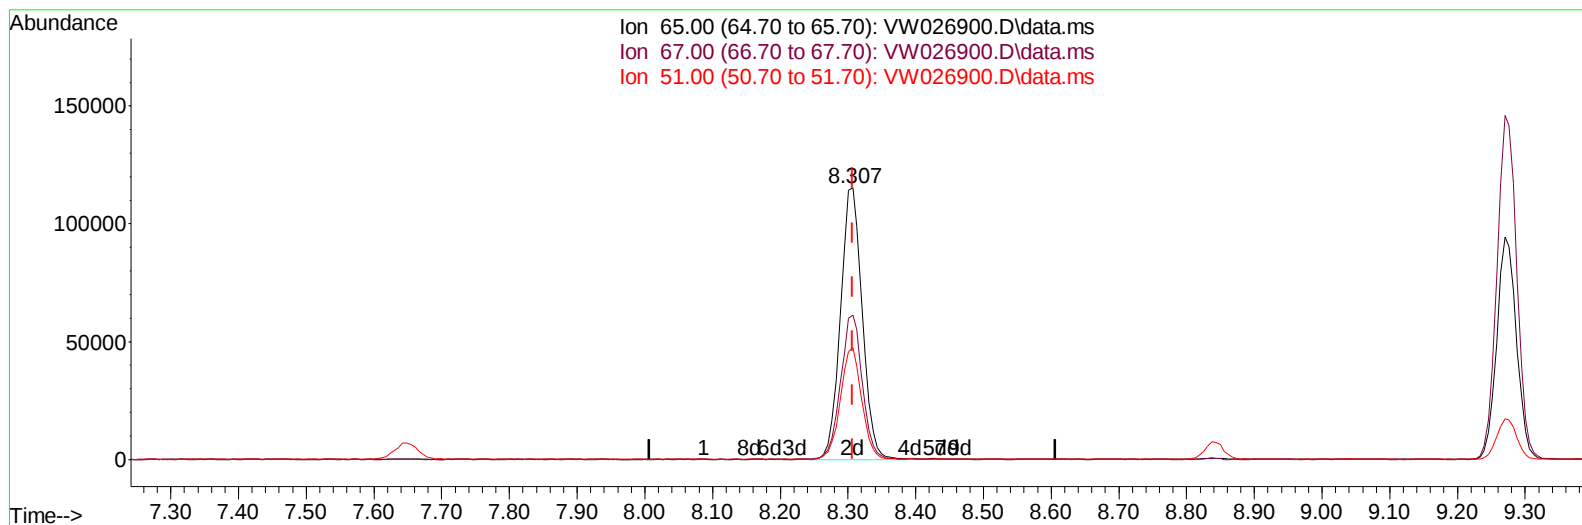

TIC: VW026900.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (+ 0.000) 21.05 ug/L m

response 257438

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.60	0.04#
51.00	112.90	0.09#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082523\
 Data File : VW026900.D
 Acq On : 25 Aug 2023 17:07
 Operator : SY/MD
 Sample : 04157-17
 Misc : 5.78g/10mL/MSVOA_W/SOIL
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCHV6

Manual IntegrationsAPPROVED

Quant Time: Aug 26 01:48:34 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 26 01:43:45 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/28/2023
 Supervised By :Mahesh Dadoda 08/28/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		660442	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		660007	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		335057	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.357	65		136668	12.588	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	50.360%		
7) Chloroethane-d5	2.893	69		125676	15.567	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	62.280%		
11) 1,1-Dichloroethene-d2	4.015	65		74648	13.980	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	55.920%		
21) 2-Butanone-d5	7.075	46		170098	54.510	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	109.020%		
24) Chloroform-d	7.648	84		432457	19.510	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	78.040%		
26) 1,2-Dichloroethane-d4	8.307	65		257438m	21.045	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	84.200%		
32) Benzene-d6	8.270	84		824284	18.121	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	72.480%		
36) 1,2-Dichloropropane-d6	9.270	67		294885	20.812	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	83.240%		
41) Toluene-d8	10.325	98		683541	17.506	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	70.040%		
43) trans-1,3-Dichloroprop...	10.575	79		108105	18.479	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	73.920%		
47) 2-Hexanone-d5	10.922	63		81734	54.899	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	109.800%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		279078	24.941	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	99.760%		
66) 1,2-Dichlorobenzene-d4	13.848	152		262236	21.867	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	87.480%		
Target Compounds							
16) Methylene chloride	4.923	84		48948	3.831	ug/L	Qvalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082523\
Data File : VW026900.D
Acq On : 25 Aug 2023 17:07
Operator : SY/MD
Sample : 04157-17
Misc : 5.78g/10mL/MSVOA_W/SOIL
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCHV6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/28/2023
Supervised By :Mahesh Dadoda 08/28/2023

Quant Time: Aug 26 01:48:34 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Aug 26 01:43:45 2023
Response via : Initial Calibration

