




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082523\
 Data File : VW026909.D
 Acq On : 25 Aug 2023 21:51
 Operator : SY/MD
 Sample : 04157-23
 Misc : 6.21g/10mL/MSVOA_W/SOIL
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCHW2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/28/2023
 Supervised By :Mahesh Dadoda 08/28/2023

Quant Time: Aug 28 01:04:38 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 26 05:14:45 2023
 Response via : Initial Calibration

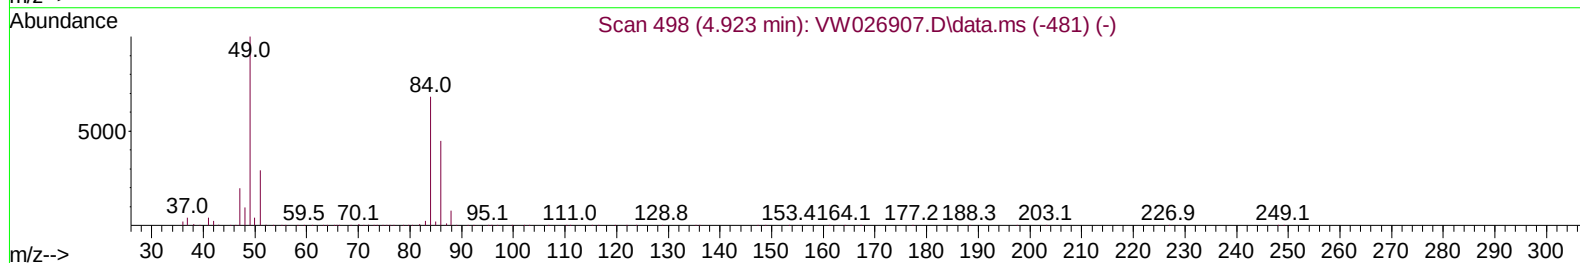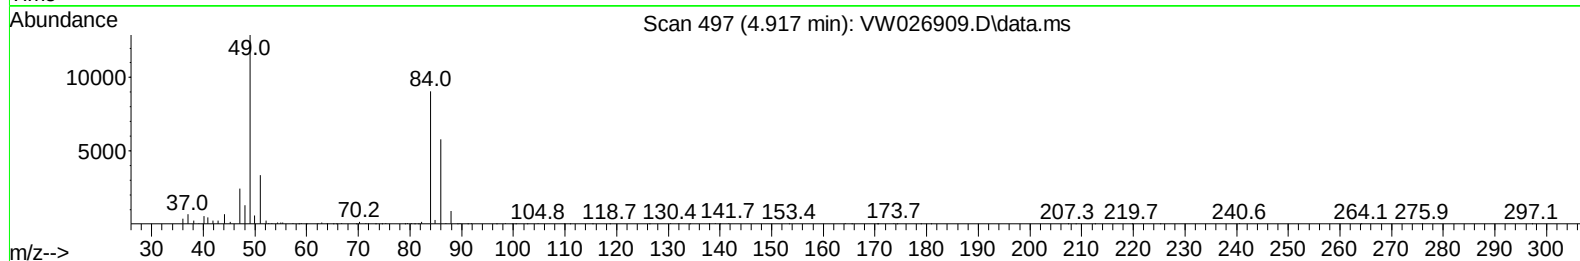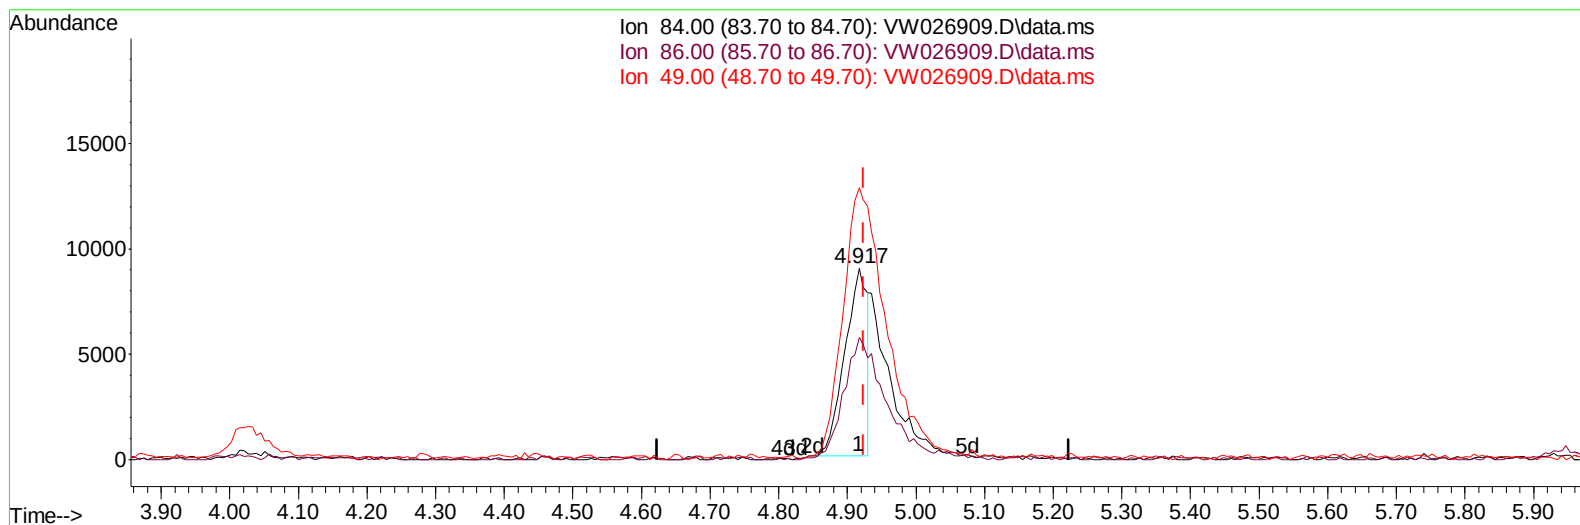

TIC: VW026909.D\data.ms

(16) Methylene chloride (T)

4.917min (-0.006) 1.84 ug/L

response 20151

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.20	63.81
49.00	137.10	142.07
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082523\
 Data File : VW026909.D
 Acq On : 25 Aug 2023 21:51
 Operator : SY/MD
 Sample : 04157-23
 Misc : 6.21g/10mL/MSVOA_W/SOIL
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCHW2

Manual IntegrationsAPPROVED

Quant Time: Aug 28 01:04:38 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 26 05:14:45 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/28/2023
 Supervised By :Mahesh Dadoda 08/28/2023

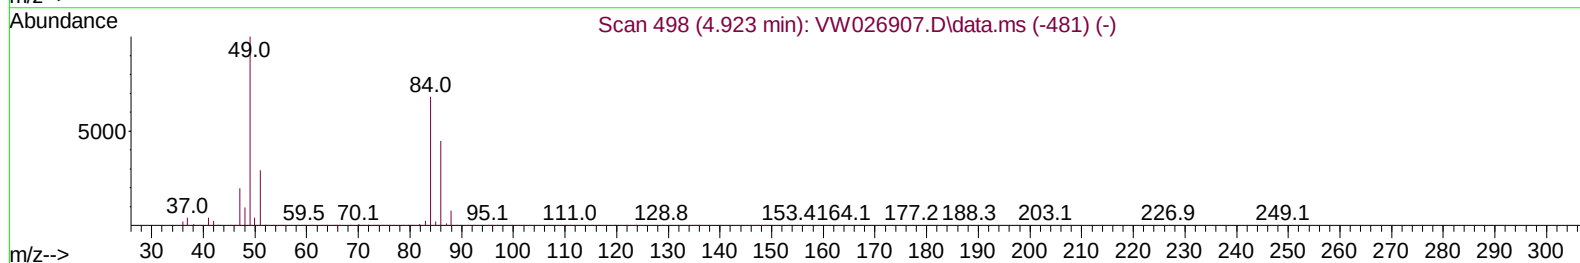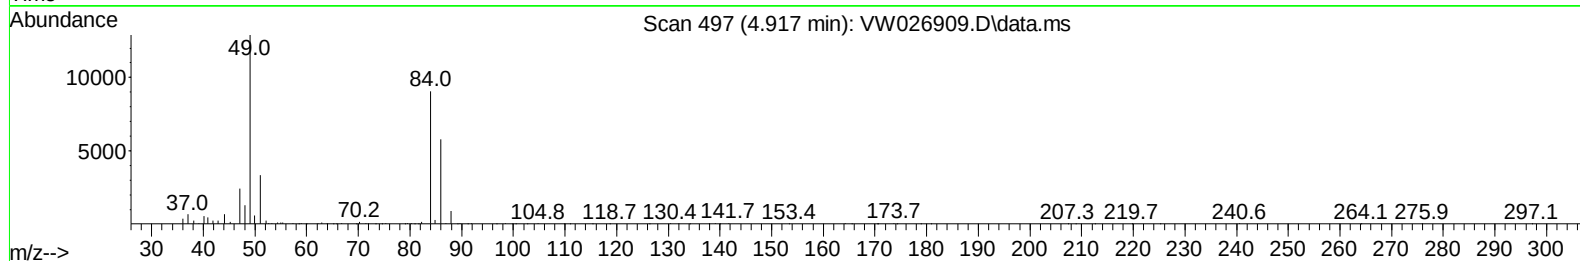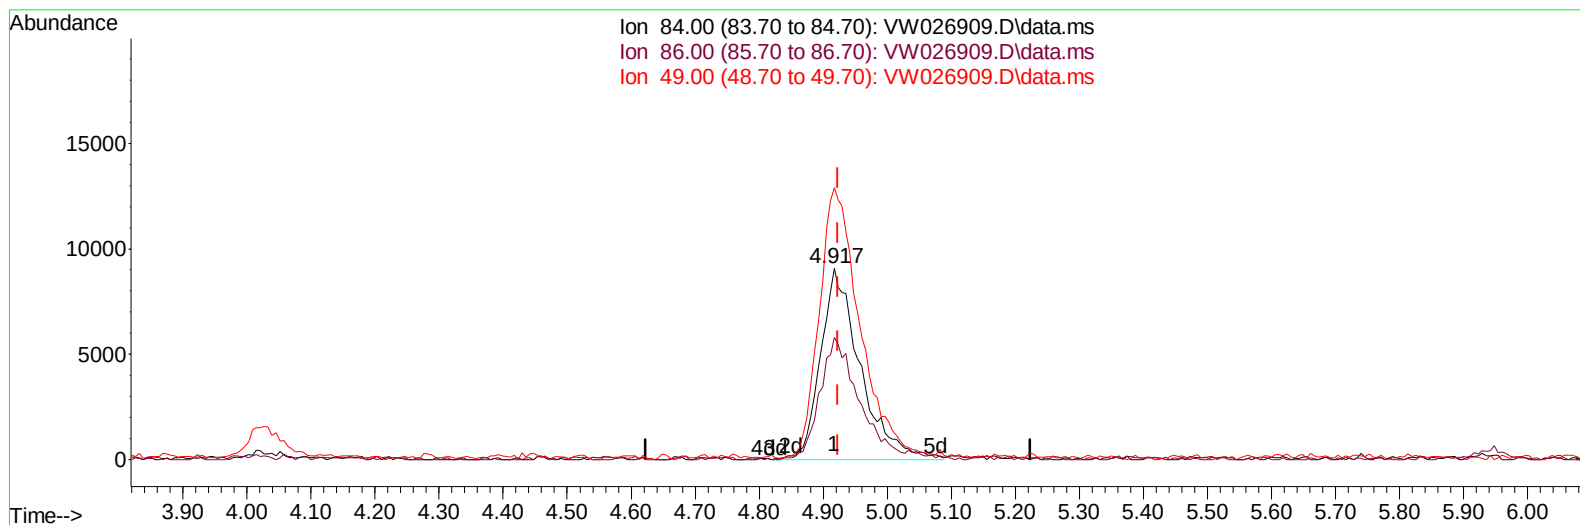

TIC: VW026909.D\data.ms

(16) Methylene chloride (T)

4.917min (-0.006) 3.56 ug/L m

response 38973

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.20	63.81
49.00	137.10	142.07
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082523\
 Data File : VW026909.D
 Acq On : 25 Aug 2023 21:51
 Operator : SY/MD
 Sample : 04157-23
 Misc : 6.21g/10mL/MSVOA_W/SOIL
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCHW2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/28/2023
 Supervised By :Mahesh Dadoda 08/28/2023

Quant Time: Aug 28 01:04:38 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 26 05:14:45 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.837	114		565305	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		553904	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		291452	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		103514	11.139	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	44.560%		
7) Chloroethane-d5	2.893	69		94487	13.673	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	54.680%		
11) 1,1-Dichloroethene-d2	4.021	65		58780	12.861	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	51.440%		
21) 2-Butanone-d5	7.075	46		124256	46.521	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	93.040%		
24) Chloroform-d	7.642	84		353642	18.639	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	74.560%		
26) 1,2-Dichloroethane-d4	8.307	65		215344	20.567	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	82.280%		
32) Benzene-d6	8.270	84		650671	17.045	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	68.160%		
36) 1,2-Dichloropropane-d6	9.270	67		230420	19.378	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	77.520%		
41) Toluene-d8	10.325	98		535222	16.333	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	65.320%		
43) trans-1,3-Dichloroprop...	10.575	79		84449	17.201	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	68.800%		
47) 2-Hexanone-d5	10.922	63		55603	44.501	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	89.000%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		199907	21.288	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	85.160%		
66) 1,2-Dichlorobenzene-d4	13.848	152		207664	19.907	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	79.640%		
Target Compounds							
16) Methylene chloride	4.917	84		38973m	3.564	ug/L	
46) Tetrachloroethene	10.855	164		9604	1.287	ug/L	86

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082523\
Data File : VW026909.D
Acq On : 25 Aug 2023 21:51
Operator : SY/MD
Sample : 04157-23
Misc : 6.21g/10mL/MSVOA_W/SOIL
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCHW2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/28/2023
Supervised By :Mahesh Dadoda 08/28/2023

Quant Time: Aug 28 01:04:38 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Aug 26 05:14:45 2023
Response via : Initial Calibration

