


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW082619\
 Data File : VW012158.D
 Acq On : 26 Aug 2019 08:38
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W082319S.M
 Title : SW846 8260
 Last Update : Mon Aug 26 07:18:31 2019

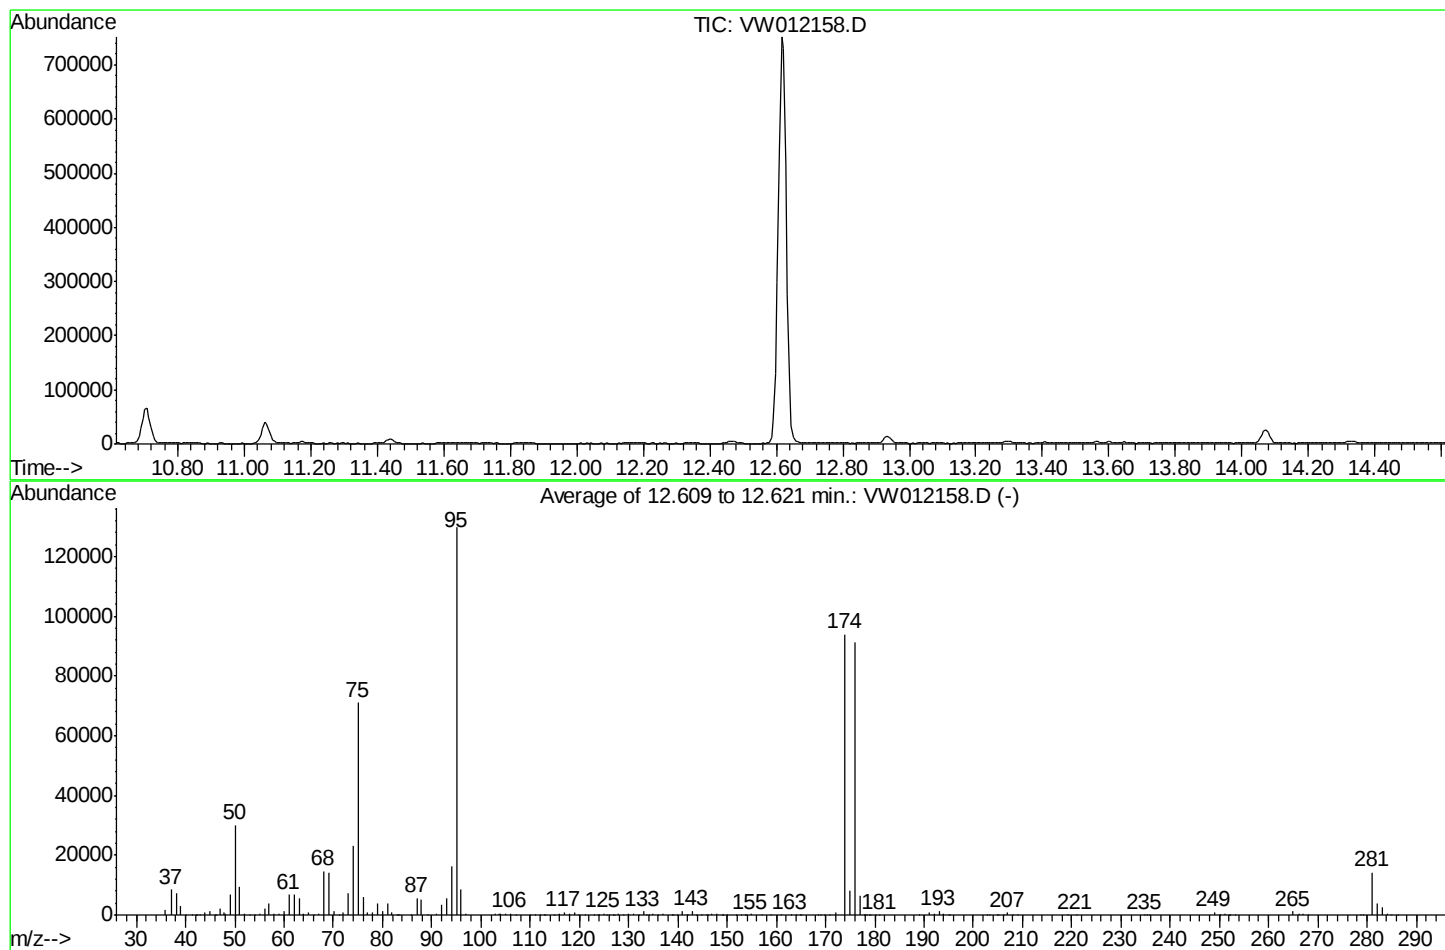

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.1	30037	PASS
75	95	30	60	54.8	71165	PASS
95	95	100	100	100.0	129848	PASS
96	95	5	9	6.7	8679	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	72.3	93922	PASS
175	174	5	9	8.5	7955	PASS
176	174	95	101	97.0	91144	PASS
177	176	5	9	7.1	6461	PASS