
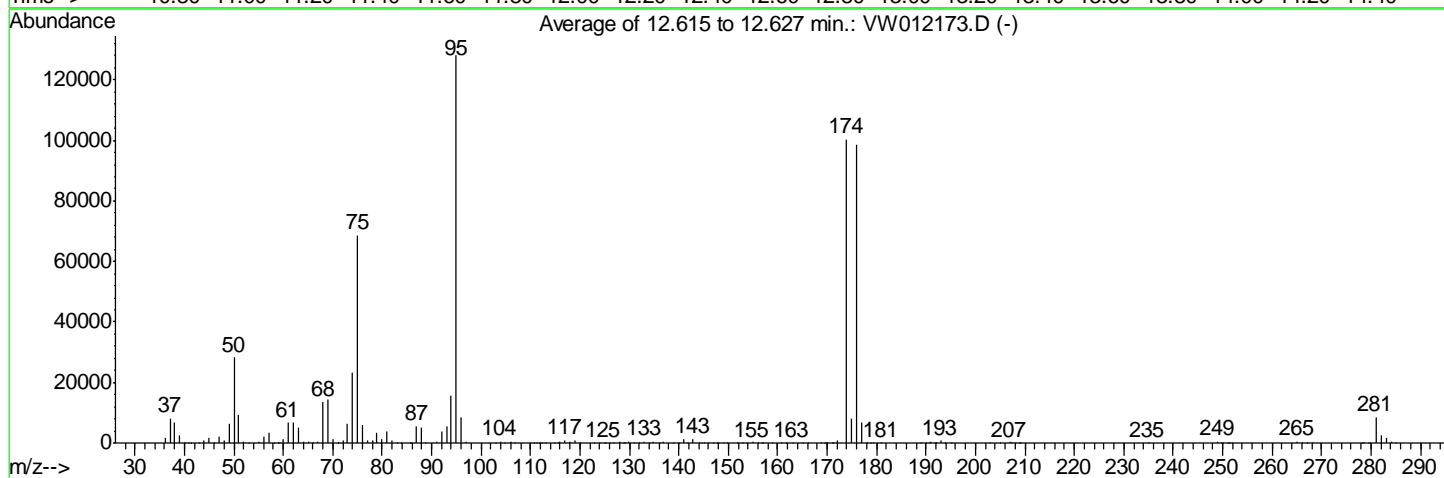


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW082619\  
 Data File : VW012173.D  
 Acq On : 26 Aug 2019 15:40  
 Operator : SY/VA  
 Sample : BFB  
 Misc : 5.00G/5ML/MSVOA W/SOIL  
 ALS Vial : 16 Sample Multiplier: 1

Instrument :  
 MSVOA\_W  
 ClientSampled :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_W\METHOD\82W082319S.M  
 Title : SW846 8260  
 Last Update : Mon Aug 26 07:18:31 2019

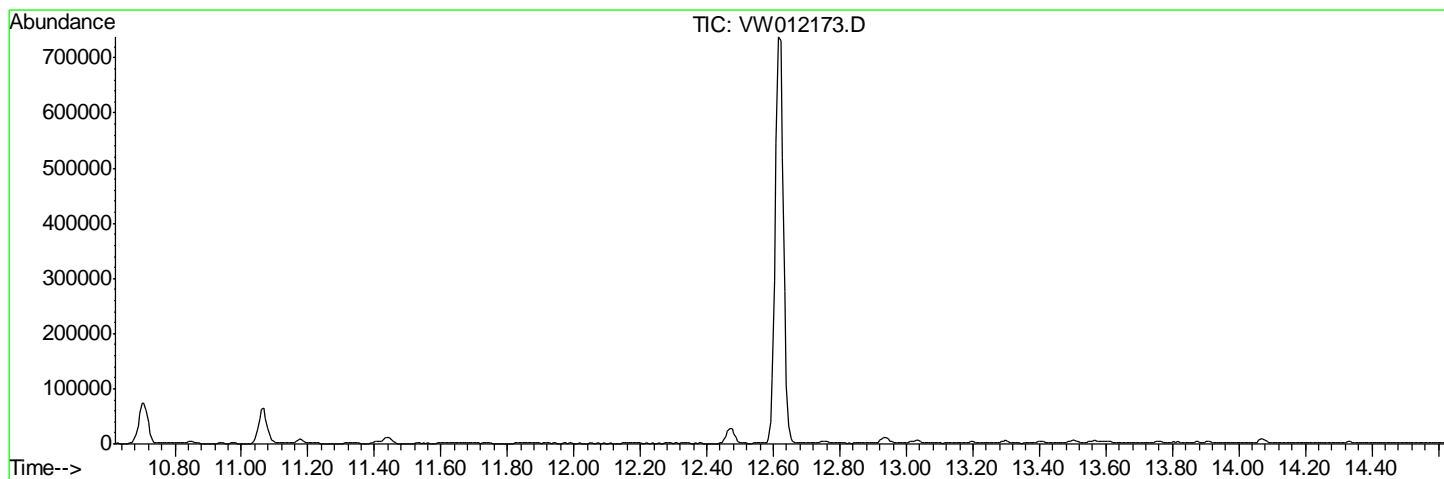

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1747

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.0	28200	PASS
75	95	30	60	53.5	68600	PASS
95	95	100	100	100.0	128122	PASS
96	95	5	9	6.5	8266	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	78.3	100346	PASS
175	174	5	9	8.0	8071	PASS
176	174	95	101	98.4	98704	PASS
177	176	5	9	6.8	6673	PASS