

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
 Data File : VW024423.D
 Acq On : 28 Aug 2022 01:20
 Operator : SY/VA
 Sample : N4363-20
 Misc : 5.46g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Aug 29 05:01:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Aug 29 04:56:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	199899	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117	211084	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	84785	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	107140	19.443	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	77.760%	
7) Chloroethane-d5	2.873	69	72542	17.570	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	70.280%	
11) 1,1-Dichloroethene-d2	4.007	63	67741	14.175	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	56.680%	
21) 2-Butanone-d5	7.073	46	39729	39.144	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	78.280%	
24) Chloroform-d	7.640	84	115279	17.938	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	71.760%	
26) 1,2-Dichloroethane-d4	8.573	65	121	0.031	ug/L	0.27
Spiked Amount 25.000	Range 70	- 130	Recovery	=	0.120%#	
32) Benzene-d6	8.268	84	216524	17.903	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	71.600%	
36) 1,2-Dichloropropane-d6	9.268	67	66878	17.781	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	71.120%	
41) Toluene-d8	10.323	98	207550	18.050	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	72.200%	
43) trans-1,3-Dichloroprop...	10.573	79	25611	14.551	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	58.200%	
47) 2-Hexanone-d5	10.920	63	30800	36.593	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	73.180%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	68218	16.020	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	64.080%	
66) 1,2-Dichlorobenzene-d4	13.853	152	63916	20.019	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	80.080%	
Target Compounds						
46) Tetrachloroethene	10.859	164	27362	10.171	ug/L	Qvalue 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
Data File : VW024423.D
Acq On : 28 Aug 2022 01:20
Operator : SY/VA
Sample : N4363-20
Misc : 5.46g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Aug 29 05:01:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Aug 29 04:56:06 2022
Response via : Initial Calibration

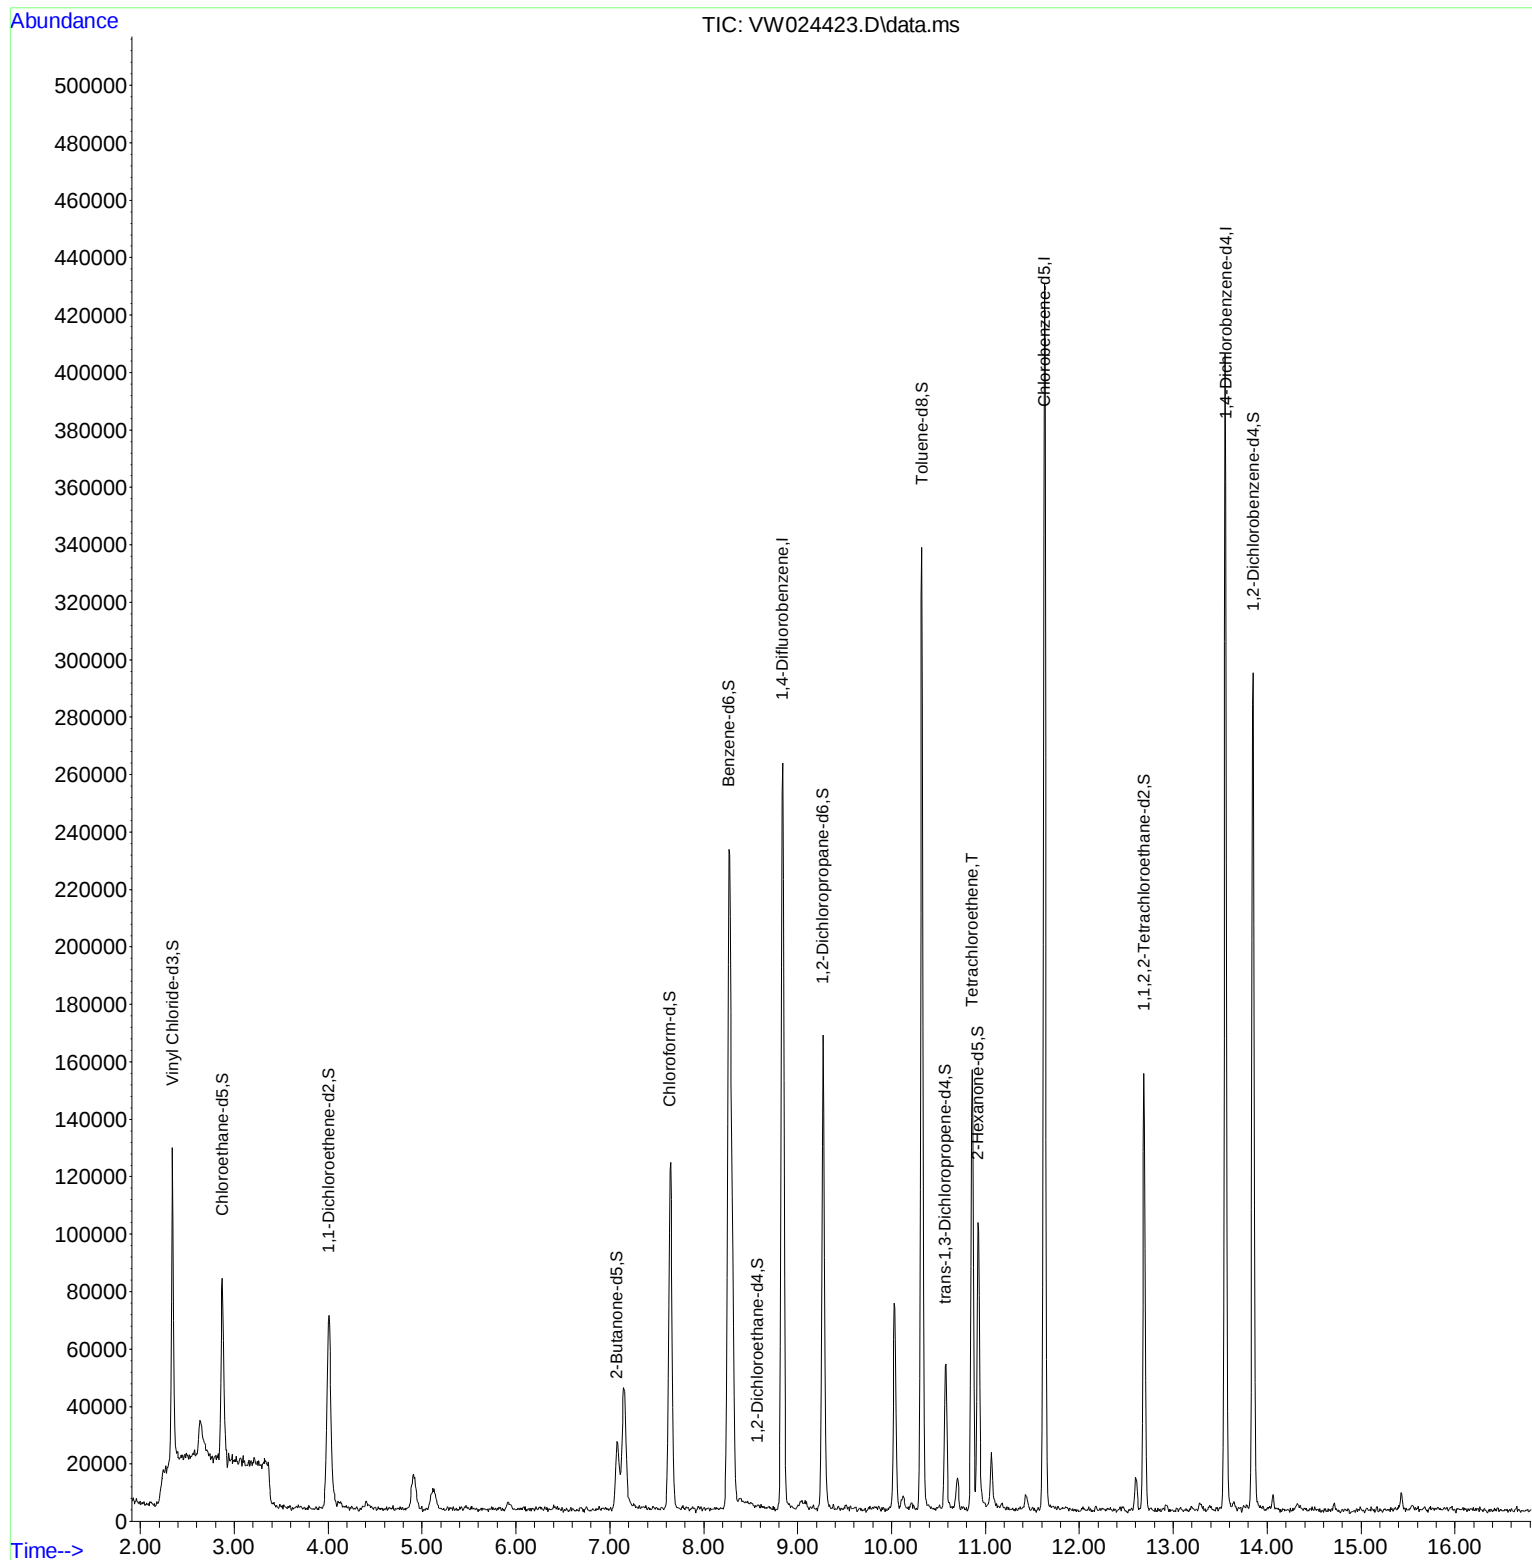

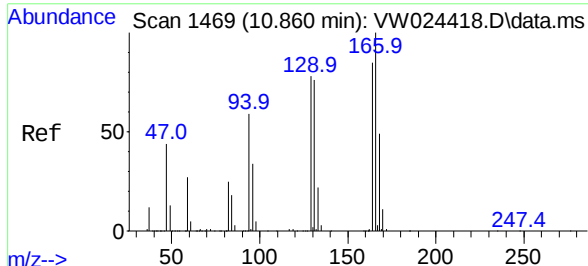

Tetrachloroethene
 Concen: 10.171 ug/L
 RT: 10.859 min Scan# 1469
 Delta R.T. -0.000 min
 Lab File: VW024423.D
 Acq: 28 Aug 2022 01:20

Instrument : MSVOA_W
 ClientSampleId :

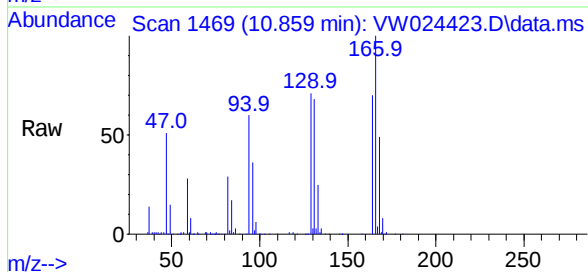

Tgt Ion:	164	Resp:	27362
Ion	Ratio	Lower	Upper
164	100		
129	100.8	72.9	135.3
131	97.3	63.7	118.3
166	142.1	86.2	160.0

