

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
 Data File : VW024424.D
 Acq On : 28 Aug 2022 01:44
 Operator : SY/VA
 Sample : N4363-21
 Misc : 5.80g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Aug 29 05:02:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Aug 29 04:56:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	256045	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	275216	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	111249	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.337	65	166039	23.525	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	94.080%		
7) Chloroethane-d5	2.867	69	107589	20.345	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	81.360%		
11) 1,1-Dichloroethene-d2	4.001	63	96662	15.791	ug/L	-0.01
Spiked Amount 25.000	Range 45 - 110		Recovery =	63.160%		
21) 2-Butanone-d5	7.336	46	263	0.202	ug/L	0.26
Spiked Amount 50.000	Range 20 - 135		Recovery =	0.400%#		
24) Chloroform-d	7.647	84	153062	18.594	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	74.360%		
26) 1,2-Dichloroethane-d4	8.415	65	169	0.034	ug/L	0.11
Spiked Amount 25.000	Range 70 - 130		Recovery =	0.120%#		
32) Benzene-d6	8.268	84	301509	19.121	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	76.480%		
36) 1,2-Dichloropropane-d6	9.268	67	90844	18.525	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	74.080%		
41) Toluene-d8	10.323	98	301911	20.137	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	80.560%		
43) trans-1,3-Dichloroprop...	10.579	79	32775	14.282	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	57.120%		
47) 2-Hexanone-d5	10.920	63	32002	29.161	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	58.320%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	79834	14.379	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	57.520%		
66) 1,2-Dichlorobenzene-d4	13.853	152	86109	20.554	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	82.200%		
Target Compounds						
					Qvalue	
46) Tetrachloroethene	10.860	164	541829	154.481	ug/L	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
Data File : VW024424.D
Acq On : 28 Aug 2022 01:44
Operator : SY/VA
Sample : N4363-21
Misc : 5.80g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Aug 29 05:02:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Aug 29 04:56:06 2022
Response via : Initial Calibration

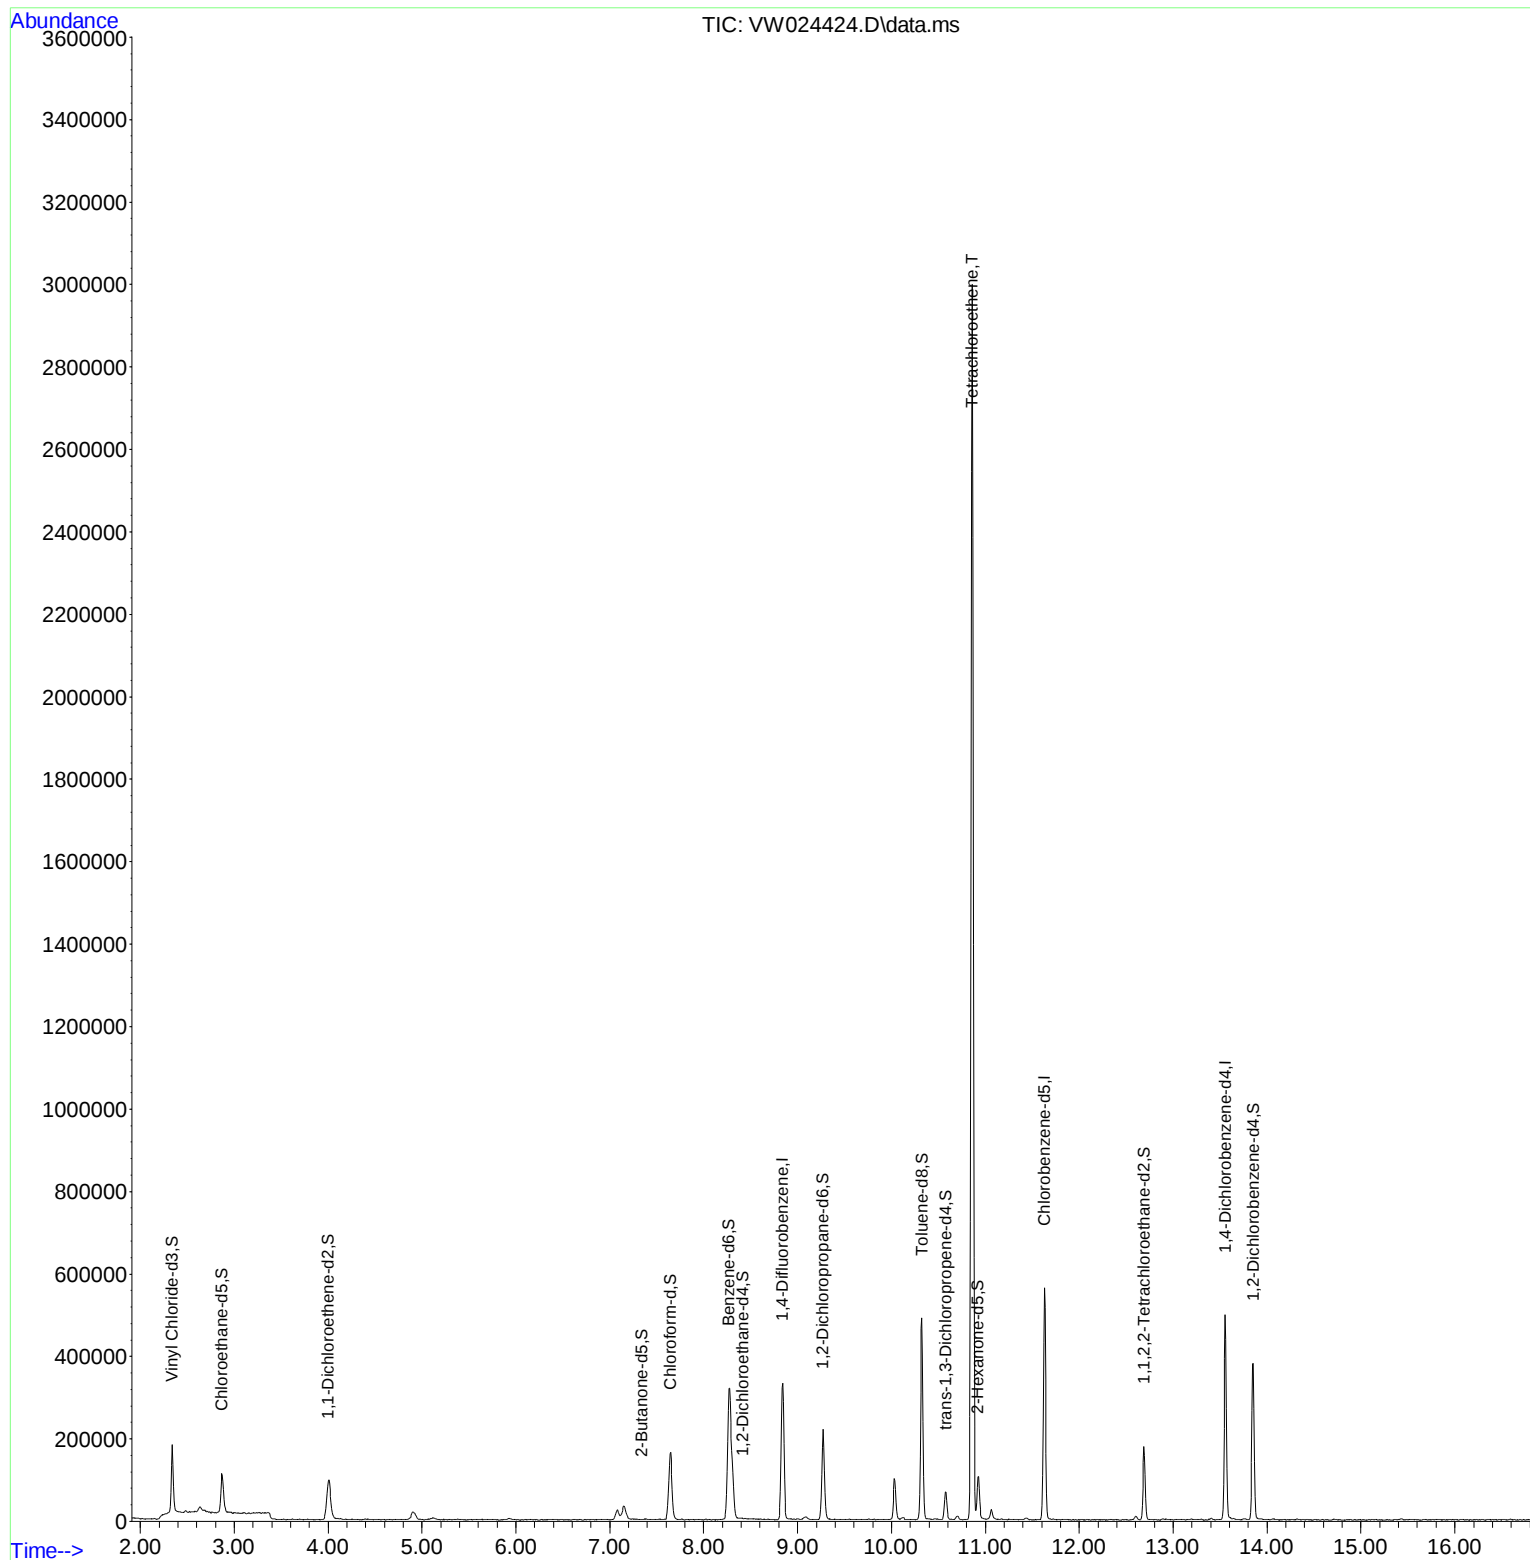

Abundance Scan 1469 (10.860 min): VW024418.D\data.ms (-1469) (-)

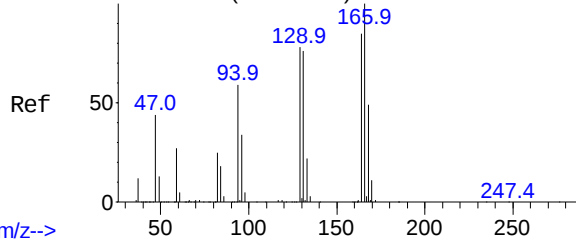

Tetrachloroethene

Concen: 154.481 ug/L

RT: 10.860 min Scan#

Delta R.T. -0.000 min

Lab File: VW024424.D


Acq: 28 Aug 2022 01:44

Instrument :

MSVOA_W

ClientSampleId :

Abundance Scan 1469 (10.860 min): VW024424.D\data.ms

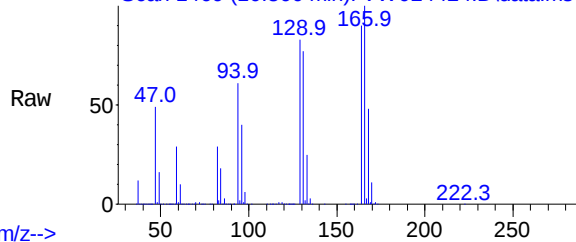

Tgt Ion:164 Resp: 541829

Ion Ratio Lower Upper


164 100

129 92.8 72.9 135.3


131 86.1 63.7 118.3

166 111.5 86.2 160.0

Abundance

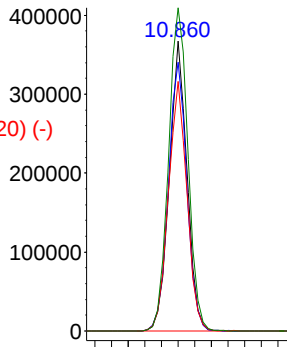

Abundance Scan 1469 (10.860 min): VW024424.D\data.ms (-1420) (-)

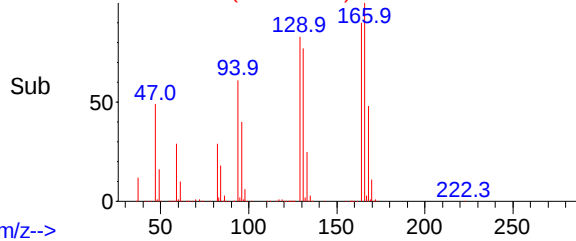

Time-->