




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
 Data File : VW024360.D
 Acq On : 26 Aug 2022 19:30
 Operator : SY/VA
 Sample : N4345-10
 Misc : 4.90g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVT0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
 Supervised By :Mahesh Dadoda 08/30/2022

Quant Time: Aug 27 00:43:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 27 00:35:21 2022
 Response via : Initial Calibration

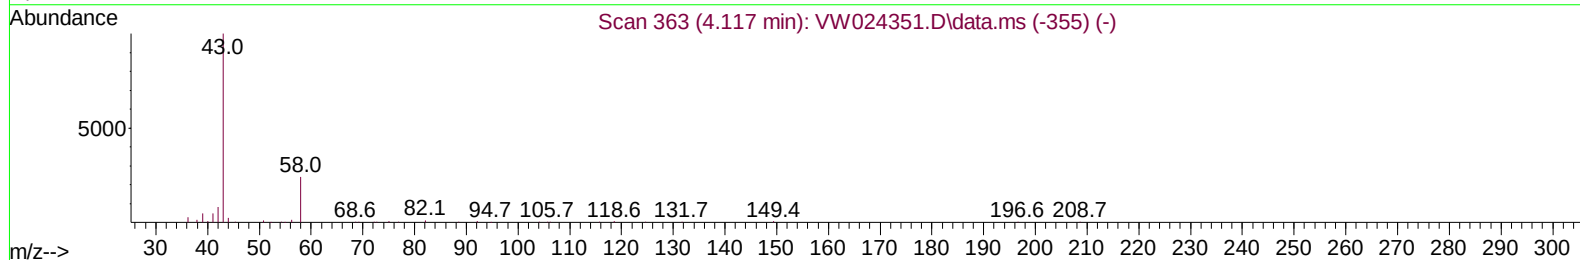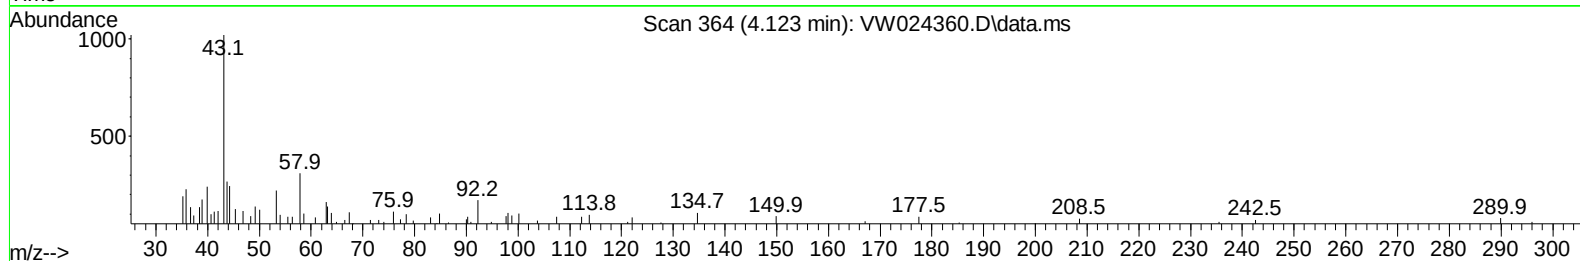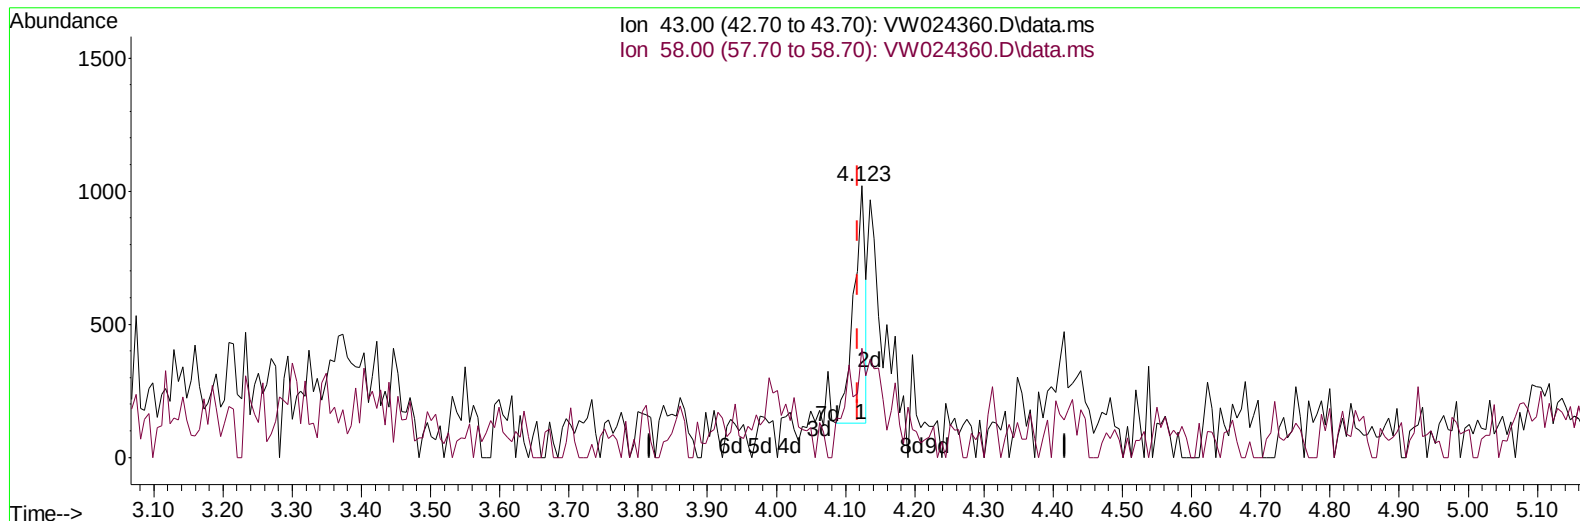

TIC: VW024360.D\data.ms

(13) Acetone (T)

4.123min (+ 0.006) 3.20 ug/L

response 1062

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	29.20	9.42
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
 Data File : VW024360.D
 Acq On : 26 Aug 2022 19:30
 Operator : SY/VA
 Sample : N4345-10
 Misc : 4.90g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVT0

Manual IntegrationsAPPROVED

Quant Time: Aug 27 00:43:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 27 00:35:21 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/30/2022
 Supervised By :Mahesh Dadoda 08/30/2022

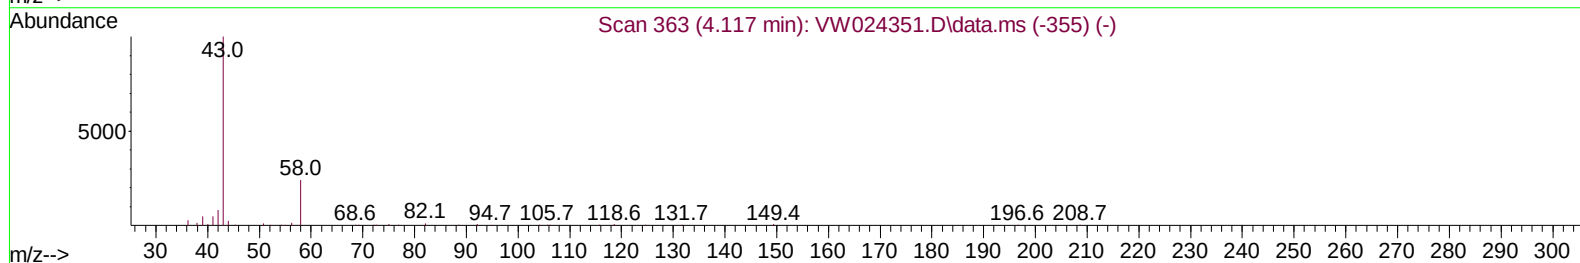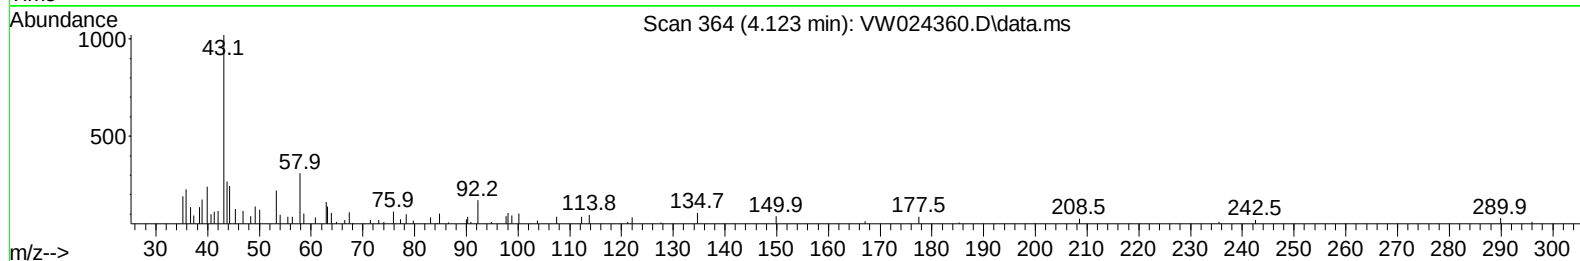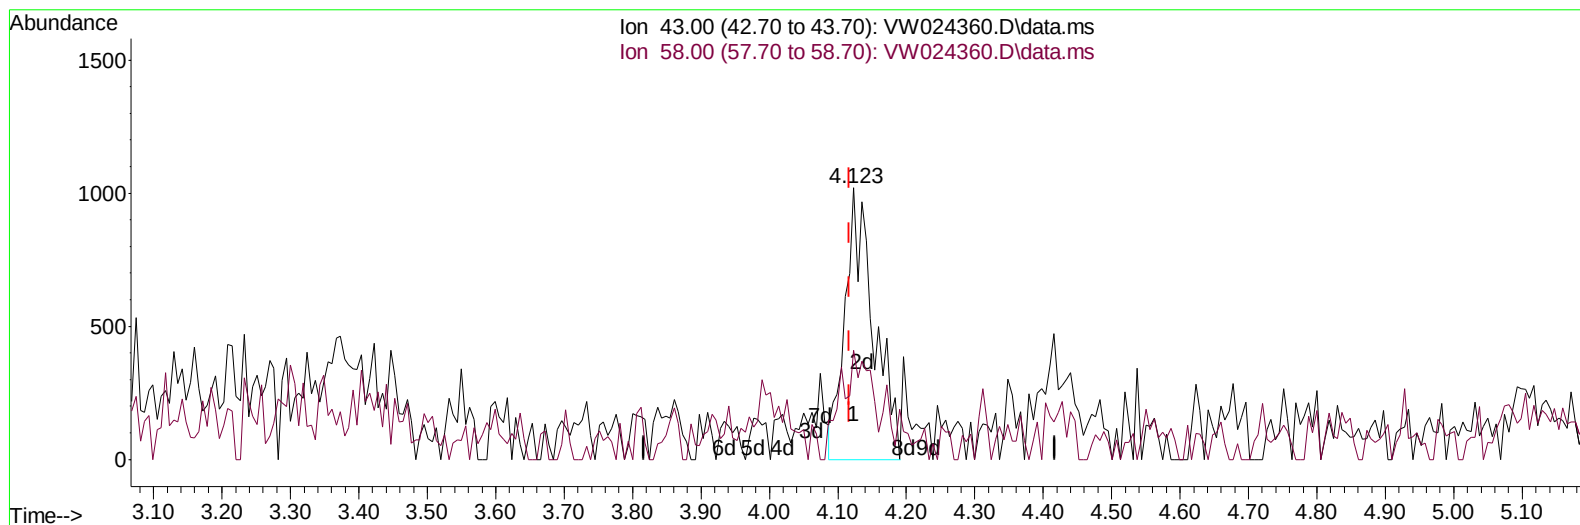

TIC: VW024360.D\data.ms

(13) Acetone (T)

4.123min (+ 0.006) 8.94 ug/L m

response 2971

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	29.20	3.37
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
 Data File : VW024360.D
 Acq On : 26 Aug 2022 19:30
 Operator : SY/VA
 Sample : N4345-10
 Misc : 4.90g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVT0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
 Supervised By :Mahesh Dadoda 08/30/2022

Quant Time: Aug 27 00:43:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 27 00:35:21 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		109699	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		118544	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152		51652	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.337	65		91954	30.409	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	121.640%		
7) Chloroethane-d5	2.873	69		50927	22.477	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	89.920%		
11) 1,1-Dichloroethene-d2	4.007	63		46641	17.784	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	71.120%		
21) 2-Butanone-d5	7.086	46		23747	42.635	ug/L	0.01
Spiked Amount 50.000	Range 20	- 135		Recovery =	85.280%		
24) Chloroform-d	7.647	84		72971	20.691	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	82.760%		
26) 1,2-Dichloroethane-d4	8.305	65		46328	21.661	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	86.640%		
32) Benzene-d6	8.269	84		141017	20.762	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	83.040%		
36) 1,2-Dichloropropane-d6	9.268	67		43933	20.799	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	83.200%		
41) Toluene-d8	10.323	98		126384	19.571	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	78.280%		
43) trans-1,3-Dichloroprop...	10.579	79		16517	16.709	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	66.840%		
47) 2-Hexanone-d5	10.921	63		15034	31.805	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	63.620%		
56) 1,1,2,2-Tetrachloroeth...	12.689	84		42559	17.796	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	71.200%		
66) 1,2-Dichlorobenzene-d4	13.853	152		40416	20.778	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	83.120%		
Target Compounds							
13) Acetone	4.123	43		2971m	8.938	ug/L	
16) Methylene chloride	4.916	84		10765	5.851	ug/L	96
46) Tetrachloroethene	10.860	164		60408	39.985	ug/L	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
Data File : VW024360.D
Acq On : 26 Aug 2022 19:30
Operator : SY/VA
Sample : N4345-10
Misc : 4.90g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBVT0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
Supervised By :Mahesh Dadoda 08/30/2022

Quant Time: Aug 27 00:43:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Aug 27 00:35:21 2022
Response via : Initial Calibration

