




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
Data File : VW024381.D
Acq On : 27 Aug 2022 05:45
Operator : SY/VA
Sample : N4345-05
Misc : 4.27g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBVS5

Manual IntegrationsAPPROVED

Quant Time: Aug 27 07:29:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Aug 27 02:57:08 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/30/2022
Supervised By :Mahesh Dadoda 08/30/2022

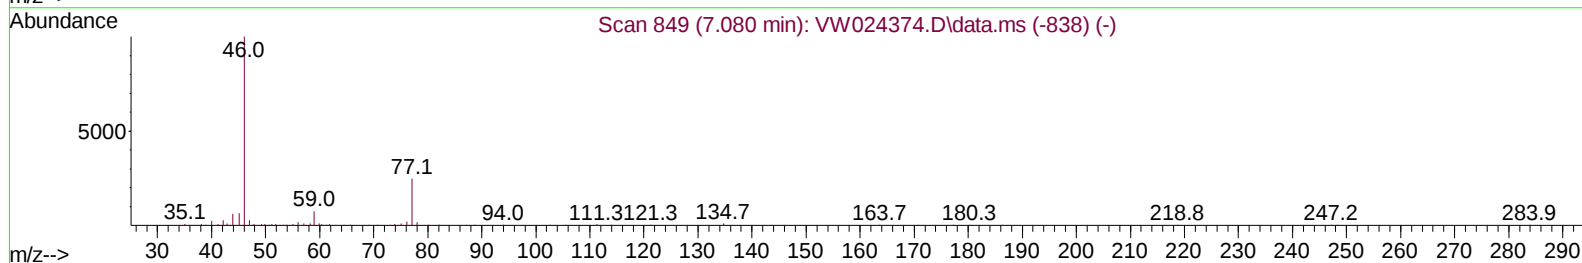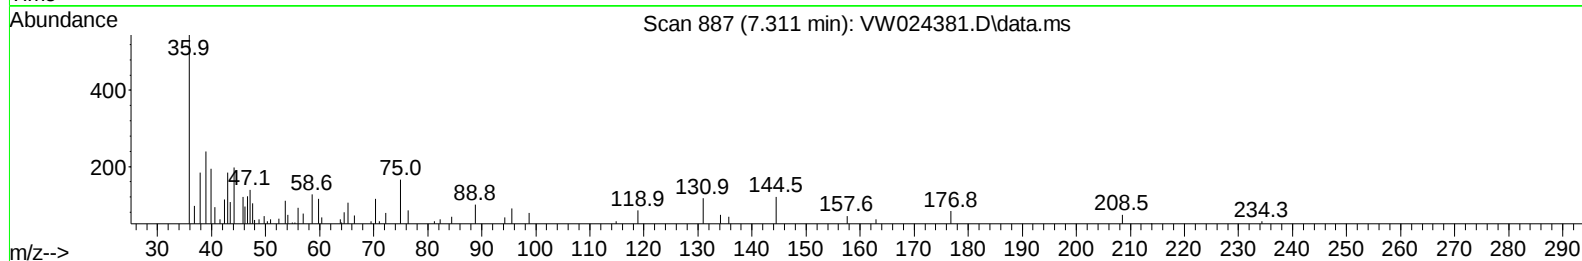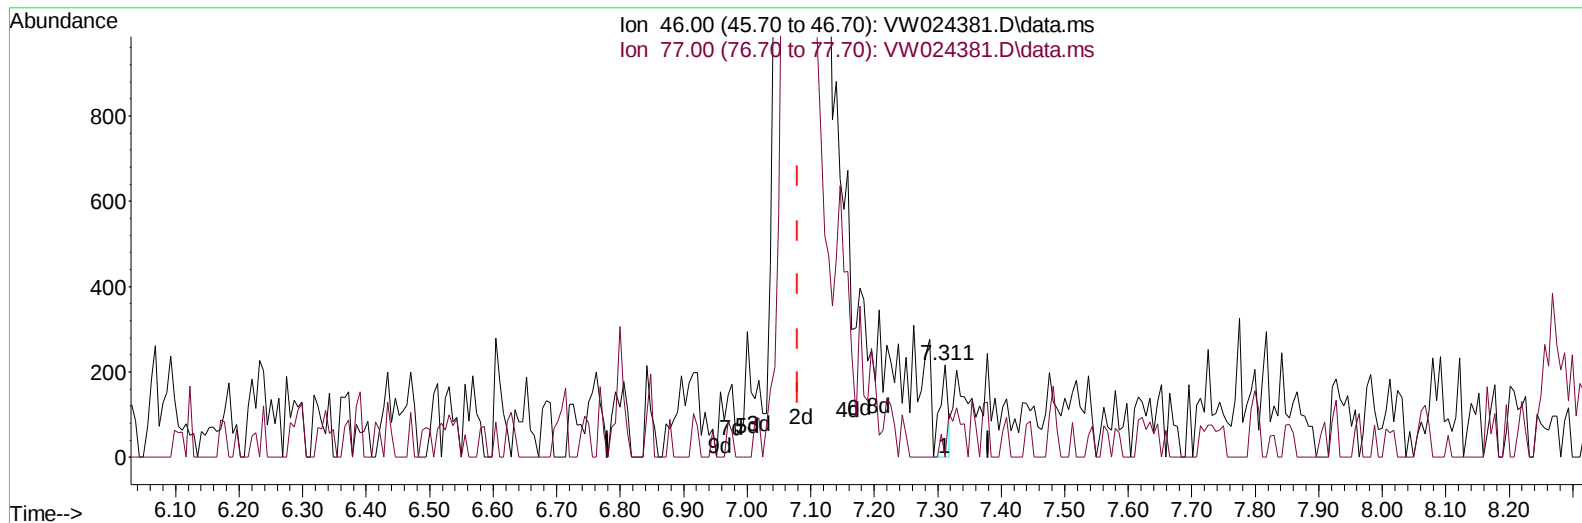

TIC: VW024381.D\data.ms

(21) 2-Butanone-d5 (S)

7.311min (+ 0.232) 0.16 ug/L

response 194

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	12.40	10.31
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
 Data File : VW024381.D
 Acq On : 27 Aug 2022 05:45
 Operator : SY/VA
 Sample : N4345-05
 Misc : 4.27g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVS5

Manual IntegrationsAPPROVED

Quant Time: Aug 27 07:29:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 27 02:57:08 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/30/2022
 Supervised By :Mahesh Dadoda 08/30/2022

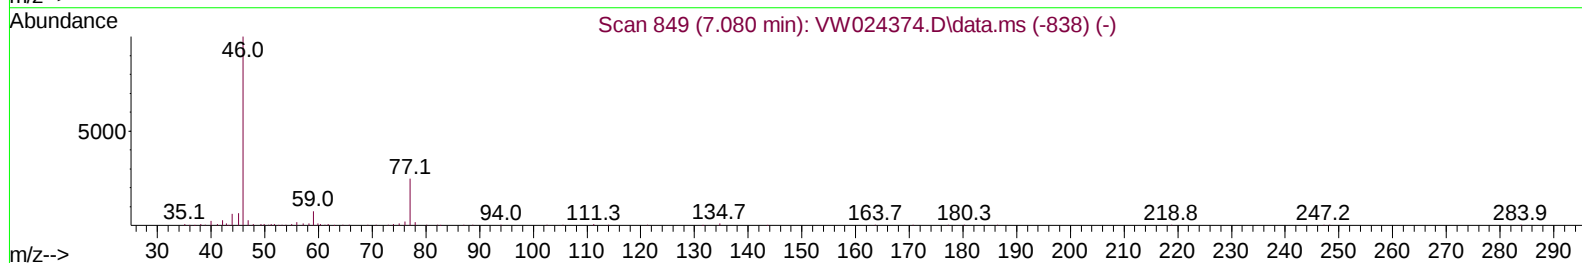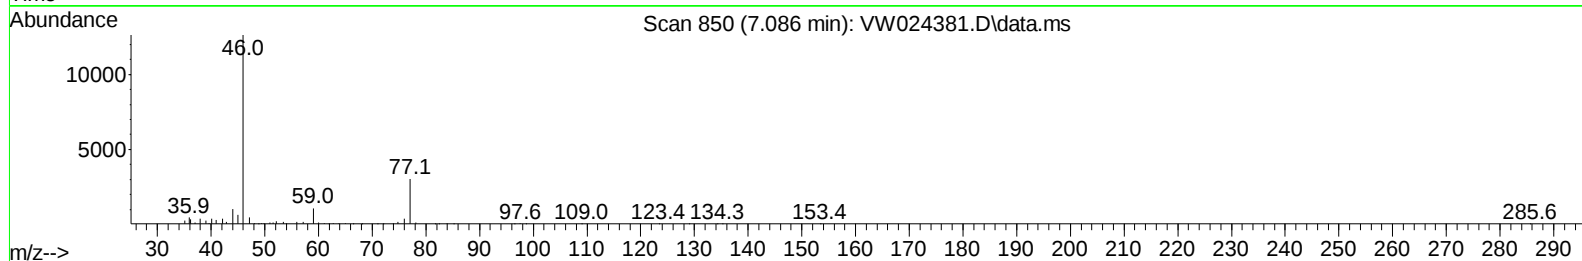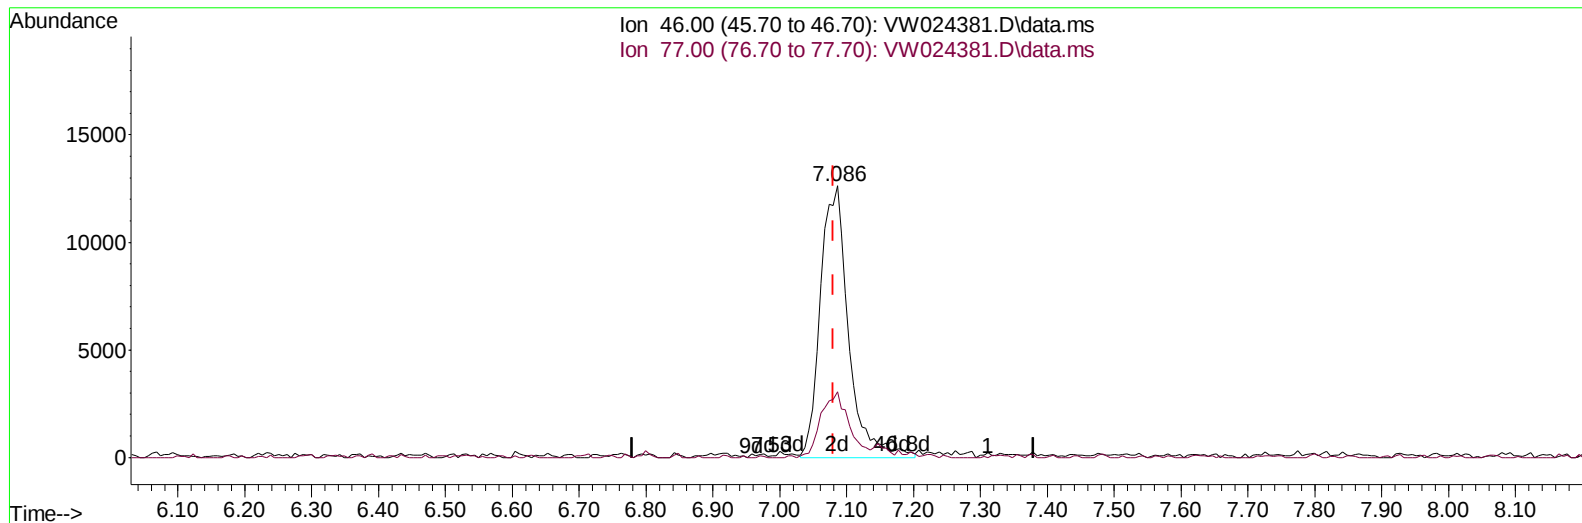

TIC: VW024381.D\data.ms

(21) 2-Butanone-d5 (S)

7.086min (+ 0.006) 30.52 ug/L m

response 36786

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	12.40	0.05#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
 Data File : VW024381.D
 Acq On : 27 Aug 2022 05:45
 Operator : SY/VA
 Sample : N4345-05
 Misc : 4.27g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVS5

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
 Supervised By :Mahesh Dadoda 08/30/2022

Quant Time: Aug 27 07:29:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 27 02:57:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	237390	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	237431	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	107064	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	143716	21.962	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	87.840%	
7) Chloroethane-d5	2.873	69	102778	20.962	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	83.840%	
11) 1,1-Dichloroethene-d2	4.007	63	87644	15.443	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	61.760%	
21) 2-Butanone-d5	7.086	46	36786m	30.520	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	61.040%	
24) Chloroform-d	7.647	84	130094	17.046	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	68.200%	
26) 1,2-Dichloroethane-d4	8.299	65	76055	16.433	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	65.720%#	
32) Benzene-d6	8.275	84	262495	19.296	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	77.200%	
36) 1,2-Dichloropropane-d6	9.268	67	76193	18.010	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	72.040%	
41) Toluene-d8	10.323	98	242910	18.781	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	75.120%	
43) trans-1,3-Dichloroprop...	10.579	79	27122	13.699	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	54.800%	
47) 2-Hexanone-d5	10.927	63	27274	28.808	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	57.620%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	65895	13.757	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	55.040%	
66) 1,2-Dichlorobenzene-d4	13.853	152	76763	19.040	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	76.160%	
Target Compounds						
46) Tetrachloroethene	10.859	164	411825	136.101	ug/L	Qvalue 95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
Data File : VW024381.D
Acq On : 27 Aug 2022 05:45
Operator : SY/VA
Sample : N4345-05
Misc : 4.27g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBVS5

Manual IntegrationsAPPROVED

Quant Time: Aug 27 07:29:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Aug 27 02:57:08 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/30/2022
Supervised By :Mahesh Dadoda 08/30/2022

