




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
Data File : VW024386.D
Acq On : 27 Aug 2022 07:47
Operator : SY/VA
Sample : N4345-13
Misc : 5.69g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBVT1

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
Supervised By :Mahesh Dadoda 08/30/2022

Quant Time: Aug 29 00:58:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Aug 29 00:57:06 2022
Response via : Initial Calibration

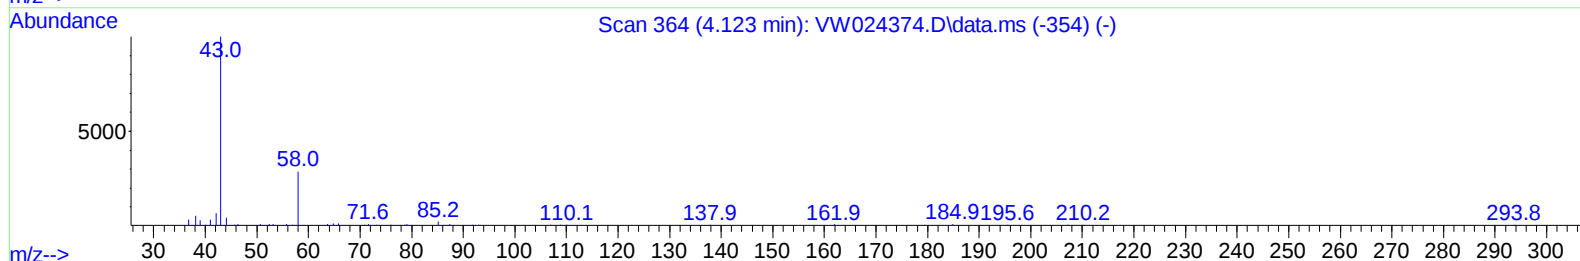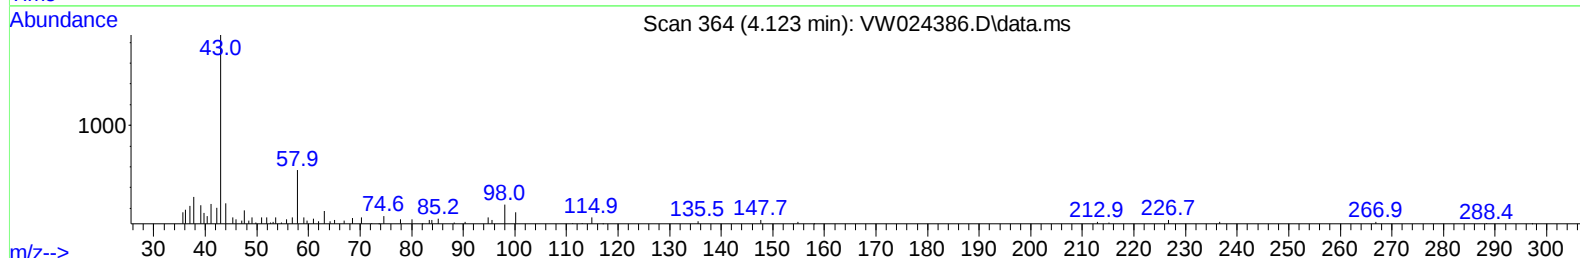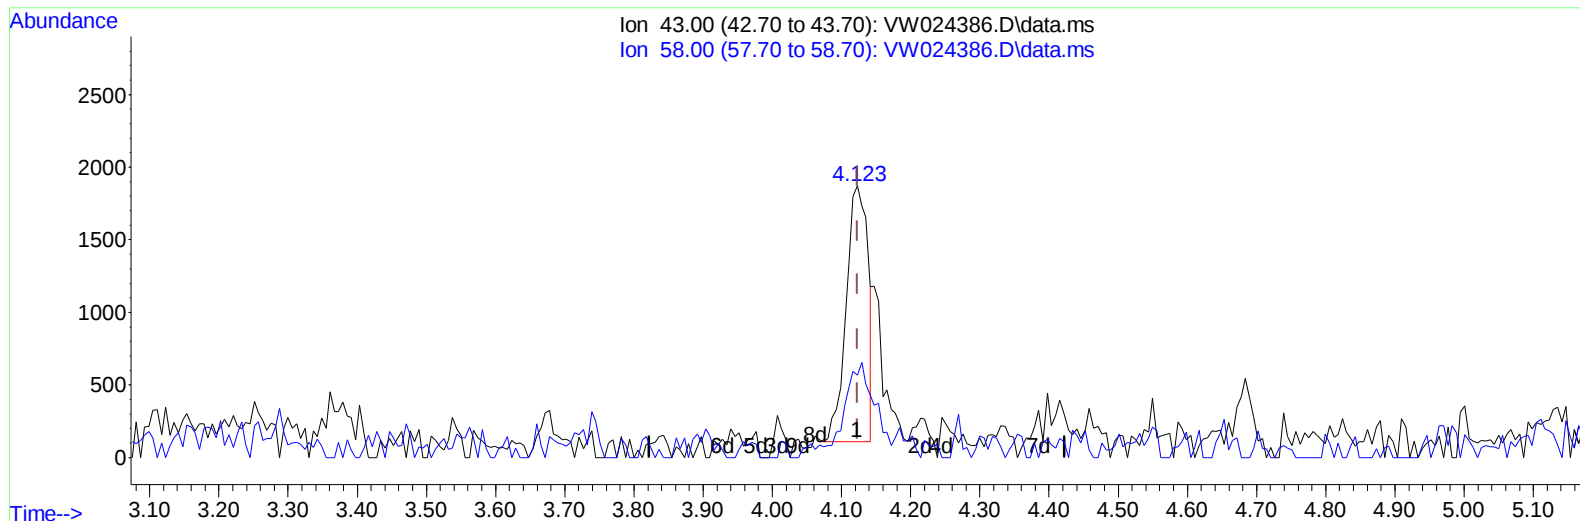

TIC: VW024386.D\data.ms

(13) Acetone (T)

4.123min (-0.000) 6.25 ug/L

response 3836

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	29.20	49.64
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
 Data File : VW024386.D
 Acq On : 27 Aug 2022 07:47
 Operator : SY/VA
 Sample : N4345-13
 Misc : 5.69g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVT1

Manual IntegrationsAPPROVED

Quant Time: Aug 29 00:58:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Aug 29 00:57:06 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/30/2022
 Supervised By :Mahesh Dadoda 08/30/2022

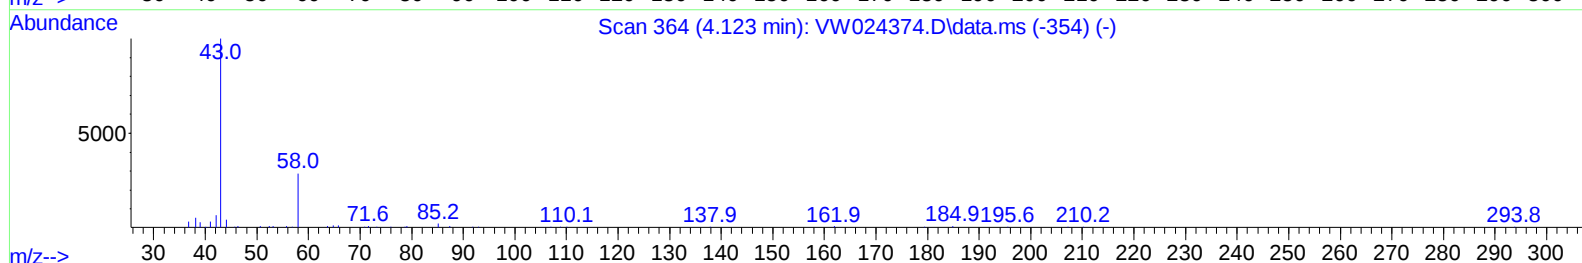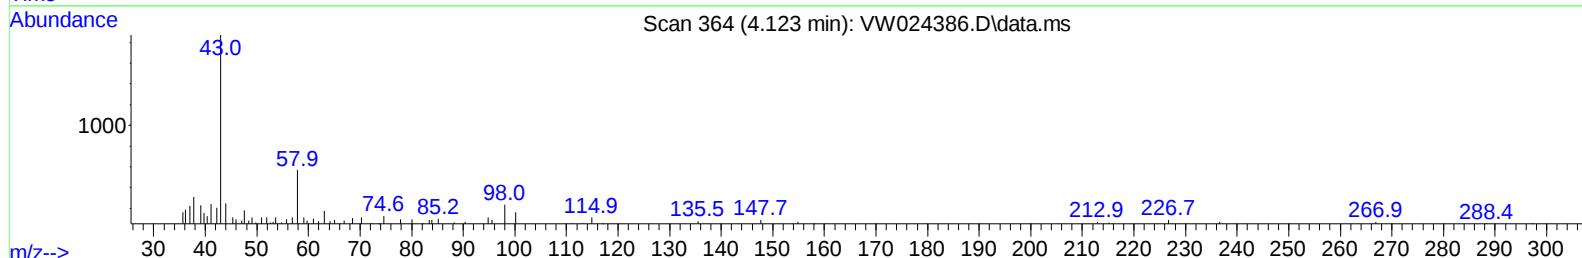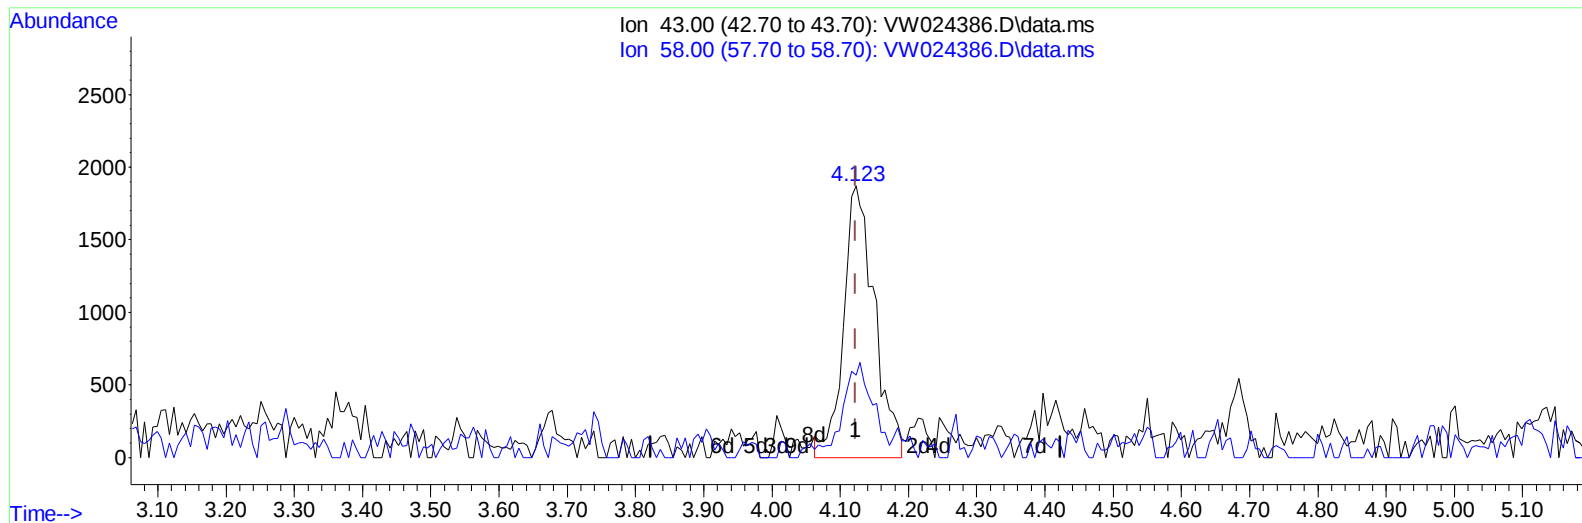

TIC: VW024386.D\data.ms

(13) Acetone (T)

4.123min (-0.000) 9.57 ug/L m

response 5874

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	29.20	32.41
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
 Data File : VW024386.D
 Acq On : 27 Aug 2022 07:47
 Operator : SY/VA
 Sample : N4345-13
 Misc : 5.69g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVT1

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
 Supervised By :Mahesh Dadoda 08/30/2022

Quant Time: Aug 29 00:58:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Aug 29 00:57:06 2022
 Response via : Initial Calibration

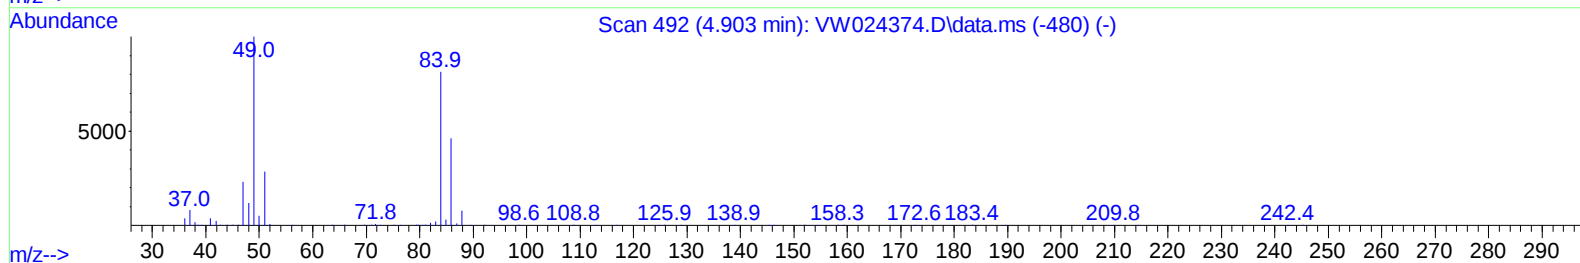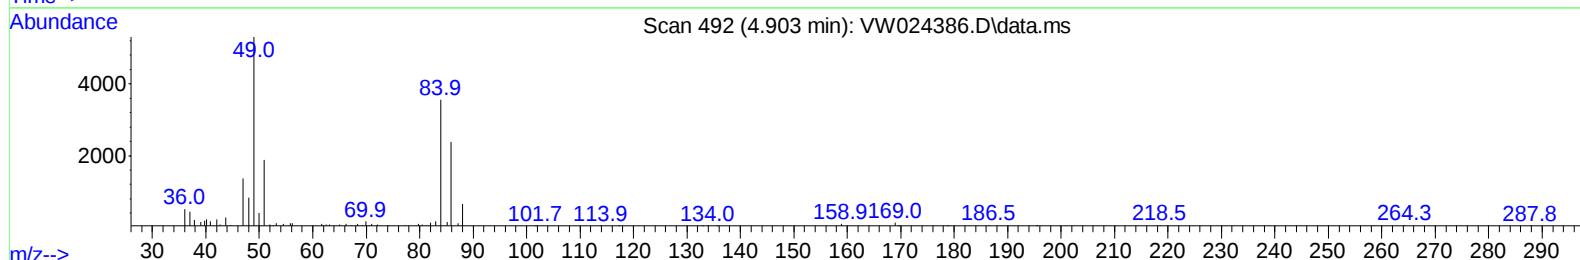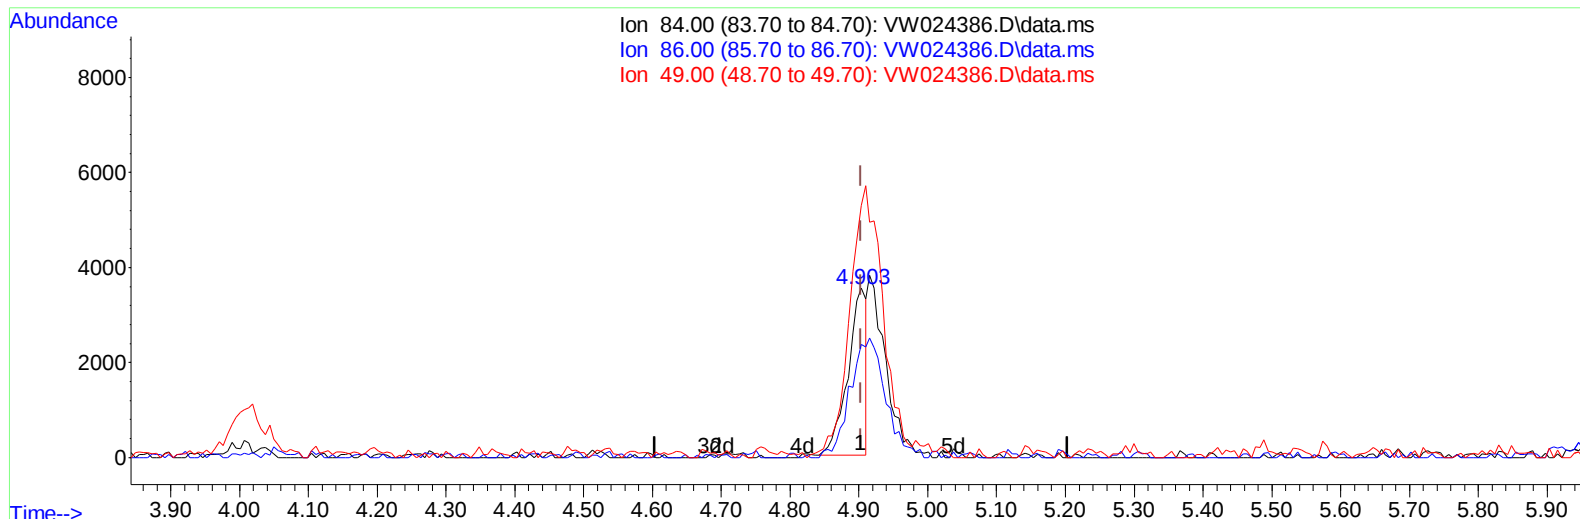

TIC: VW024386.D\data.ms

(16) Methylene chloride (T)

4.903min (0.000) 1.91 ug/L

response 6483

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	68.20	66.82
49.00	138.00	148.70
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
 Data File : VW024386.D
 Acq On : 27 Aug 2022 07:47
 Operator : SY/VA
 Sample : N4345-13
 Misc : 5.69g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVT1

Manual IntegrationsAPPROVED

Quant Time: Aug 29 00:58:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Aug 29 00:57:06 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/30/2022
 Supervised By :Mahesh Dadoda 08/30/2022

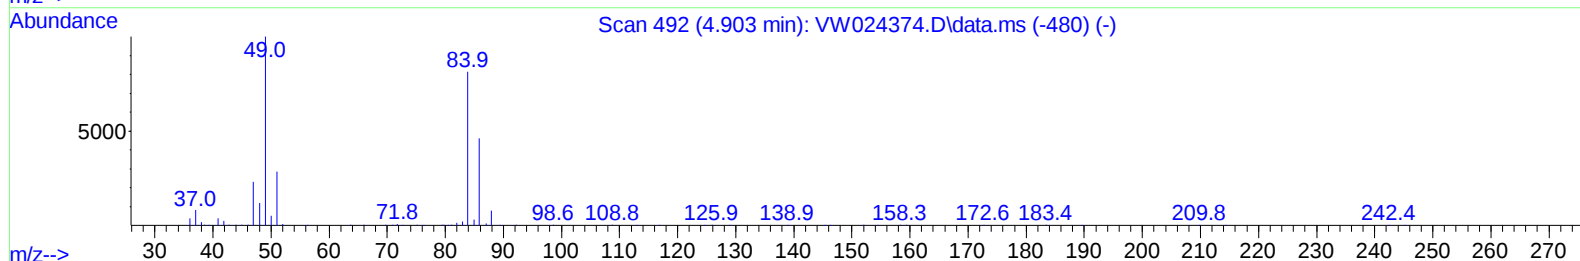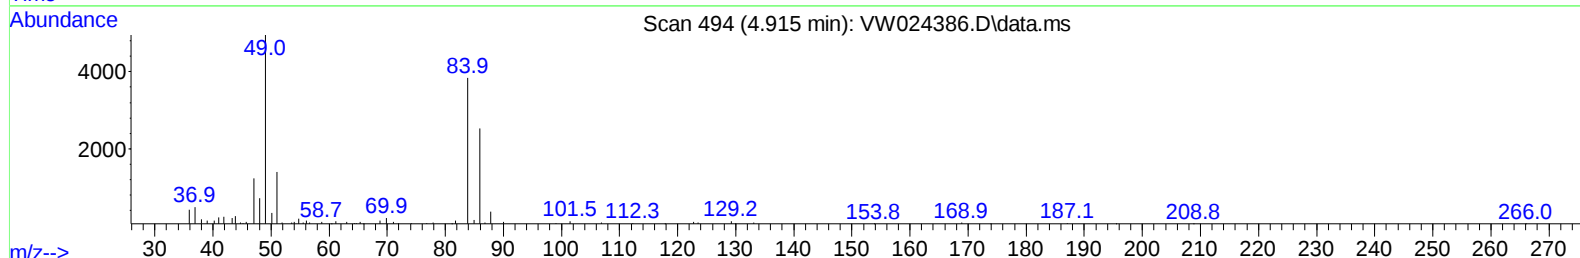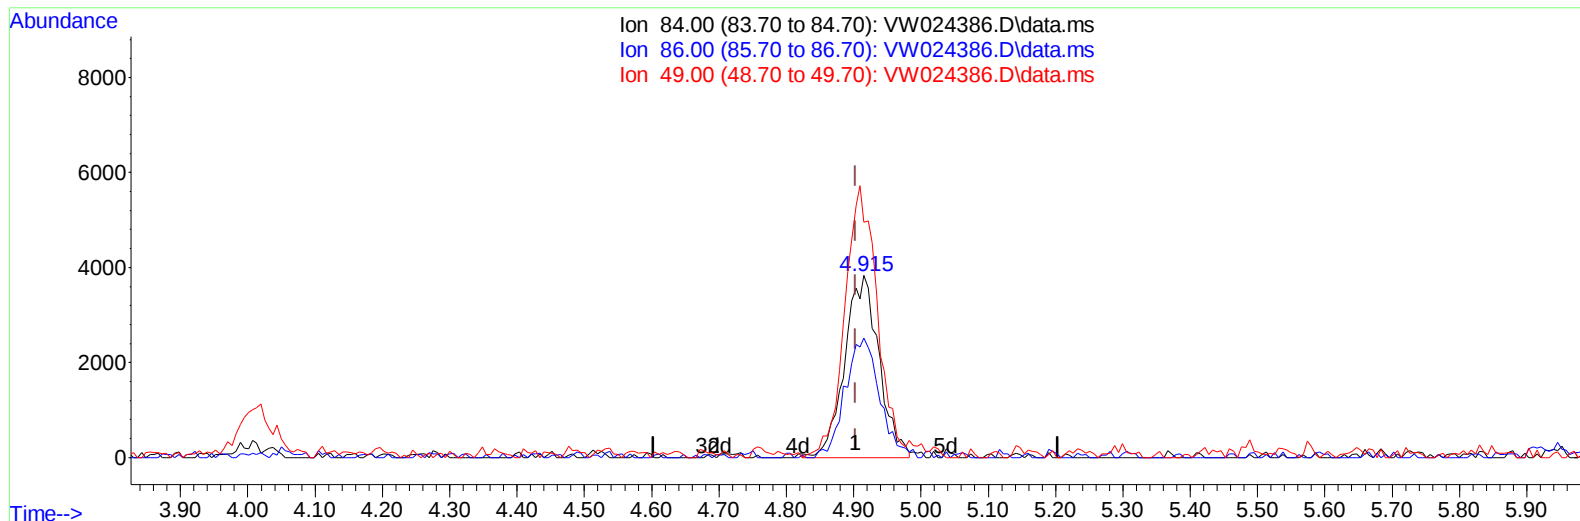

TIC: VW024386.D\data.ms

(16) Methylene chloride (T)

4.915min (+ 0.012) 3.99 ug/L m

response 13560

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	68.20	65.71
49.00	138.00	129.15
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
 Data File : VW024386.D
 Acq On : 27 Aug 2022 07:47
 Operator : SY/VA
 Sample : N4345-13
 Misc : 5.69g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVT1

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
 Supervised By :Mahesh Dadoda 08/30/2022

Quant Time: Aug 29 00:58:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Aug 29 00:57:06 2022
 Response via : Initial Calibration

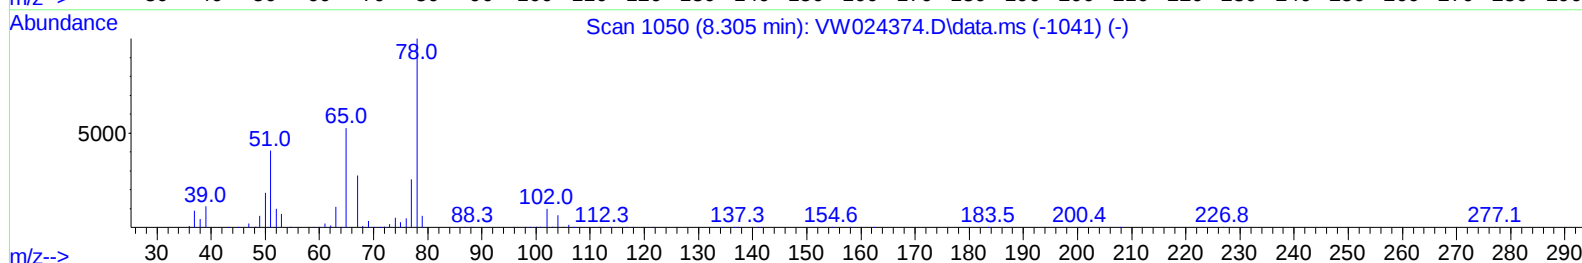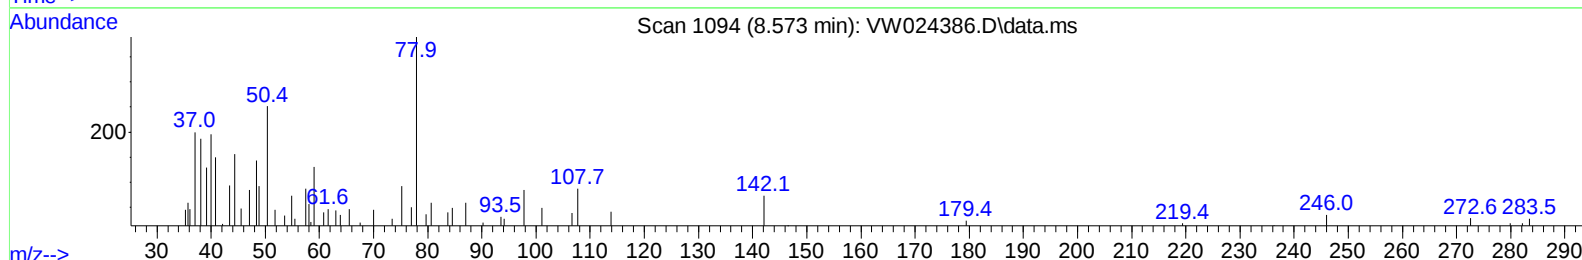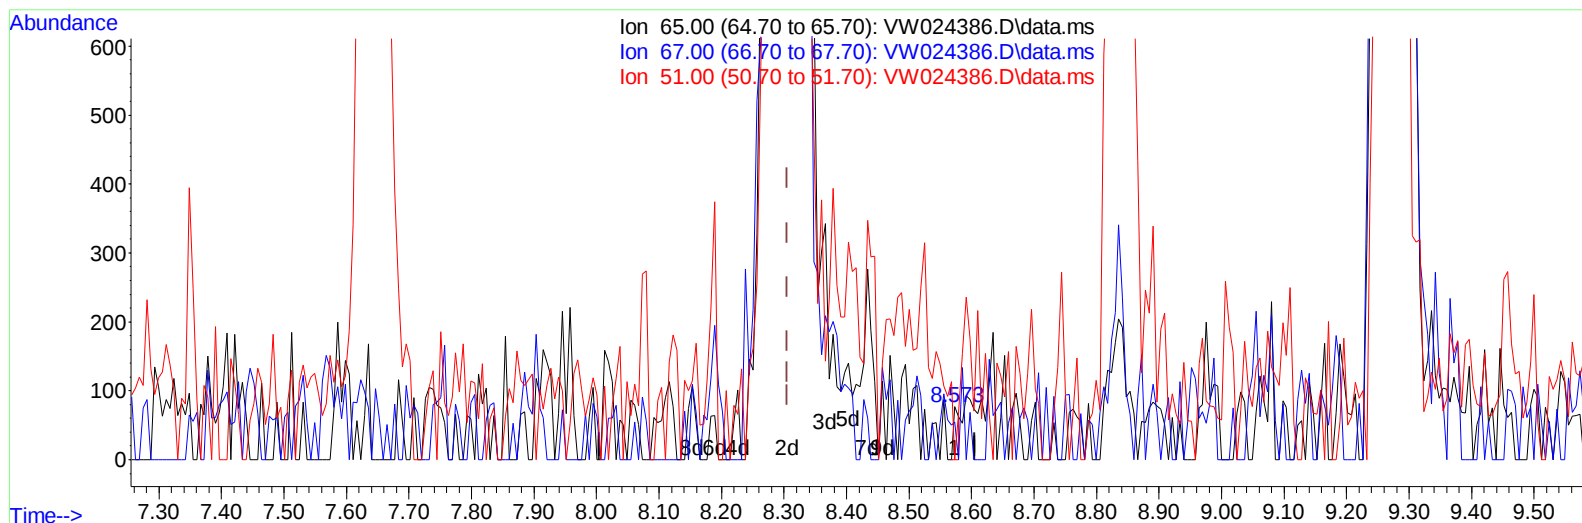

TIC: VW024386.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.573min (+ 0.268) 0.01 ug/L

response 51

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.10	39.22
51.00	96.50	80.39
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
 Data File : VW024386.D
 Acq On : 27 Aug 2022 07:47
 Operator : SY/VA
 Sample : N4345-13
 Misc : 5.69g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVT1

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
 Supervised By :Mahesh Dadoda 08/30/2022

Quant Time: Aug 29 00:58:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Aug 29 00:57:06 2022
 Response via : Initial Calibration

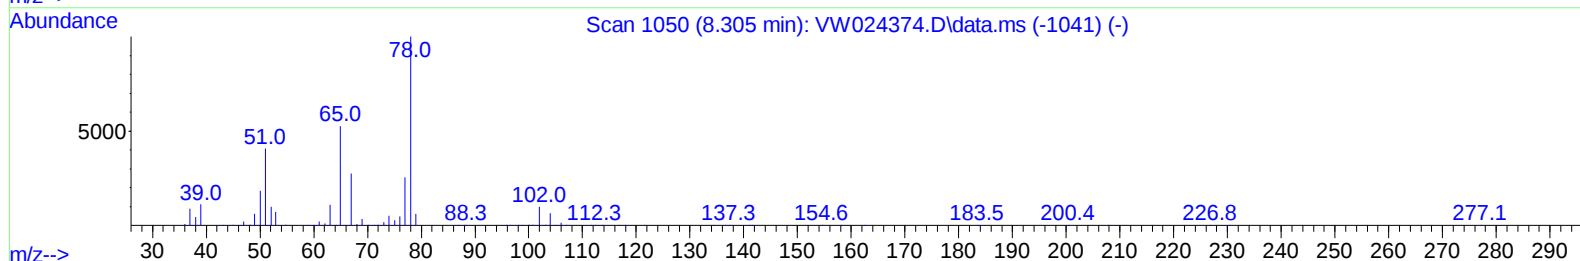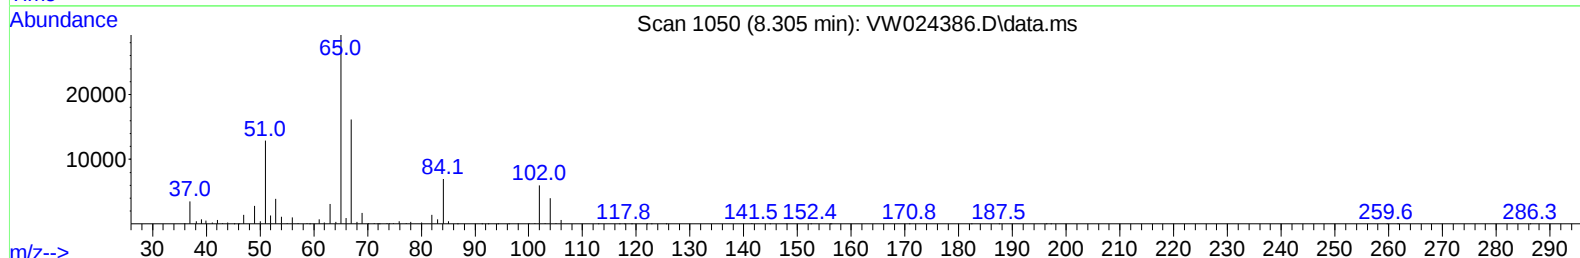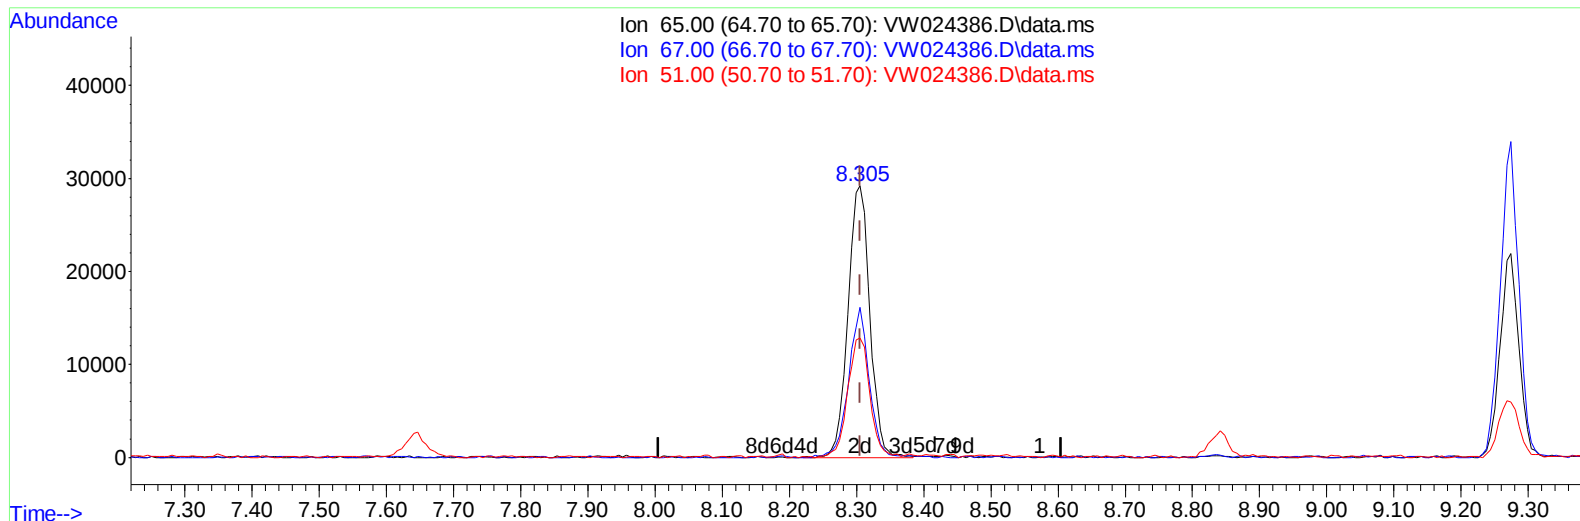

TIC: VW024386.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (0.000) 16.71 ug/L m

response 65953

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.10	0.03#
51.00	96.50	0.06#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
 Data File : VW024386.D
 Acq On : 27 Aug 2022 07:47
 Operator : SY/VA
 Sample : N4345-13
 Misc : 5.69g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVT1

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
 Supervised By :Mahesh Dadoda 08/30/2022

Quant Time: Aug 29 00:58:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Aug 29 00:57:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	202494	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	199653	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	86609	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	105482	18.897	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	75.600%	
7) Chloroethane-d5	2.873	69	86332	20.642	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	82.560%	
11) 1,1-Dichloroethene-d2	4.007	63	66353	13.706	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	54.840%	
21) 2-Butanone-d5	7.080	46	31322	30.465	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	60.940%	
24) Chloroform-d	7.647	84	106620	16.378	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	65.520%	
26) 1,2-Dichloroethane-d4	8.305	65	65953m	16.706	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	66.840%#	
32) Benzene-d6	8.275	84	210738	18.422	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	73.680%	
36) 1,2-Dichloropropane-d6	9.274	67	65035	18.281	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	73.120%	
41) Toluene-d8	10.323	98	199592	18.351	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	73.400%	
43) trans-1,3-Dichloroprop...	10.579	79	20841	12.518	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	50.080%	
47) 2-Hexanone-d5	10.921	63	20344	25.554	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	51.100%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	61492	15.267	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	61.080%	
66) 1,2-Dichlorobenzene-d4	13.853	152	59120	18.127	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	72.520%#	
Target Compounds						Qvalue
13) Acetone	4.123	43	5874m	9.574	ug/L	
16) Methylene chloride	4.915	84	13560m	3.993	ug/L	
46) Tetrachloroethene	10.860	164	332447	130.657	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
Data File : VW024386.D
Acq On : 27 Aug 2022 07:47
Operator : SY/VA
Sample : N4345-13
Misc : 5.69g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBVT1

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
Supervised By :Mahesh Dadoda 08/30/2022

Quant Time: Aug 29 00:58:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Aug 29 00:57:06 2022
Response via : Initial Calibration

