




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
 Data File : VW024430.D
 Acq On : 28 Aug 2022 04:11
 Operator : SY/VA
 Sample : N4346-05
 Misc : 5.50g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVU5

Manual IntegrationsAPPROVED

Quant Time: Aug 30 11:58:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 30 07:05:43 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/10/2022
 Supervised By :Mahesh Dadoda 09/10/2022

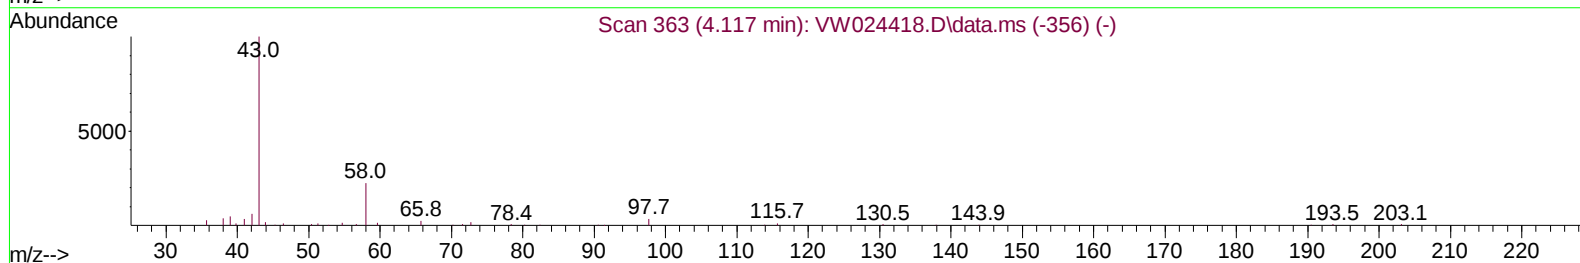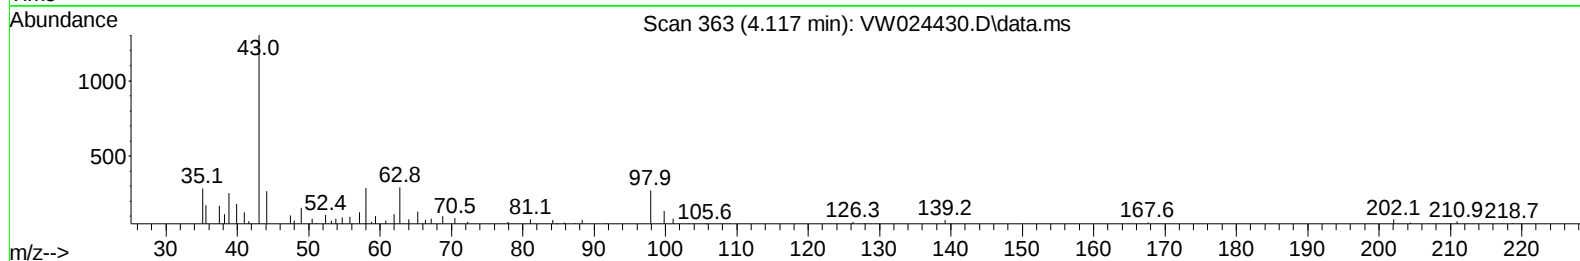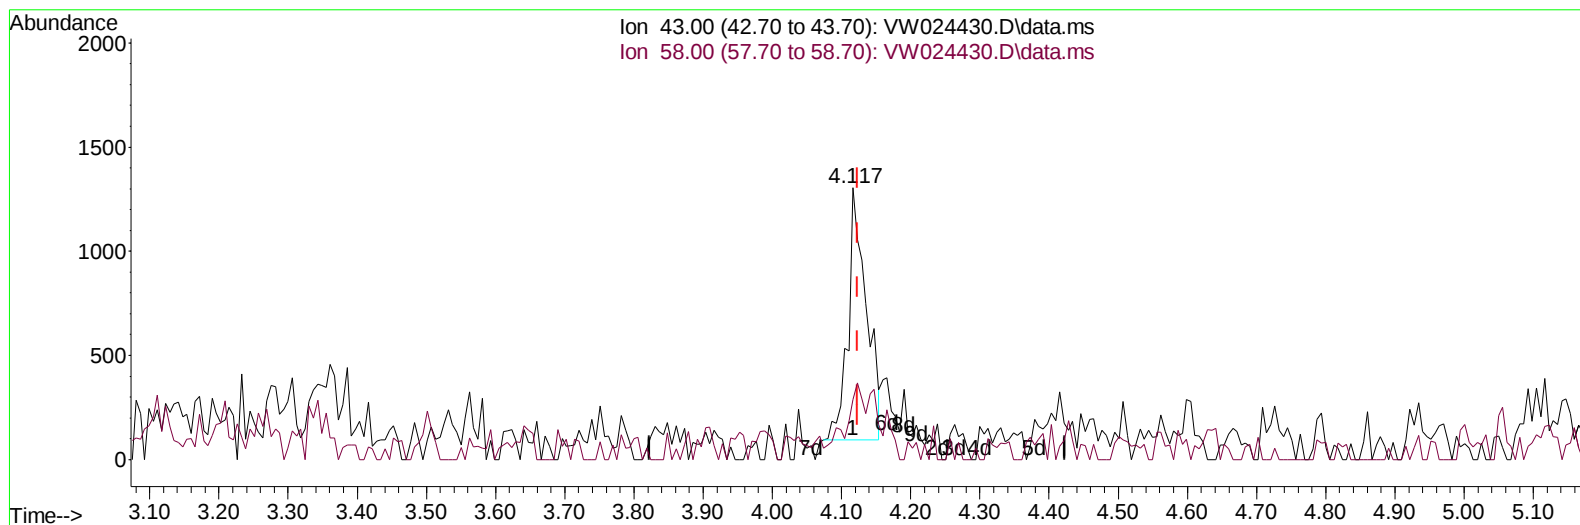

TIC: VW024430.D\data.ms

(13) Acetone (T)

4.117min (-0.006) 4.19 ug/L

response 2239

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	29.20	22.11
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
 Data File : VW024430.D
 Acq On : 28 Aug 2022 04:11
 Operator : SY/VA
 Sample : N4346-05
 Misc : 5.50g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVU5

Manual IntegrationsAPPROVED

Quant Time: Aug 30 11:58:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 30 07:05:43 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/10/2022
 Supervised By :Mahesh Dadoda 09/10/2022

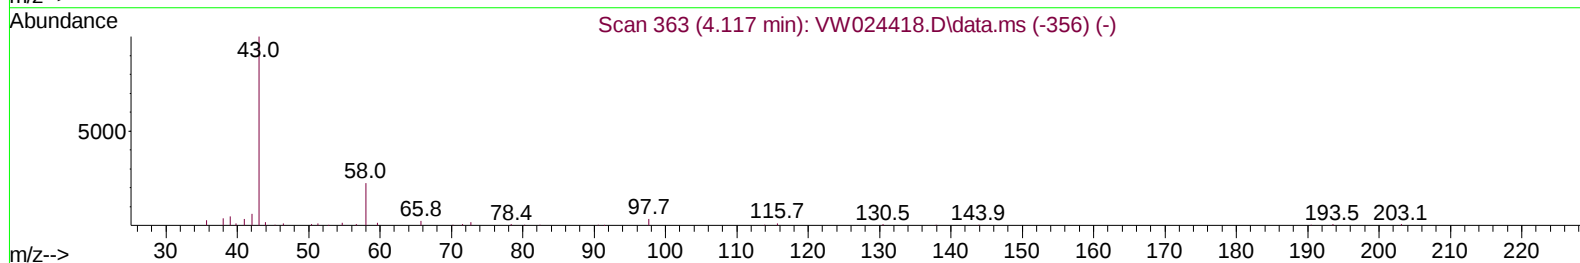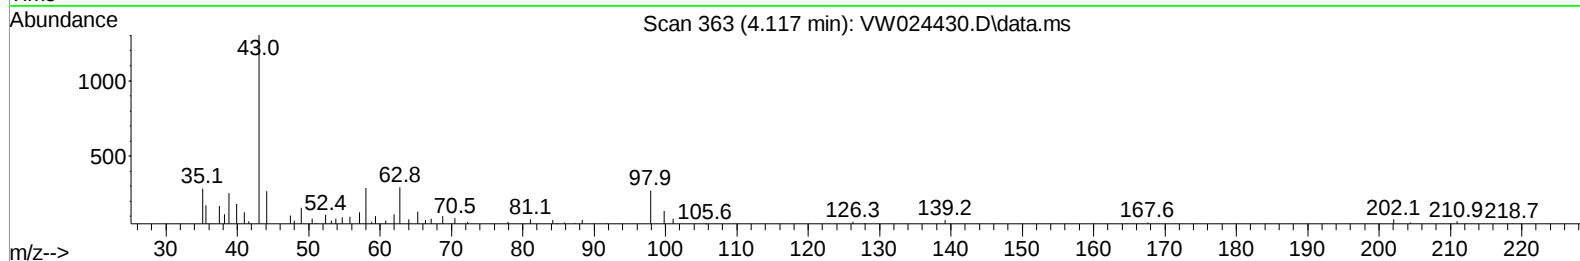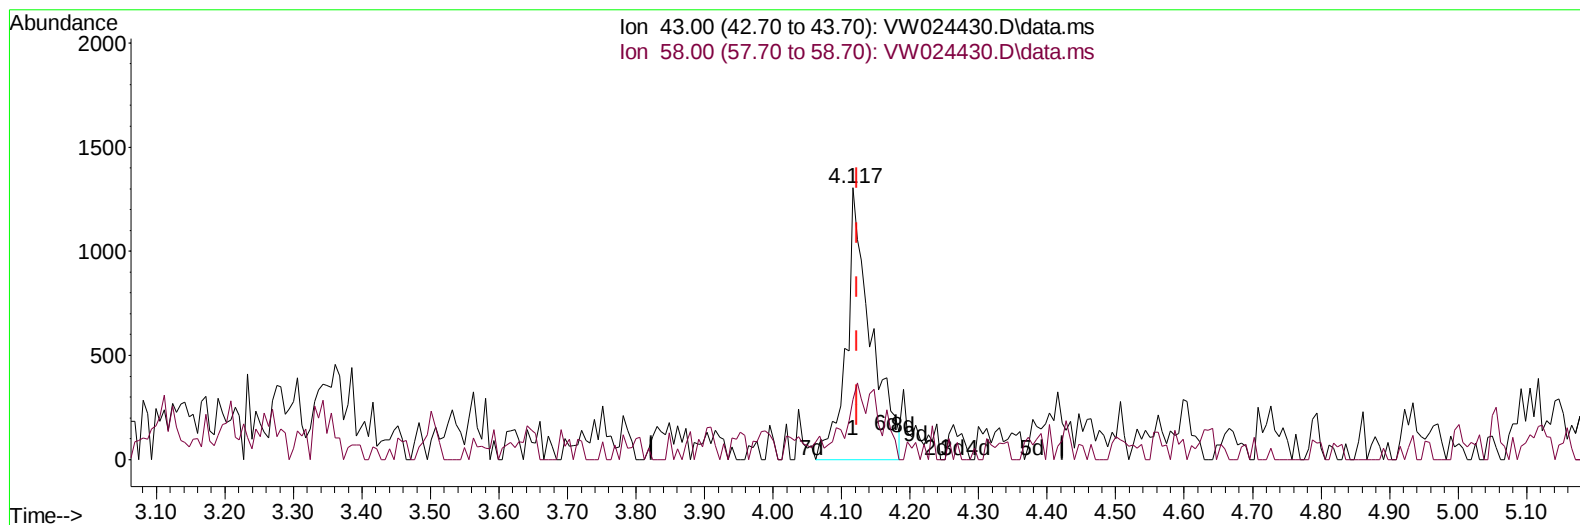

TIC: VW024430.D\data.ms

(13) Acetone (T)

4.117min (-0.006) 6.06 ug/L m

response 3242

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	29.20	15.27
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
 Data File : VW024430.D
 Acq On : 28 Aug 2022 04:11
 Operator : SY/VA
 Sample : N4346-05
 Misc : 5.50g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVU5

Manual IntegrationsAPPROVED

Quant Time: Aug 30 11:58:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 30 07:05:43 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/10/2022
 Supervised By :Mahesh Dadoda 09/10/2022

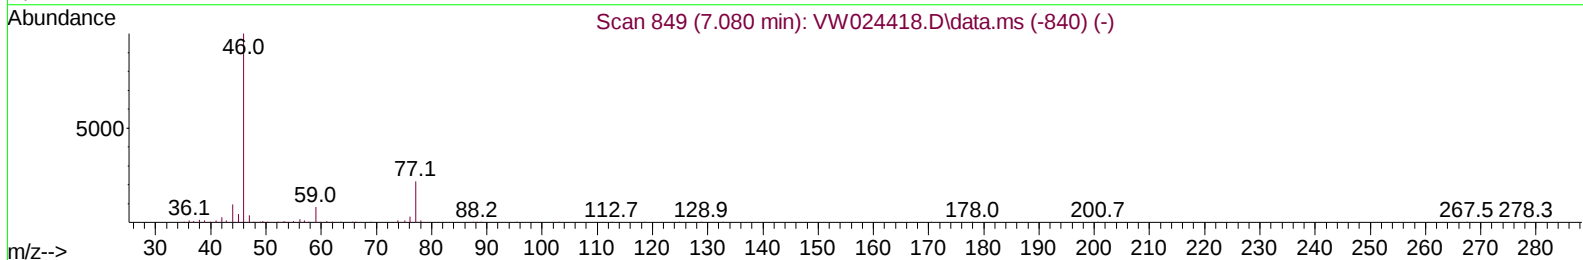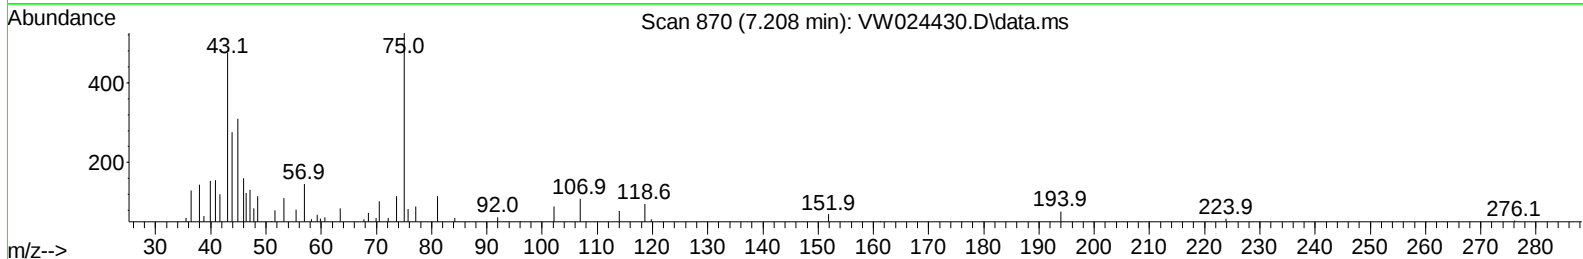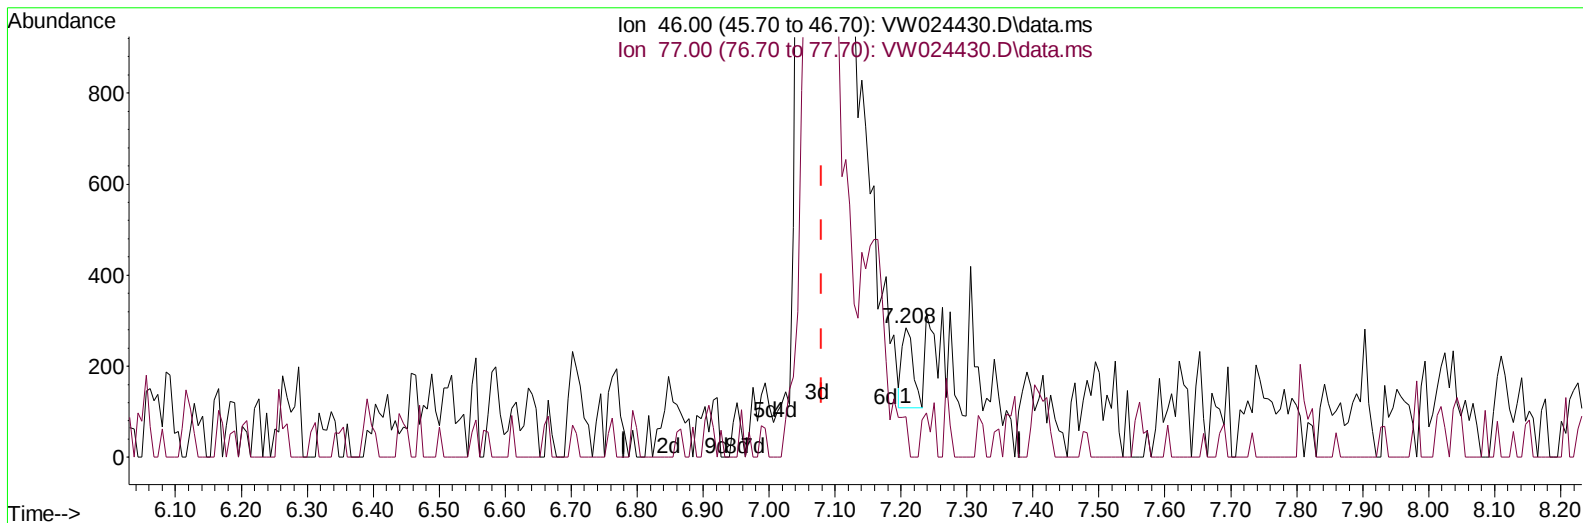

TIC: VW024430.D\data.ms

(21) 2-Butanone-d5 (S)

7.208min (+ 0.128) 0.23 ug/L

response 205

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	12.40	16.10
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
 Data File : VW024430.D
 Acq On : 28 Aug 2022 04:11
 Operator : SY/VA
 Sample : N4346-05
 Misc : 5.50g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVU5

Manual IntegrationsAPPROVED

Quant Time: Aug 30 11:58:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 30 07:05:43 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/10/2022
 Supervised By :Mahesh Dadoda 09/10/2022

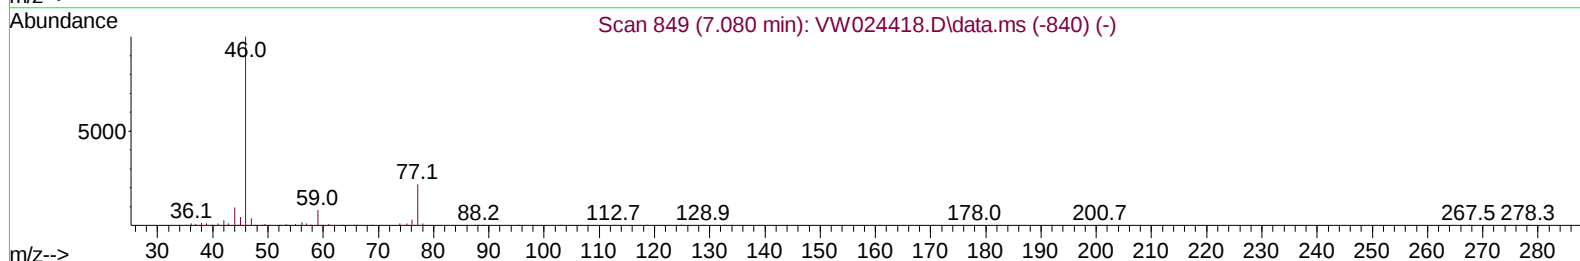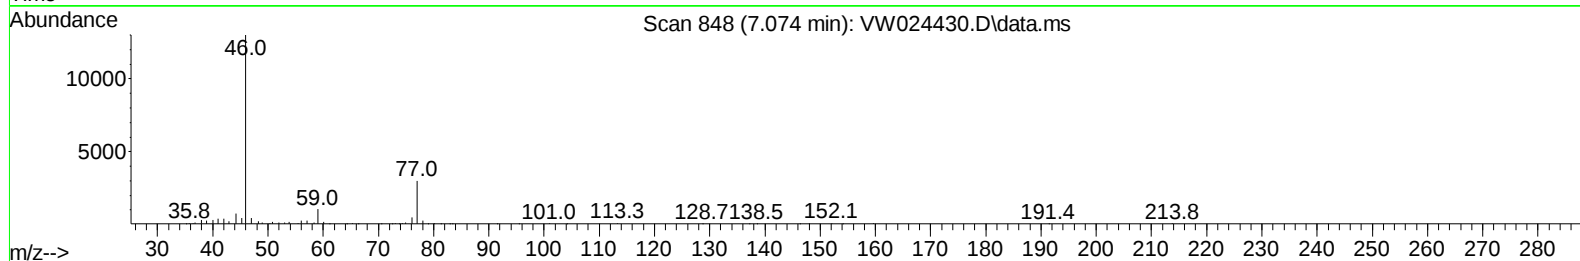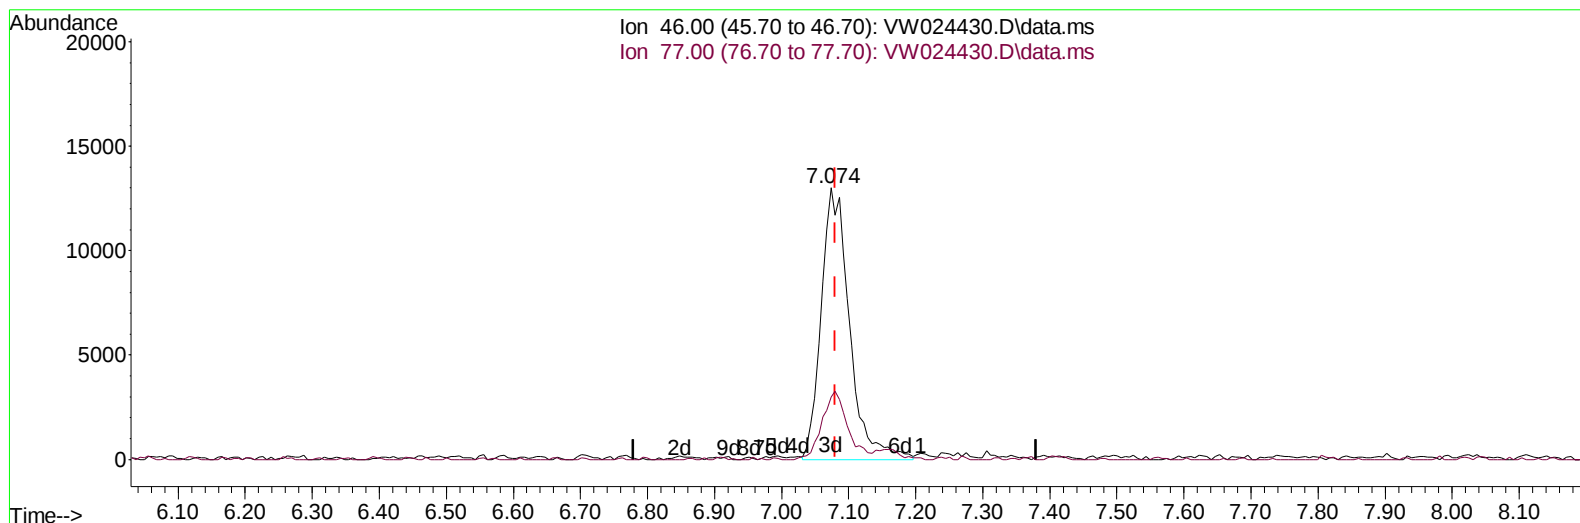

TIC: VW024430.D\data.ms

(21) 2-Butanone-d5 (S)

7.074min (-0.006) 42.40 ug/L m

response 38012

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	12.40	0.09#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
 Data File : VW024430.D
 Acq On : 28 Aug 2022 04:11
 Operator : SY/VA
 Sample : N4346-05
 Misc : 5.50g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVU5

Manual IntegrationsAPPROVED

Quant Time: Aug 30 11:58:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 30 07:05:43 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/10/2022
 Supervised By :Mahesh Dadoda 09/10/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		176564	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		173396	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		75295	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.343	65		149966	30.812	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	123.240%	
7) Chloroethane-d5	2.873	69		98120	26.907	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	107.640%	
11) 1,1-Dichloroethene-d2	4.001	63		76376	18.094	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	72.360%	
21) 2-Butanone-d5	7.074	46		38012m	42.402	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	84.800%	
24) Chloroform-d	7.647	84		111643	19.668	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	78.680%	
26) 1,2-Dichloroethane-d4	8.305	65		69066	20.064	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	80.240%	
32) Benzene-d6	8.269	84		208717	21.009	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	84.040%	
36) 1,2-Dichloropropane-d6	9.268	67		63257	20.474	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	81.880%	
41) Toluene-d8	10.323	98		194744	20.617	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	82.480%	
43) trans-1,3-Dichloroprop...	10.579	79		23379	16.169	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	64.680%	
47) 2-Hexanone-d5	10.921	63		29069	42.043	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	84.080%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84		63511	18.156	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	72.640%	
66) 1,2-Dichlorobenzene-d4	13.853	152		59719	21.062	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	84.240%	
Target Compounds							
13) Acetone	4.117	43		3242m	6.060	ug/L	
46) Tetrachloroethene	10.860	164		181430	82.102	ug/L	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082622\
Data File : VW024430.D
Acq On : 28 Aug 2022 04:11
Operator : SY/VA
Sample : N4346-05
Misc : 5.50g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBVU5

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 09/10/2022
Supervised By :Mahesh Dadoda 09/10/2022

Quant Time: Aug 30 11:58:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Aug 30 07:05:43 2022
Response via : Initial Calibration

