


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082624\
Data File : VW030021.D
Acq On : 26 Aug 2024 10:43
Operator : SY/MD
Sample : BFB551
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB551

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
Title : SFAM01.0
Last Update : Tue Aug 27 05:31:07 2024

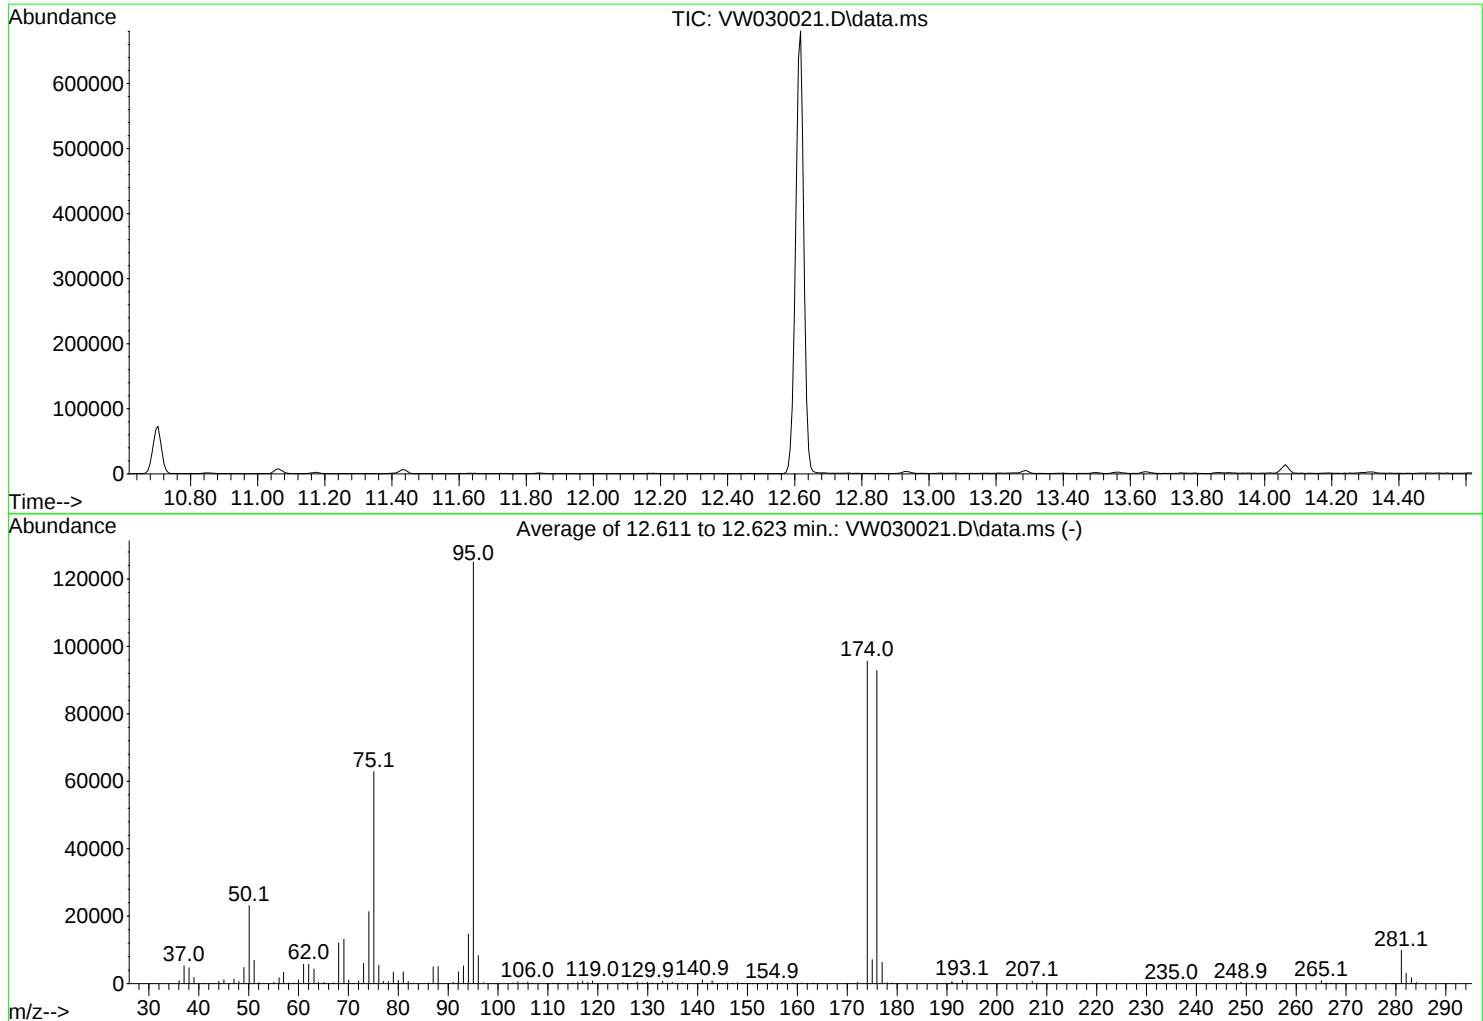

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	23173	PASS
75	95	30	80	50.3	62861	PASS
95	95	100	100	100.0	125067	PASS
96	95	5	9	6.6	8305	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	76.4	95600	PASS
175	174	5	9	7.4	7116	PASS
176	174	95	101	97.1	92864	PASS
177	176	5	9	6.8	6312	PASS

Scan 1751 (12.562 min): VW030021.D\data.ms
BFB551

m/z	Abundance
39.90	180.0
44.00	160.0

Instrument :
MSVOA_W
ClientSampleId :
BFB551

m/z	Abundance
36.00	1061.0
37.00	5863.0
38.00	5265.0
39.10	1947.0
40.00	129.0
43.10	164.0
44.10	1019.0
45.10	1525.0
46.00	99.0
46.20	93.0
47.10	1728.0
48.00	698.0
49.10	5133.0
50.10	24224.0
51.10	7223.0
52.00	304.0
53.00	73.0
55.00	469.0
56.10	1730.0
57.00	3685.0
58.00	200.0
59.10	240.0
60.00	1243.0
61.00	5893.0
62.10	6107.0
63.10	4640.0
64.10	601.0
65.10	472.0
66.10	63.0
67.00	364.0
68.10	13254.0
69.10	14287.0
70.00	1204.0
71.00	80.0
72.00	693.0
73.00	7028.0
74.10	22112.0
75.10	65992.0
76.10	6029.0
77.00	690.0
78.10	569.0
79.00	3731.0
80.00	1015.0
81.00	3681.0
82.00	664.0
83.10	121.0
86.00	230.0
87.00	5482.0
88.00	5377.0
91.00	565.0
92.10	3843.0
93.10	5516.0
94.00	15226.0
95.00	132288.0
96.10	8726.0
97.10	299.0
103.10	312.0
103.90	534.0
105.00	231.0
106.00	472.0
106.90	147.0
110.10	143.0
111.00	286.0
111.80	149.0
112.90	157.0
115.00	194.0
116.00	511.0
116.90	809.0
117.90	602.0
119.00	993.0
120.70	50.0
123.80	99.0
125.00	498.0
126.00	177.0
126.90	95.0
128.00	519.0
128.90	246.0
130.00	432.0
131.00	159.0
132.10	75.0
133.00	1291.0
134.00	386.0
134.90	404.0
135.90	61.0
136.90	274.0
141.00	1140.0
142.00	140.0
142.90	1298.0
144.10	83.0
145.10	147.0
145.90	232.0
147.00	240.0

Instrument :
MSVOA_W
ClientSampleId :
BFB551

147.90	327.0
148.90	183.0
149.90	51.0
151.00	52.0
153.00	151.0
154.00	63.0
155.00	226.0
157.00	269.0
159.00	245.0
160.90	212.0
161.90	64.0
162.90	273.0
164.00	56.0
165.00	149.0
170.80	87.0
172.10	556.0
174.00	88680.0
175.00	7229.0
175.90	82376.0
177.00	5835.0
178.10	350.0
179.00	398.0
189.10	156.0
190.00	99.0
190.90	1507.0
192.10	357.0
193.10	1869.0
194.00	293.0
195.00	224.0
203.10	236.0
205.20	323.0
205.90	82.0
207.10	1199.0
208.20	188.0
208.90	168.0
235.00	153.0
248.90	1115.0
250.10	329.0
251.00	455.0
252.00	78.0
253.00	64.0
265.10	1460.0
266.10	394.0
266.90	349.0
267.20	367.0
268.20	80.0
278.40	100.0
279.20	91.0
281.10	14921.0
282.10	5329.0
283.10	2557.0
284.10	647.0
285.30	142.0

Instrument :
MSVOA_W
ClientSampleId :
BFB551

m/z	Abundance
36.10	866.0
37.10	5818.0
38.00	5211.0
39.10	2003.0
39.90	175.0
42.90	122.0
44.10	864.0
45.00	1262.0
46.10	106.0
47.00	1414.0
48.10	823.0
49.00	5204.0
50.10	26752.0
51.10	8032.0
52.00	317.0
53.00	70.0
55.10	420.0
56.10	2037.0
57.00	3700.0
58.10	160.0
59.00	114.0
60.00	1243.0
61.00	6602.0
62.10	6327.0
63.10	4748.0
64.00	408.0
65.10	412.0
66.90	300.0
68.00	13168.0
69.10	14560.0
70.00	1086.0
71.00	78.0
72.10	872.0
73.10	6295.0
74.10	23456.0
75.10	69632.0
76.10	5665.0
77.00	820.0
77.90	588.0
79.00	3814.0
80.00	1081.0
81.00	3585.0
82.00	676.0
83.10	156.0
86.00	148.0
87.00	5678.0
88.00	5727.0
91.00	411.0
92.00	3665.0
93.00	6118.0
94.00	16568.0
95.10	138112.0
96.10	9044.0
97.10	319.0
103.00	220.0
104.00	596.0
105.00	247.0
105.90	494.0
106.80	141.0
109.80	116.0
111.10	216.0
111.80	118.0
112.90	108.0
114.90	212.0
116.00	346.0
117.00	958.0
117.90	468.0
119.00	831.0
123.90	95.0
125.00	333.0
126.00	132.0
126.80	77.0
127.80	523.0
129.00	263.0
129.90	539.0
131.00	239.0
132.20	56.0
133.00	657.0
133.90	196.0
135.00	341.0
136.00	86.0
136.90	197.0
140.10	106.0
141.00	1311.0
142.00	215.0
142.90	1388.0
144.10	80.0
144.80	117.0
146.00	204.0
147.10	181.0
148.00	272.0
149.10	130.0

Instrument :
MSVOA_W
ClientSampleId :
BFB551

149.80	115.0
151.90	72.0
152.80	109.0
153.90	80.0
154.90	312.0
156.00	65.0
156.90	214.0
159.00	185.0
160.90	160.0
163.00	147.0
165.10	163.0
170.80	75.0
172.20	431.0
174.00	107576.0
175.00	7905.0
176.00	104504.0
177.00	7499.0
178.00	297.0
179.10	153.0
189.20	52.0
190.20	52.0
191.10	859.0
193.10	887.0
194.10	194.0
195.10	81.0
203.00	72.0
205.00	169.0
205.80	50.0
207.10	714.0
208.00	155.0
209.20	90.0
235.00	126.0
249.10	572.0
250.00	121.0
251.10	220.0
253.00	78.0
265.00	898.0
265.90	188.0
267.10	189.0
267.80	61.0
269.10	51.0
278.50	52.0
279.70	119.0
281.10	10109.0
282.00	2728.0
283.10	1746.0
284.10	330.0
285.10	100.0

Instrument :
MSVOA_W
ClientSampleId :
BFB551

m/z	Abundance
36.10	741.0
37.00	4173.0
38.10	3685.0
39.00	1626.0
40.10	186.0
40.90	62.0
43.10	67.0
44.00	630.0
45.10	846.0
46.00	65.0
47.10	1037.0
48.00	517.0
49.10	4093.0
50.10	18544.0
51.10	5410.0
52.10	235.0
53.00	55.0
55.00	275.0
56.10	1464.0
57.00	2910.0
58.00	133.0
59.10	53.0
60.00	992.0
61.00	4706.0
62.00	4857.0
63.10	3550.0
63.90	284.0
65.10	286.0
66.20	59.0
67.00	254.0
68.00	9840.0
69.10	10715.0
70.10	919.0
71.00	142.0
72.00	591.0
73.00	4794.0
74.10	18432.0
75.10	52960.0
76.10	4547.0
77.00	685.0
77.90	358.0
79.00	2796.0
80.00	845.0
81.00	3210.0
82.00	532.0
83.00	98.0
86.10	171.0
87.00	3784.0
88.00	4106.0
91.00	346.0
92.00	3075.0
93.00	4136.0
94.10	12249.0
95.10	104800.0
96.00	7145.0
97.10	185.0
102.90	150.0
103.90	414.0
105.00	208.0
105.90	472.0
107.00	110.0
110.00	85.0
111.00	83.0
111.70	81.0
112.10	55.0
112.90	87.0
114.90	140.0
116.00	303.0
117.00	558.0
118.10	439.0
118.90	637.0
123.90	97.0
124.90	92.0
125.60	64.0
127.90	372.0
129.00	198.0
130.00	364.0
130.90	165.0
133.10	368.0
135.00	219.0
136.00	54.0
137.00	219.0
140.90	910.0
141.90	133.0
143.10	928.0
145.10	93.0
145.90	155.0
146.90	131.0
148.10	239.0
148.80	84.0
149.80	78.0
150.20	77.0

Instrument :
MSVOA_W
ClientSampleId :
BFB551

152.00	66.0
153.00	90.0
154.00	96.0
155.00	278.0
156.10	53.0
156.90	193.0
159.00	81.0
160.90	145.0
163.20	87.0
165.20	56.0
170.00	54.0
172.00	343.0
174.00	90544.0
175.00	6213.0
176.00	91712.0
177.00	5601.0
178.00	159.0
179.00	74.0
191.10	236.0
192.00	51.0
192.90	211.0
194.20	60.0
205.10	53.0
207.00	334.0
208.10	117.0
249.00	299.0
250.10	79.0
251.00	77.0
265.00	360.0
265.70	77.0
267.00	109.0
281.00	4534.0
282.10	1270.0
283.10	822.0
283.80	130.0
285.20	76.0

Instrument :
MSVOA_W
ClientSampleId :
BFB551