

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082724\
 Data File : VW030031.D
 Acq On : 27 Aug 2024 09:23
 Operator : SY/MD
 Sample : VW0827SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Aug 28 01:12:11 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 28 01:11:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	297854	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	271473	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	124157	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	101323	22.859	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.440%
7) Chloroethane-d5	2.899	69	71686	22.787	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.160%
11) 1,1-Dichloroethene-d2	4.021	65	43669	23.060	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	92.240%
21) 2-Butanone-d5	7.081	46	41618	47.102	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	94.200%
24) Chloroform-d	7.648	84	183142	22.801	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.200%
26) 1,2-Dichloroethane-d4	8.307	65	99297	24.346	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	97.400%
32) Benzene-d6	8.270	84	374147	23.349	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	93.400%
36) 1,2-Dichloropropane-d6	9.270	67	112674	24.000	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	96.000%
41) Toluene-d8	10.325	98	340420	23.340	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	93.360%
43) trans-1,3-Dichloroprop...	10.575	79	44709	23.151	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	92.600%
47) 2-Hexanone-d5	10.922	63	34364	47.825	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	95.660%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	85162	24.637	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	98.560%
66) 1,2-Dichlorobenzene-d4	13.854	152	107203	23.872	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.480%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.038	75	3270	0.482	ug/L	# 77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082724\
Data File : VW030031.D
Acq On : 27 Aug 2024 09:23
Operator : SY/MD
Sample : VW0827SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Aug 28 01:12:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Aug 28 01:11:30 2024
Response via : Initial Calibration

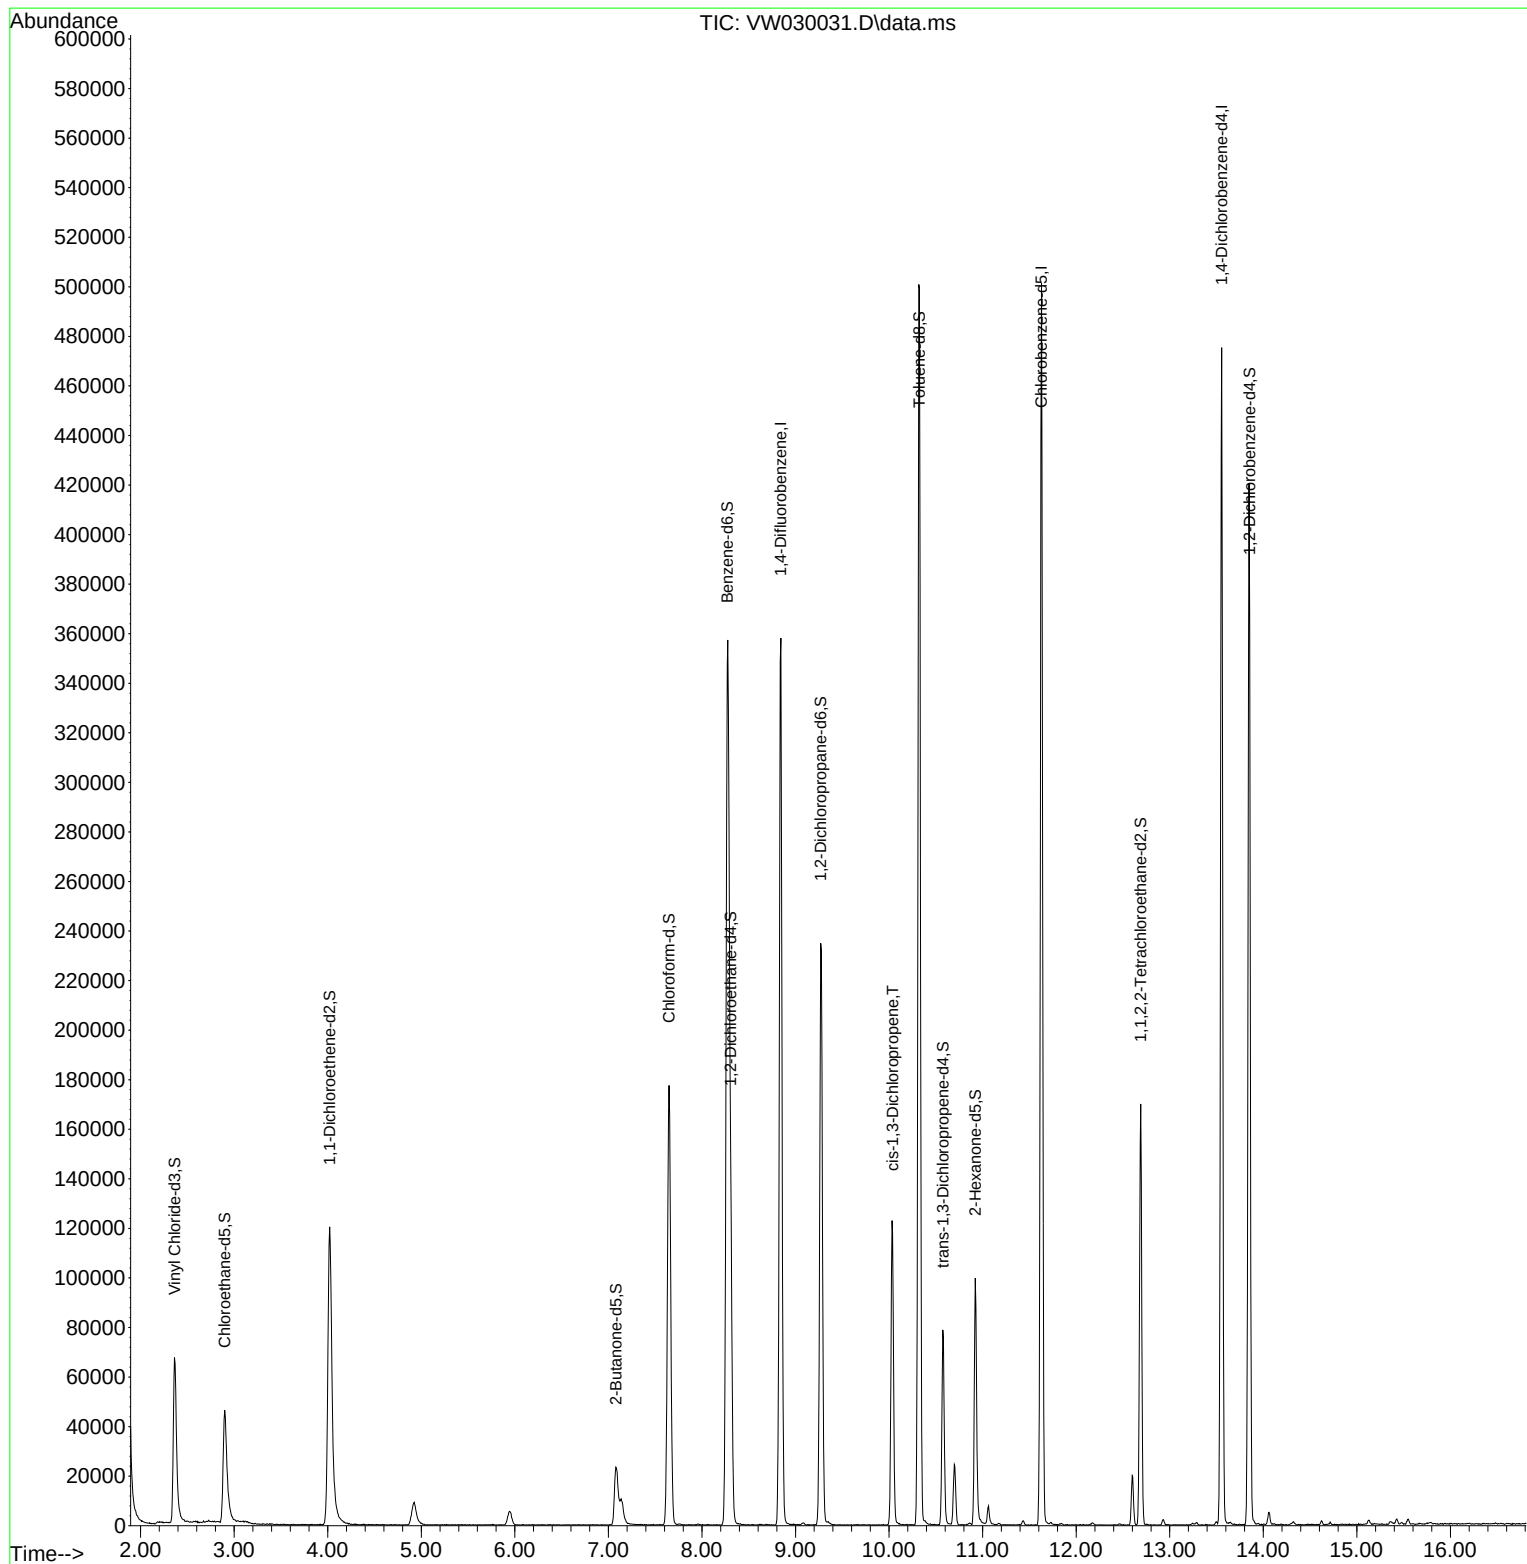

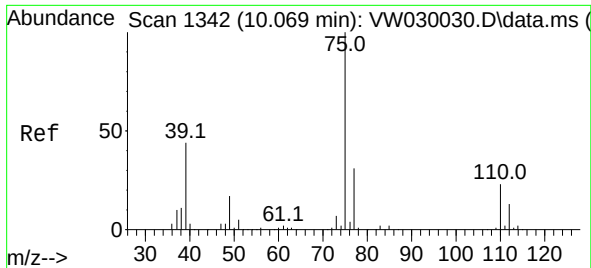

#39
 cis-1,3-Dichloropropene
 Concen: 0.482 ug/L
 RT: 10.038 min Scan# 14
 Delta R.T. -0.031 min
 Lab File: VW030031.D
 Acq: 27 Aug 2024 09:23

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 3270
 Ion Ratio Lower Upper
 75 100
 77 45.3 22.8 42.4#

