




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082724\
Data File : VW030040.D
Acq On : 27 Aug 2024 13:33
Operator : SY/MD
Sample : P3675-17
Misc : 5.10g/10mL/MSVOA_W/SOIL/A
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCXZ1

Manual IntegrationsAPPROVED

Quant Time: Aug 28 01:14:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Aug 28 01:11:30 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 08/28/2024
Supervised By :Mahesh Dadoda 08/28/2024

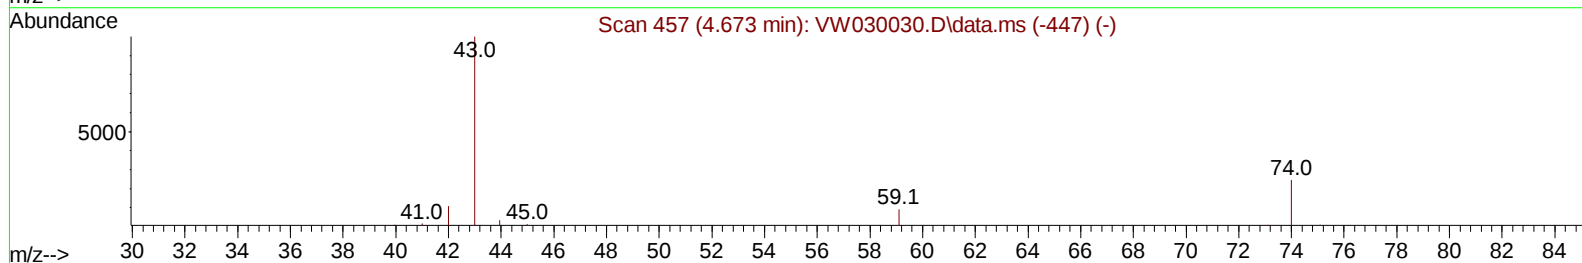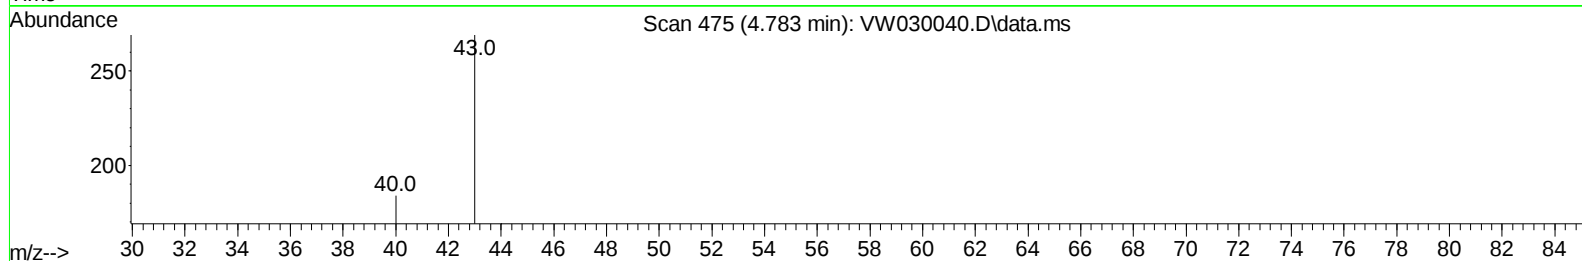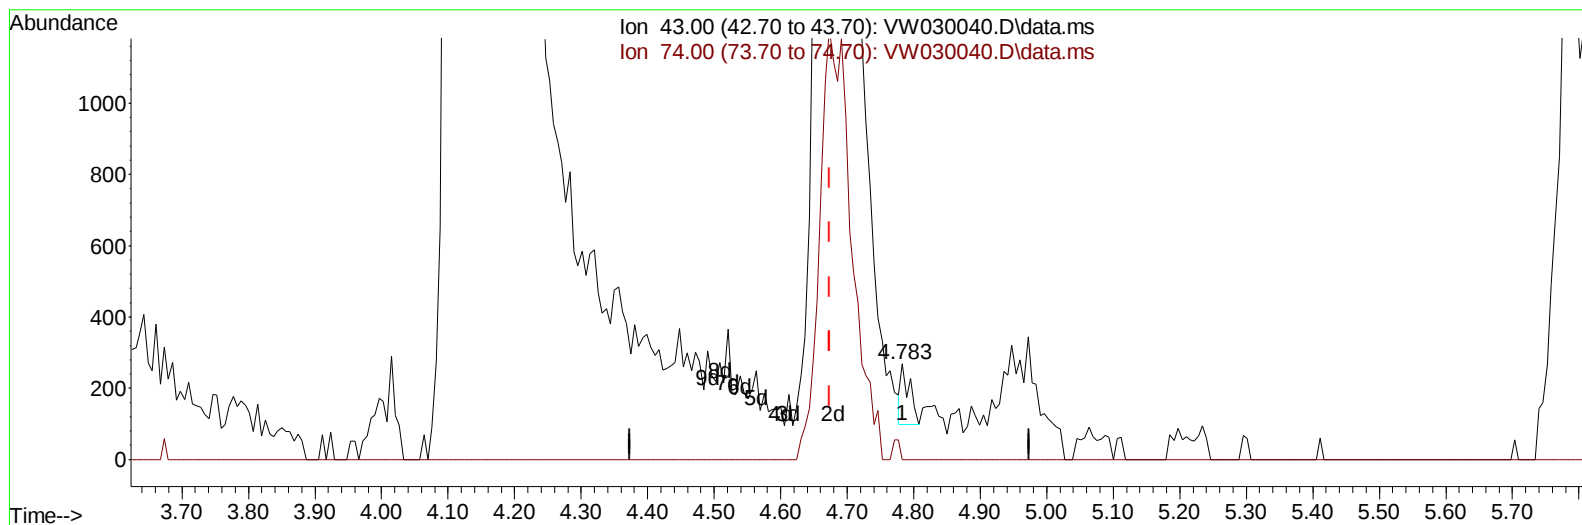

TIC: VW030040.D\data.ms

(15) Methyl Acetate (T)

4.783min (+ 0.110) 0.11 ug/L

response 155

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	24.90	26.45
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082724\
Data File : VW030040.D
Acq On : 27 Aug 2024 13:33
Operator : SY/MD
Sample : P3675-17
Misc : 5.10g/10mL/MSVOA_W/SOIL/A
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCXZ1

Manual IntegrationsAPPROVED

Quant Time: Aug 28 01:14:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Aug 28 01:11:30 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 08/28/2024
Supervised By :Mahesh Dadoda 08/28/2024

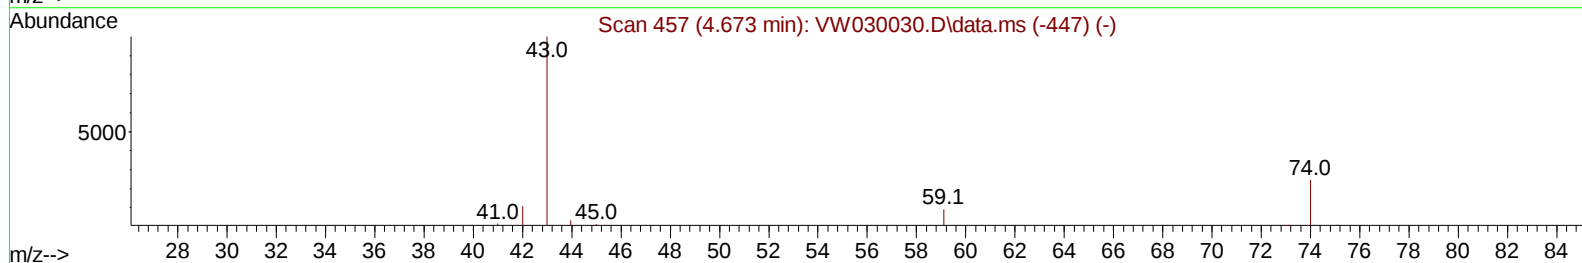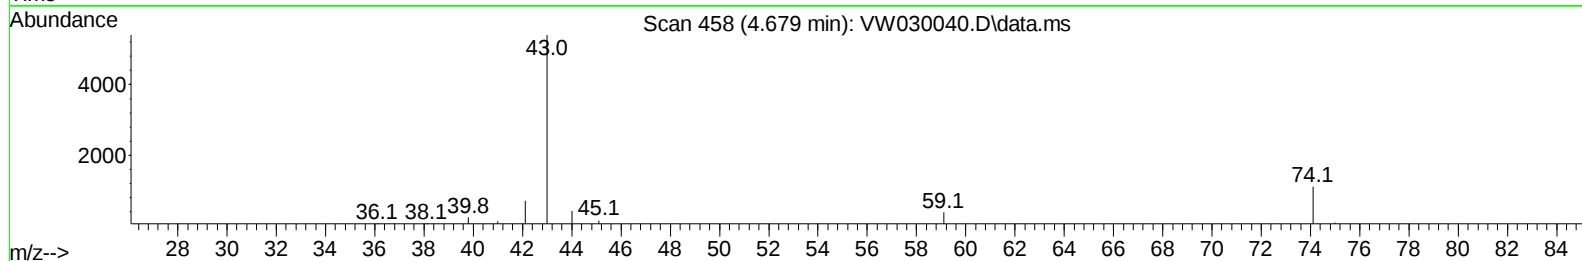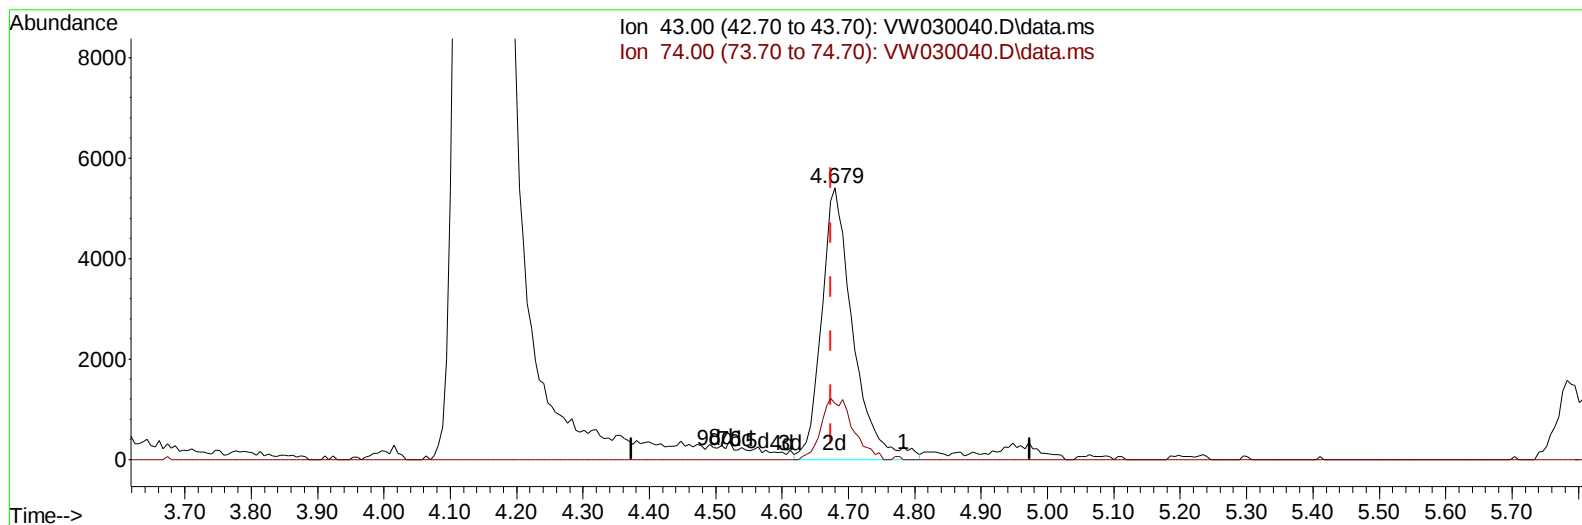

TIC: VW030040.D\data.ms

(15) Methyl Acetate (T)

4.679min (+ 0.006) 12.40 ug/L m

response 17656

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	24.90	0.23#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082724\
 Data File : VW030040.D
 Acq On : 27 Aug 2024 13:33
 Operator : SY/MD
 Sample : P3675-17
 Misc : 5.10g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCXZ1

Manual IntegrationsAPPROVED

Quant Time: Aug 28 01:14:22 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 28 01:11:30 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 08/28/2024
 Supervised By :Mahesh Dadoda 08/28/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	269203	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	168262	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	41882	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	87224	21.773	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	87.080%	
7) Chloroethane-d5	2.899	69	58478	20.567	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	82.280%	
11) 1,1-Dichloroethene-d2	4.021	65	37246	21.761	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	87.040%	
21) 2-Butanone-d5	7.087	46	44753	56.041	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	112.080%	
24) Chloroform-d	7.648	84	148952	20.518	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	82.080%	
26) 1,2-Dichloroethane-d4	8.301	65	85009	23.061	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	92.240%	
32) Benzene-d6	8.270	84	292313	29.431	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	117.720%	
36) 1,2-Dichloropropane-d6	9.270	67	92076	31.643	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	126.560%#	
41) Toluene-d8	10.325	98	224388	24.822	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	99.280%	
43) trans-1,3-Dichloroprop...	10.575	79	33071	27.629	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	110.520%	
47) 2-Hexanone-d5	10.922	63	36217	81.322	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	162.640%#	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	52343	24.431	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	97.720%	
66) 1,2-Dichlorobenzene-d4	13.848	152	27162	17.930	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	71.720%#	
Target Compounds						
						Qvalue
13) Acetone	4.143	43	251652	344.528	ug/L	97
15) Methyl Acetate	4.679	43	17656m	12.398	ug/L	
16) Methylene chloride	4.917	84	25434	5.719	ug/L	96
22) 2-Butanone	7.185	43	16390	15.681	ug/L	97
42) Toluene	10.386	91	81859	7.130	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082724\
Data File : VW030040.D
Acq On : 27 Aug 2024 13:33
Operator : SY/MD
Sample : P3675-17
Misc : 5.10g/10mL/MSVOA_W/SoIL/A
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCXZ1

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 08/28/2024
Supervised By :Mahesh Dadoda 08/28/2024

Quant Time: Aug 28 01:14:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Aug 28 01:11:30 2024
Response via : Initial Calibration

