




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082724\
Data File : VW030058.D
Acq On : 27 Aug 2024 22:22
Operator : SY/MD
Sample : P3733-14
Misc : 7.17g/10mL/MSVOA_W/SOIL/A
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A44A6

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 08/28/2024
Supervised By :Mahesh Dadoda 08/28/2024

Quant Time: Aug 28 02:45:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Aug 28 02:43:49 2024
Response via : Initial Calibration

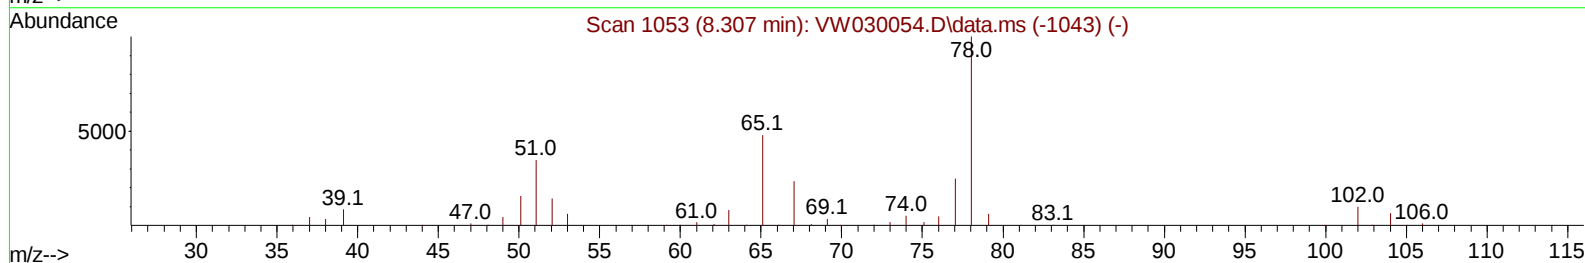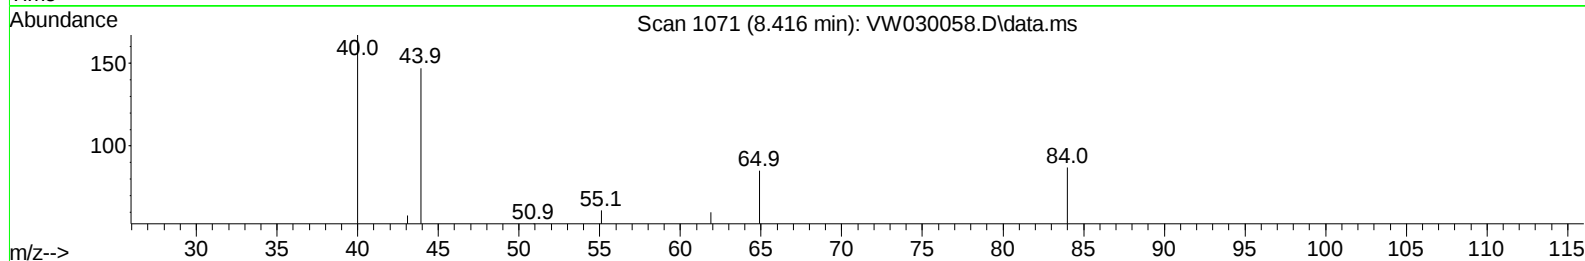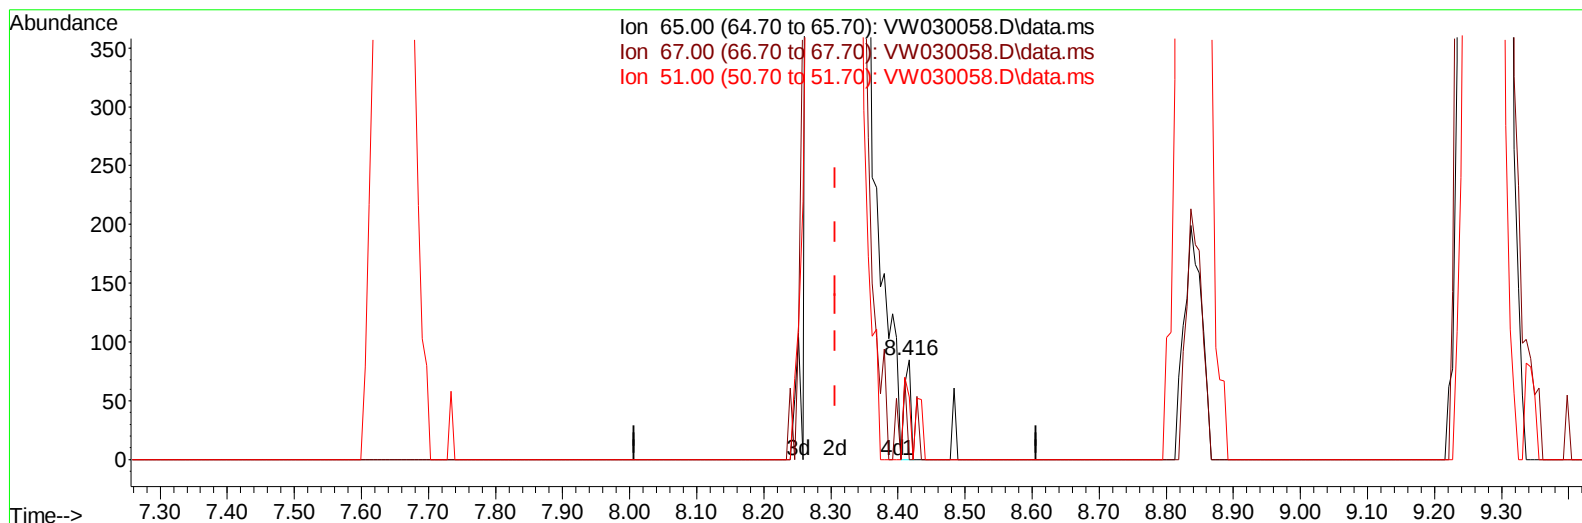

TIC: VW030058.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.416min (+ 0.110) 0.01 ug/L

response 55

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.00	45.45
51.00	108.00	81.82
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082724\
Data File : VW030058.D
Acq On : 27 Aug 2024 22:22
Operator : SY/MD
Sample : P3733-14
Misc : 7.17g/10mL/MSVOA_W/SOIL/A
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A44A6

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 08/28/2024
Supervised By :Mahesh Dadoda 08/28/2024

Quant Time: Aug 28 02:45:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Aug 28 02:43:49 2024
Response via : Initial Calibration

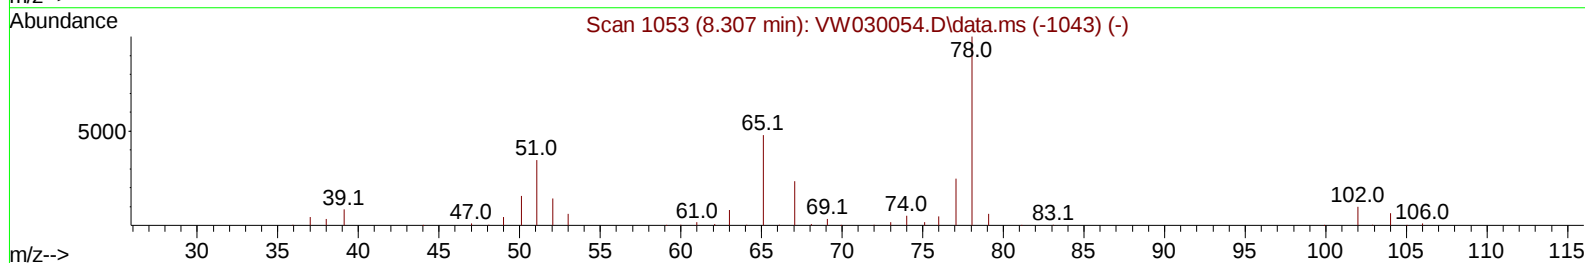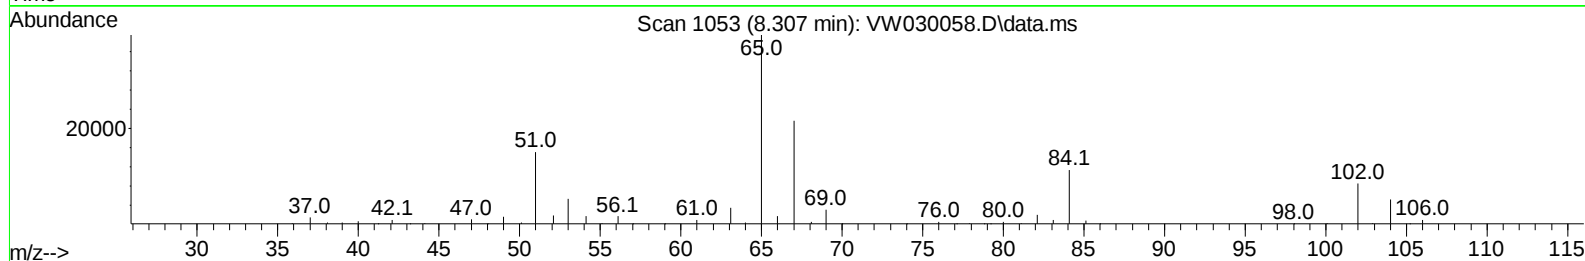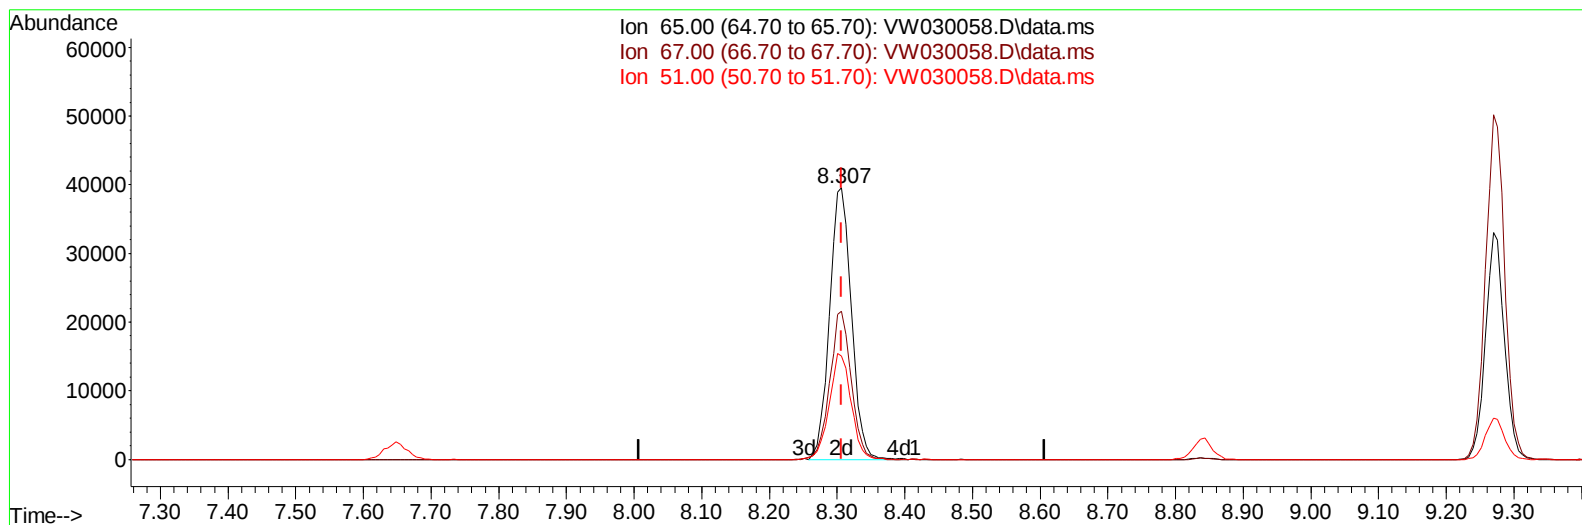

TIC: VW030058.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (+ 0.000) 22.80 ug/L m

response 88819

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.00	0.03#
51.00	108.00	0.05#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082724\
 Data File : VW030058.D
 Acq On : 27 Aug 2024 22:22
 Operator : SY/MD
 Sample : P3733-14
 Misc : 7.17g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A44A6

Manual IntegrationsAPPROVED

Quant Time: Aug 28 02:45:14 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 28 02:43:49 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 08/28/2024
 Supervised By :Mahesh Dadoda 08/28/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	284528	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	249666	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	85852	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	73666	17.398	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	69.600%	
7) Chloroethane-d5	2.899	69	56087	18.664	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	74.640%	
11) 1,1-Dichloroethene-d2	4.021	65	34761	19.215	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	76.880%	
21) 2-Butanone-d5	7.087	46	49964	59.196	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	118.400%	
24) Chloroform-d	7.648	84	150920	19.669	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	78.680%	
26) 1,2-Dichloroethane-d4	8.307	65	88819m	22.797	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	91.200%	
32) Benzene-d6	8.276	84	306862	20.823	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	83.280%	
36) 1,2-Dichloropropane-d6	9.270	67	99260	22.989	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	91.960%	
41) Toluene-d8	10.325	98	260079	19.389	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	77.560%	
43) trans-1,3-Dichloroprop...	10.575	79	38624	21.747	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	87.000%	
47) 2-Hexanone-d5	10.922	63	43394	65.668	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	131.340%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	82861	26.066	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	104.280%	
66) 1,2-Dichlorobenzene-d4	13.848	152	60600	19.515	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	78.080%	
Target Compounds						
					Qvalue	
13) Acetone	4.149	43	21822	28.267	ug/L	95
14) Carbon disulfide	4.393	76	14254	1.260	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082724\
Data File : VW030058.D
Acq On : 27 Aug 2024 22:22
Operator : SY/MD
Sample : P3733-14
Misc : 7.17g/10mL/MSVOA_W/SOIL/A
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A44A6

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 08/28/2024
Supervised By :Mahesh Dadoda 08/28/2024

Quant Time: Aug 28 02:45:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Aug 28 02:43:49 2024
Response via : Initial Calibration

