




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082724\
 Data File : VW030062.D
 Acq On : 27 Aug 2024 23:58
 Operator : SY/MD
 Sample : P3733-07
 Misc : 6.17g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A44A1

Manual IntegrationsAPPROVED

Quant Time: Aug 28 02:46:09 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 28 02:43:49 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 08/28/2024
 Supervised By :Mahesh Dadoda 08/28/2024

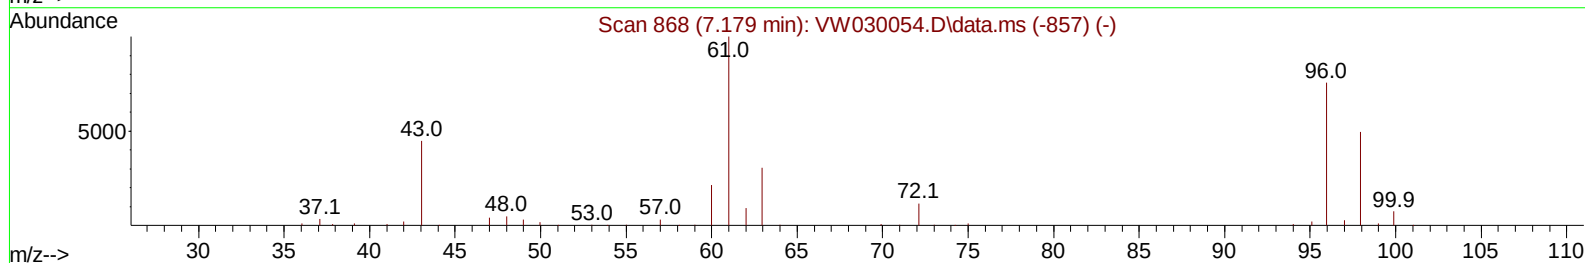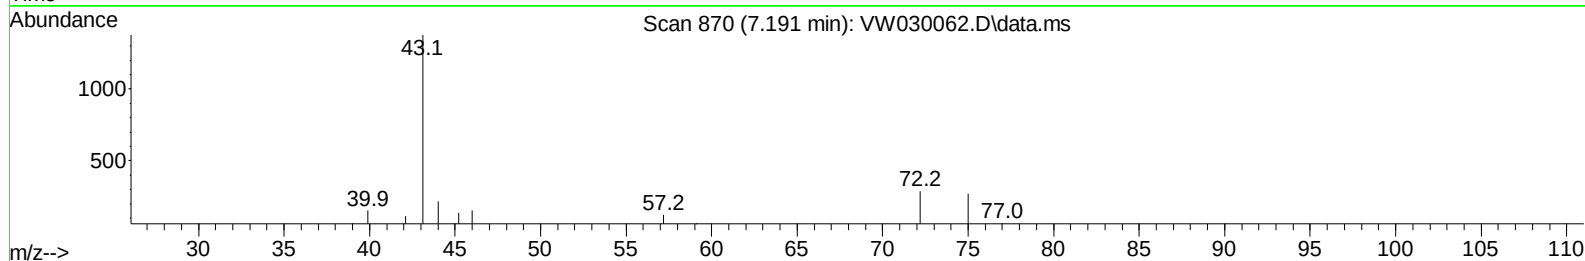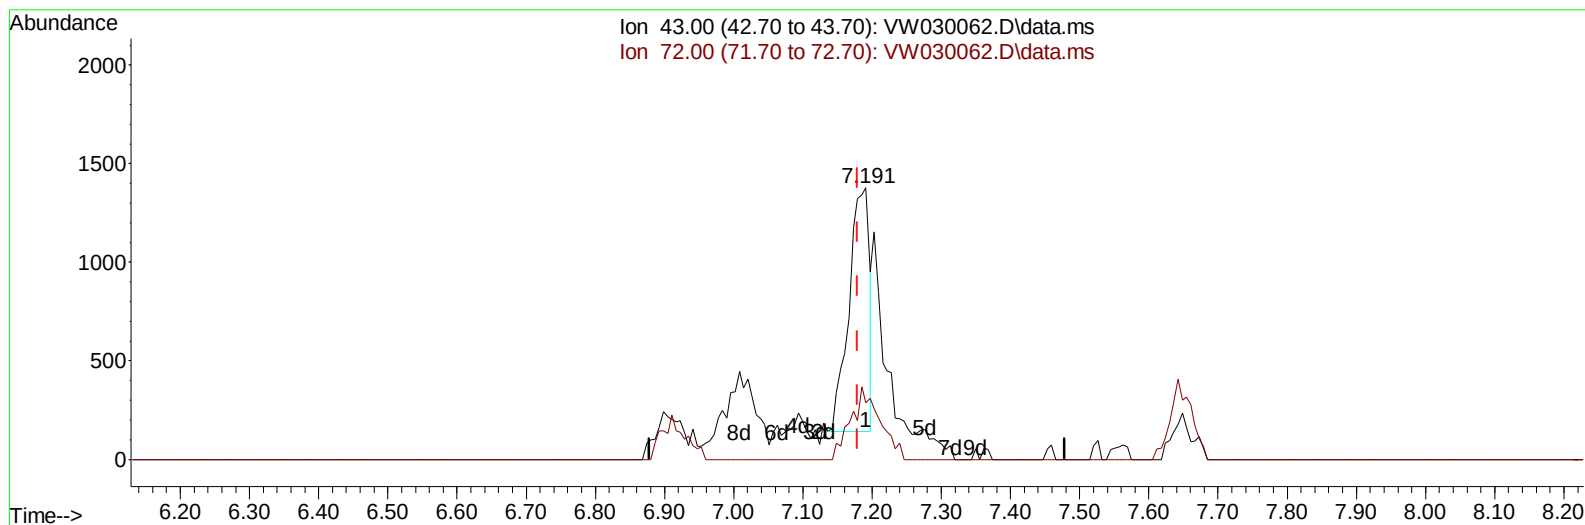

TIC: VW030062.D\data.ms

(22) 2-Butanone (T)

7.191min (+ 0.012) 3.65 ug/L

response 2556

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	30.10	28.52
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082724\
Data File : VW030062.D
Acq On : 27 Aug 2024 23:58
Operator : SY/MD
Sample : P3733-07
Misc : 6.17g/10mL/MSVOA_W/SOIL/A
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A44A1

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 08/28/2024
Supervised By :Mahesh Dadoda 08/28/2024

Quant Time: Aug 28 02:46:09 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Aug 28 02:43:49 2024
Response via : Initial Calibration

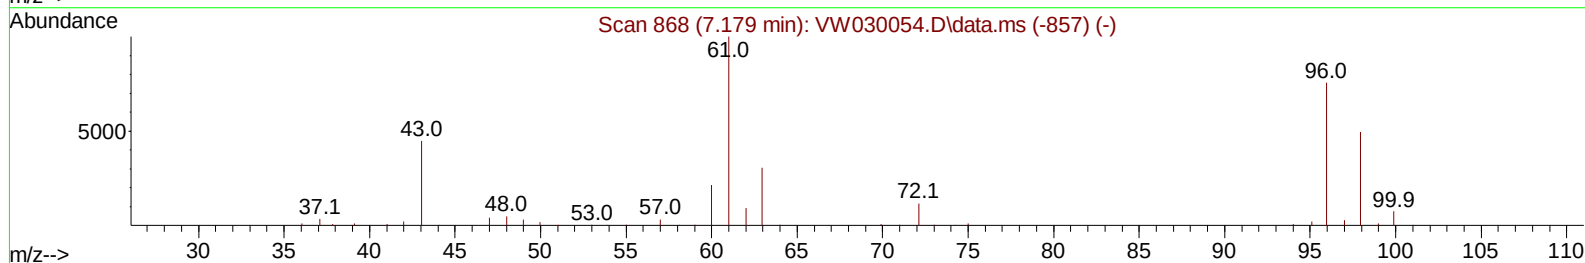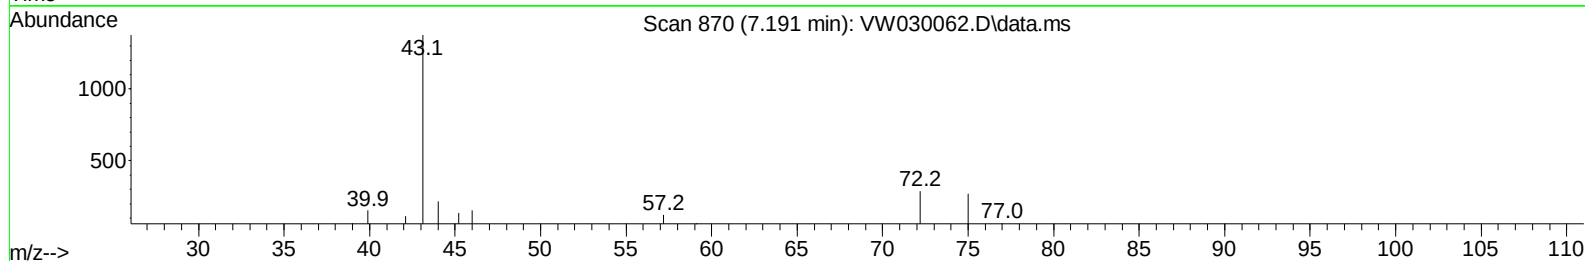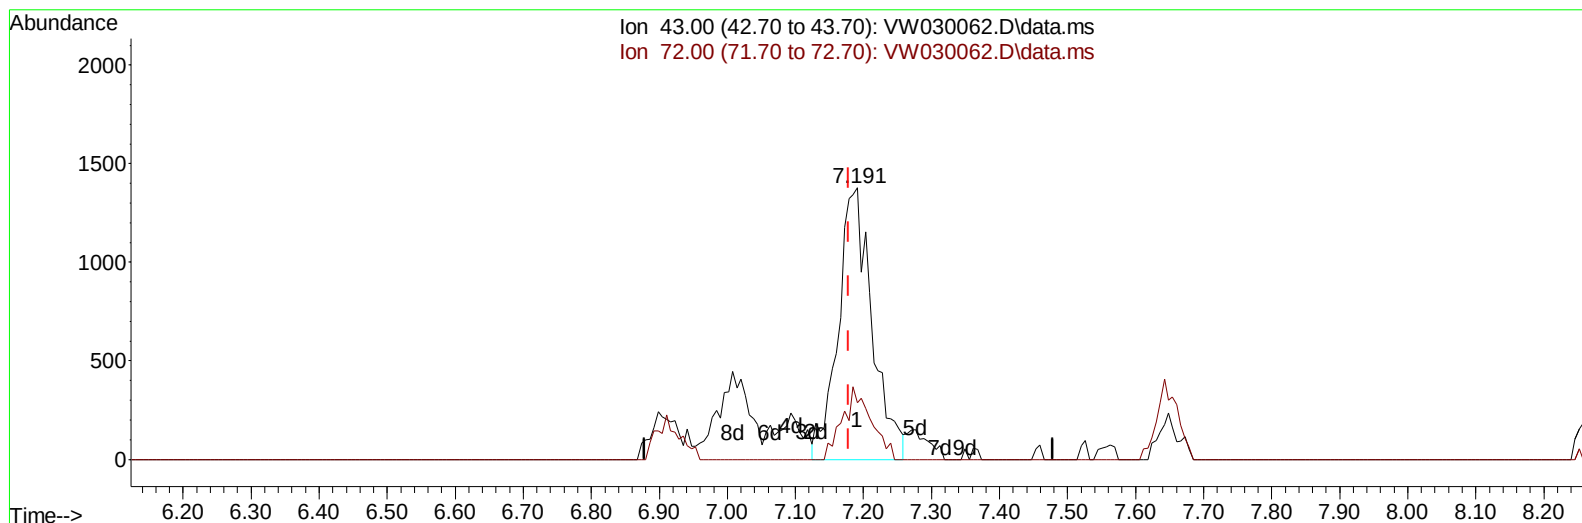

TIC: VW030062.D\data.ms

(22) 2-Butanone (T)

7.191min (+ 0.012) 6.78 ug/L m

response 4746

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	30.10	15.36
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082724\
 Data File : VW030062.D
 Acq On : 27 Aug 2024 23:58
 Operator : SY/MD
 Sample : P3733-07
 Misc : 6.17g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A44A1

Manual IntegrationsAPPROVED

Quant Time: Aug 28 02:46:09 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 28 02:43:49 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 08/28/2024
 Supervised By :Mahesh Dadoda 08/28/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		180213	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		100903	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		16694	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		70556	26.309	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	105.240%	
7) Chloroethane-d5	2.893	69		51347	26.977	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	107.920%	
11) 1,1-Dichloroethene-d2	4.015	65		29730	25.947	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110		Recovery	=	103.800%	
21) 2-Butanone-d5	7.081	46		42541	79.576	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	159.160%#	
24) Chloroform-d	7.642	84		123996	25.514	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	102.040%	
26) 1,2-Dichloroethane-d4	8.307	65		74916	30.359	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	121.440%	
32) Benzene-d6	8.276	84		226393	38.011	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	152.040%#	
36) 1,2-Dichloropropane-d6	9.270	67		77714	44.536	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	178.160%#	
41) Toluene-d8	10.318	98		154566	28.512	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	114.040%	
43) trans-1,3-Dichloroprop...	10.575	79		24218	33.739	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	134.960%	
47) 2-Hexanone-d5	10.922	63		30402	113.836	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	227.680%#	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		48108	37.445	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	149.760%#	
66) 1,2-Dichlorobenzene-d4	13.848	152		14004	23.192	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	92.760%	
Target Compounds							
13) Acetone	4.137	43		41848	85.584	ug/L	98
15) Methyl Acetate	4.691	43		1526	1.601	ug/L	93
22) 2-Butanone	7.191	43		4746m	6.783	ug/L	
30) 1,1,1-Trichloroethane	7.874	97		14780	6.254	ug/L	99
46) Tetrachloroethene	10.867	164		2106	1.594	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082724\
Data File : VW030062.D
Acq On : 27 Aug 2024 23:58
Operator : SY/MD
Sample : P3733-07
Misc : 6.17g/10mL/MSVOA_W/SoIL/A
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A44A1

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 08/28/2024
Supervised By :Mahesh Dadoda 08/28/2024

Quant Time: Aug 28 02:46:09 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Aug 28 02:43:49 2024
Response via : Initial Calibration

