




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082724\
 Data File : VW030063.D
 Acq On : 28 Aug 2024 00:22
 Operator : SY/MD
 Sample : P3733-08
 Misc : 9.13g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A44A2

Manual IntegrationsAPPROVED

Quant Time: Aug 28 02:46:27 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 28 02:43:49 2024
 Response via : Initial Calibration

Reviewed By :Romaben
 Patel

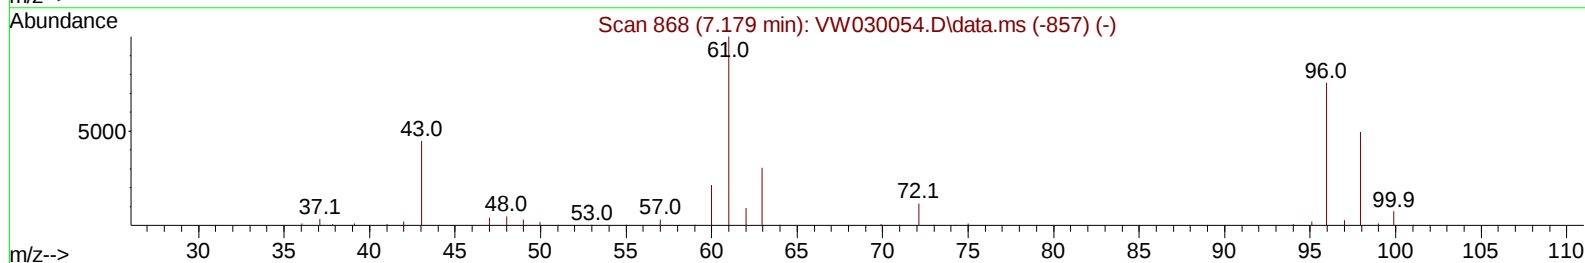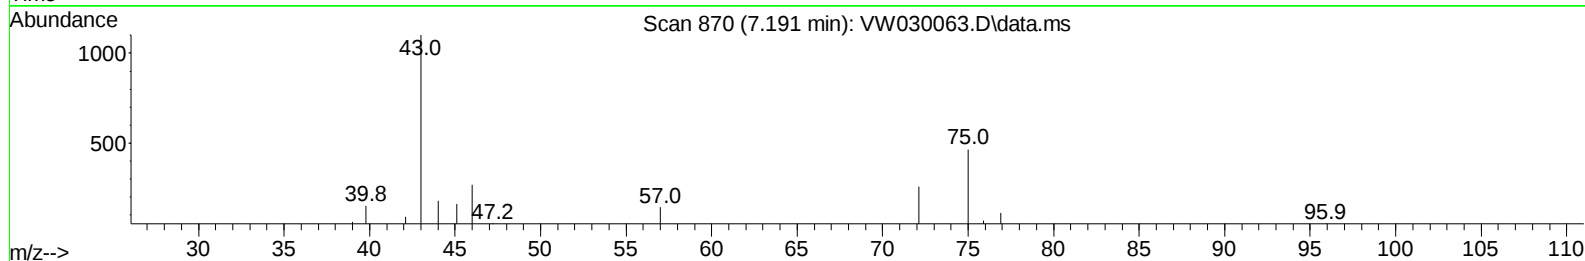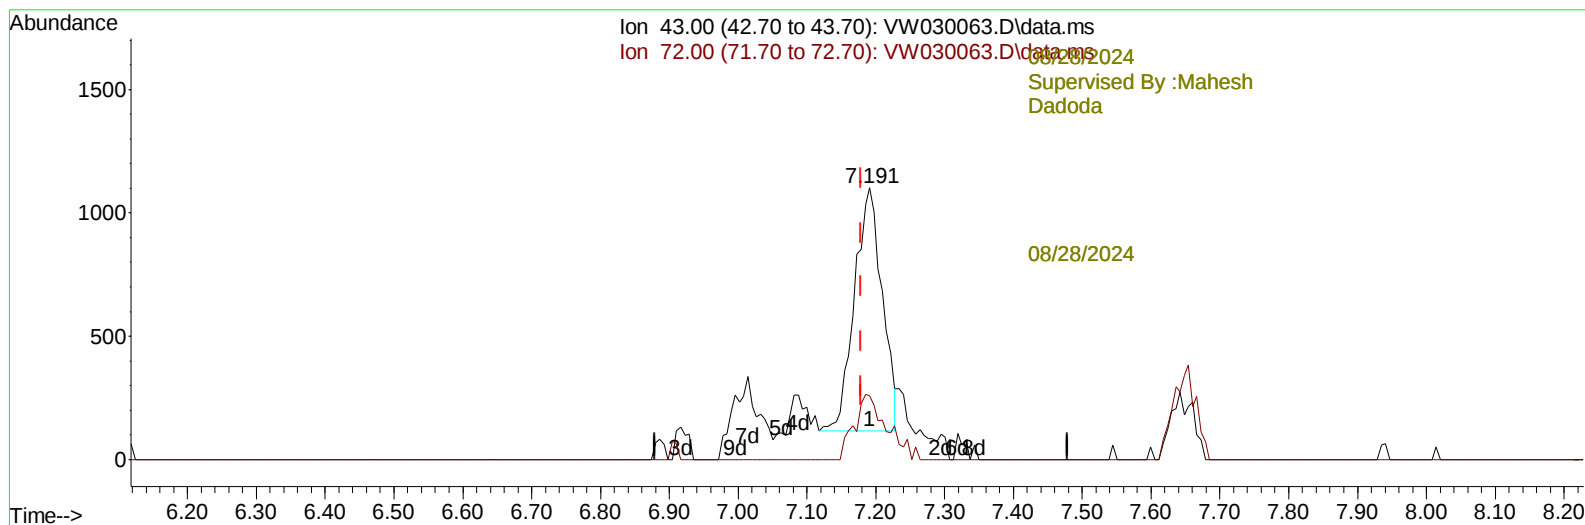

TIC: VW030063.D\data.ms

(22) 2-Butanone (T)

7.191min (+ 0.012) 2.76 ug/L

response 2756

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	30.10	20.03
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082724\
 Data File : VW030063.D
 Acq On : 28 Aug 2024 00:22
 Operator : SY/MD
 Sample : P3733-08
 Misc : 9.13g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A44A2

Manual IntegrationsAPPROVED

Quant Time: Aug 28 02:46:27 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 28 02:43:49 2024
 Response via : Initial Calibration

Reviewed By :Romaben
 Patel

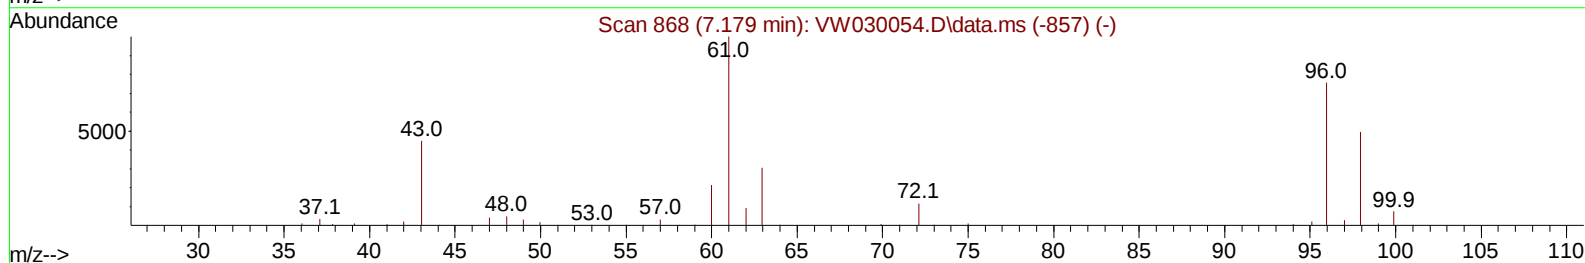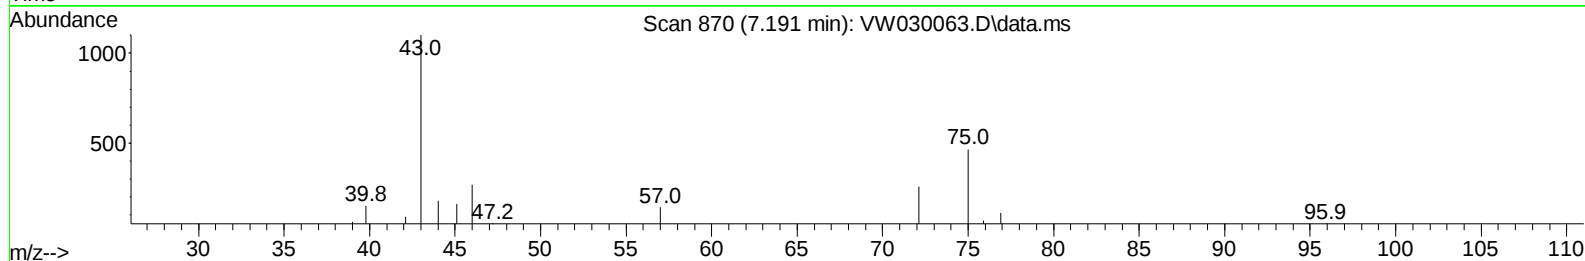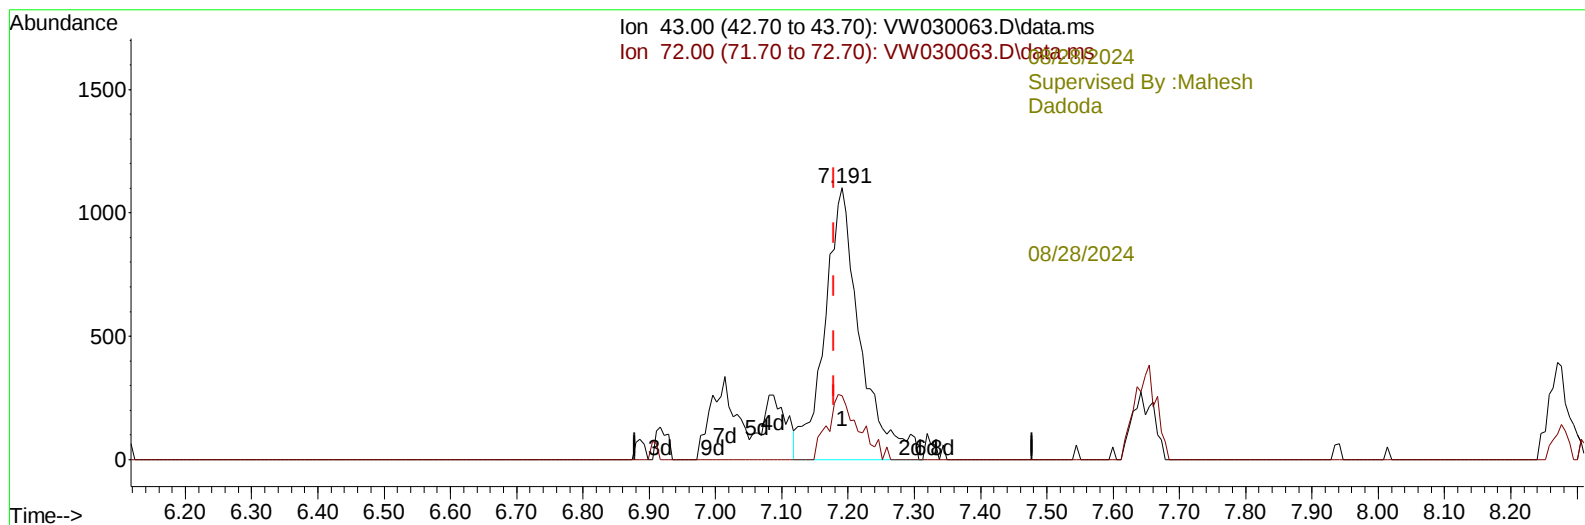

TIC: VW030063.D\data.ms

(22) 2-Butanone (T)

7.191min (+ 0.012) 4.12 ug/L m

response 4109

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	30.10	13.43#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082724\
 Data File : VW030063.D
 Acq On : 28 Aug 2024 00:22
 Operator : SY/MD
 Sample : P3733-08
 Misc : 9.13g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A44A2

Manual IntegrationsAPPROVED

Quant Time: Aug 28 02:46:27 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 28 02:43:49 2024
 Response via : Initial Calibration

Reviewed By :Romaben
 Patel

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)
-----08/28/2024							
Supervised By :Mahesh							
Padoda							
Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		256769	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		229777	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		95413	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.369	65		71770	18.783	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.120%	
7) Chloroethane-d5	2.899	69		51991	19.171	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	76.680%	
11) 1,1-Dichloroethene-d2	4.027	65		30803	18.868	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	75.480%	
21) 2-Butanone-d5	7.087	46		52628	69.093	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	138.180%#	
24) Chloroform-d	7.648	84		138544	20.008	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	80.040%	
26) 1,2-Dichloroethane-d4	8.307	65		83350	23.706	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	94.840%	
32) Benzene-d6	8.276	84		272244	20.072	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	80.280%	
36) 1,2-Dichloropropane-d6	9.270	67		89273	22.466	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	89.880%	
41) Toluene-d8	10.318	98		239015	19.361	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	77.440%	
43) trans-1,3-Dichloroprop...	10.575	79		34094	20.858	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	83.440%	
47) 2-Hexanone-d5	10.922	63		44675	73.458	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	146.920%#	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		85431	29.200	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	116.800%	
66) 1,2-Dichlorobenzene-d4	13.848	152		67605	19.589	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	78.360%	
Target Compounds							
						Qvalue	
13) Acetone	4.149	43		33954	48.736	ug/L	96
14) Carbon disulfide	4.387	76		18196	1.782	ug/L #	95
22) 2-Butanone	7.191	43		4109m	4.122	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082724\
Data File : VW030063.D
Acq On : 28 Aug 2024 00:22
Operator : SY/MD
Sample : P3733-08
Misc : 9.13g/10mL/MSVOA_W/SoIL/A
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A44A2

Manual IntegrationsAPPROVED

Reviewed By :Romaben
Patel

Quant Time: Aug 28 02:46:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Aug 28 02:43:49 2024
Response via : Initial Calibration

