




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082724\
Data File : VW030064.D
Acq On : 28 Aug 2024 00:47
Operator : SY/MD
Sample : P3733-03
Misc : 8.36g/10mL/MSVOA_W/SOIL/A
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4497

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 08/28/2024
Supervised By :Mahesh Dadoda 08/28/2024

Quant Time: Aug 28 02:46:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Aug 28 02:43:49 2024
Response via : Initial Calibration

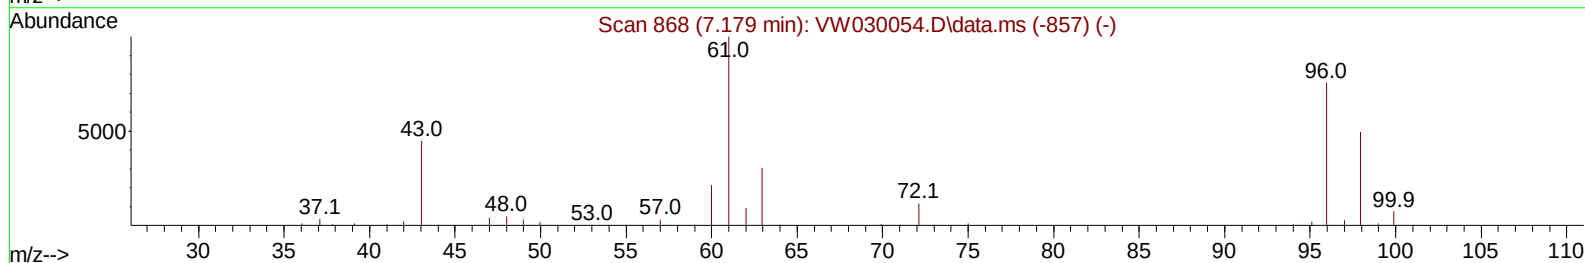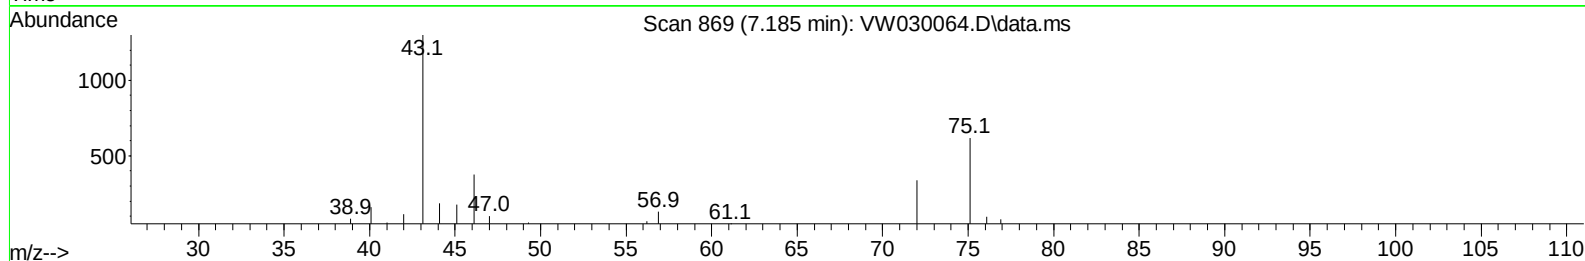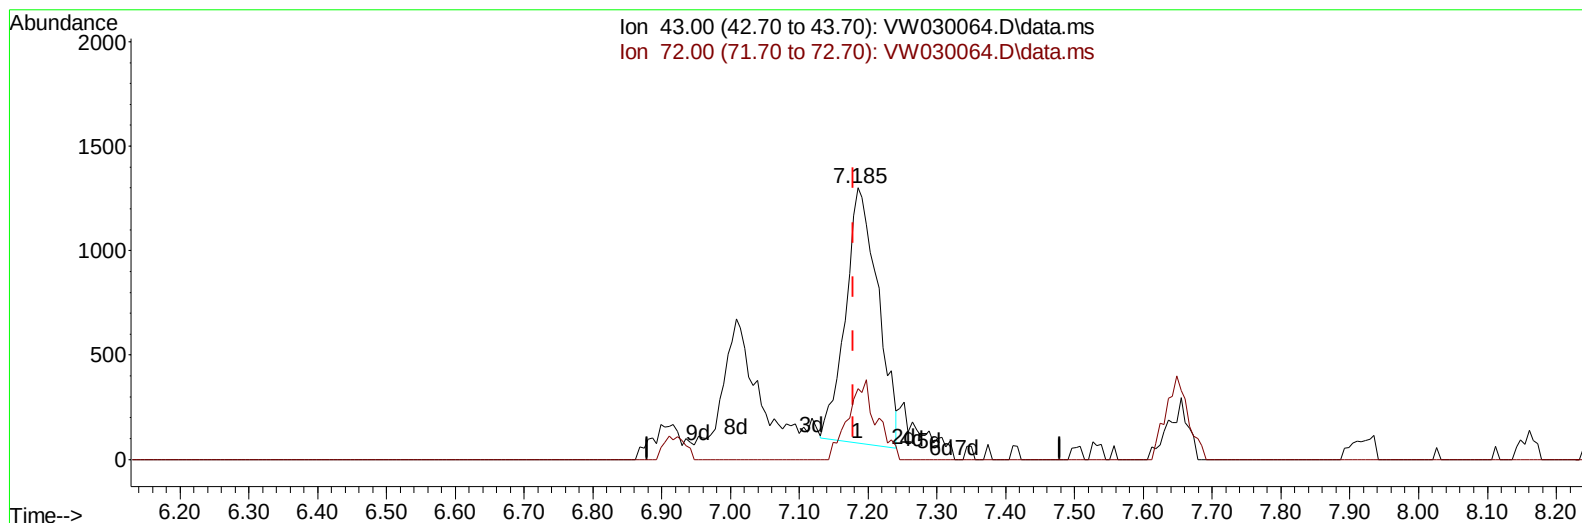

TIC: VW030064.D\data.ms

(22) 2-Butanone (T)

7.185min (+ 0.006) 4.24 ug/L

response 4004

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	30.10	21.88
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082724\
Data File : VW030064.D
Acq On : 28 Aug 2024 00:47
Operator : SY/MD
Sample : P3733-03
Misc : 8.36g/10mL/MSVOA_W/SOIL/A
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4497

Manual IntegrationsAPPROVED

Quant Time: Aug 28 02:46:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Aug 28 02:43:49 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 08/28/2024
Supervised By :Mahesh Dadoda 08/28/2024

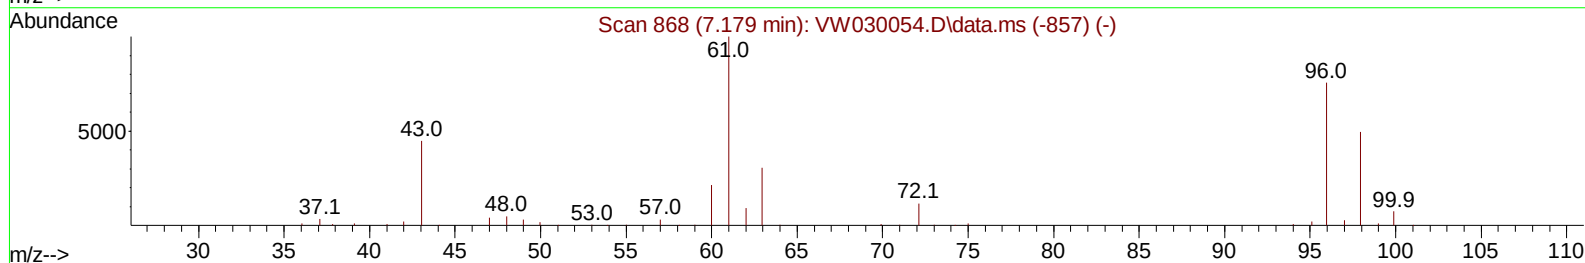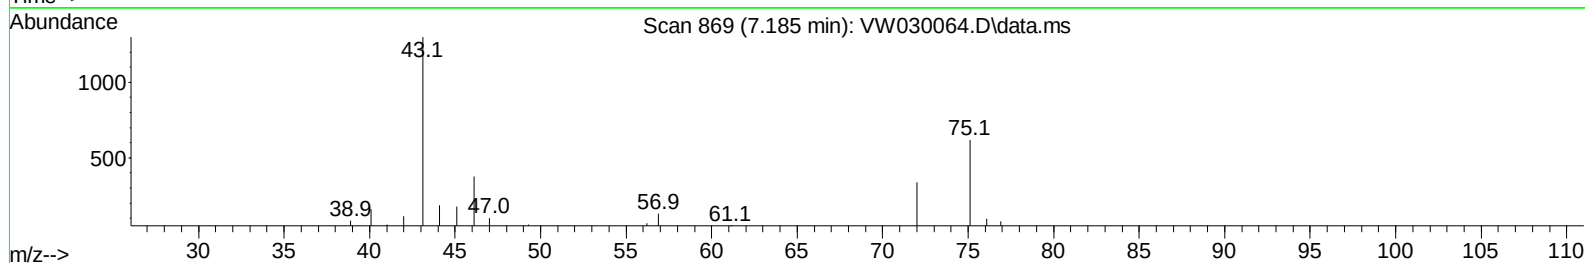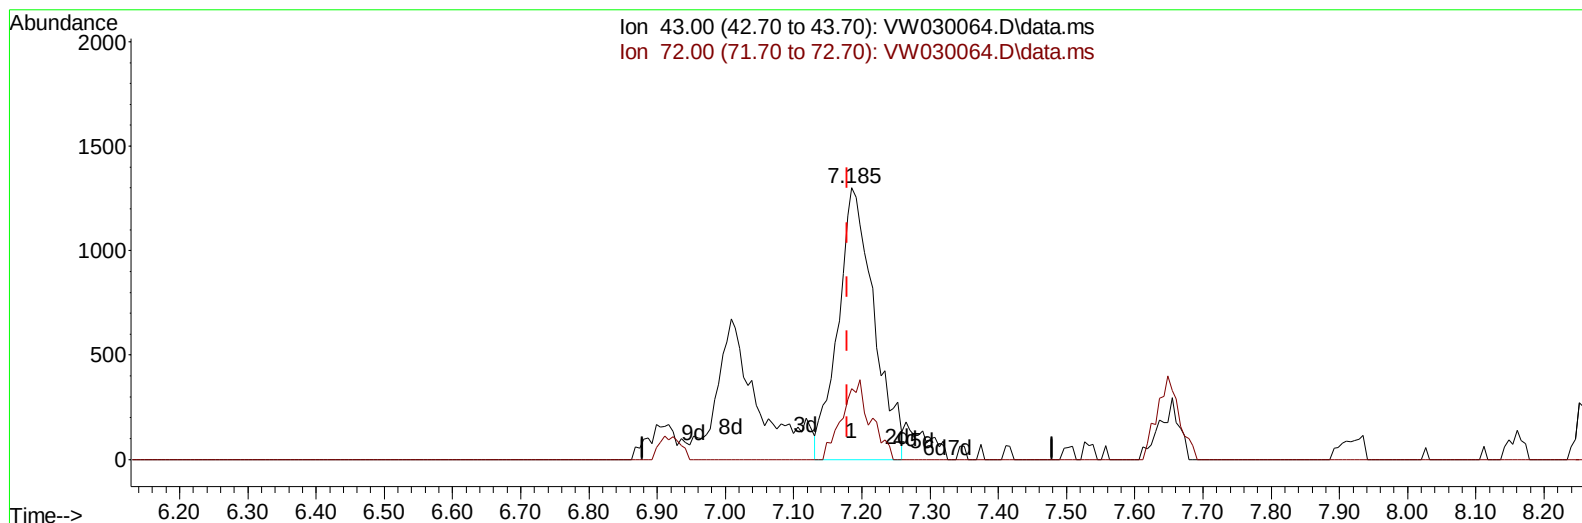

TIC: VW030064.D\data.ms

(22) 2-Butanone (T)

7.185min (+ 0.006) 5.05 ug/L m

response 4766

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	30.10	18.38
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082724\
 Data File : VW030064.D
 Acq On : 28 Aug 2024 00:47
 Operator : SY/MD
 Sample : P3733-03
 Misc : 8.36g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4497

Manual IntegrationsAPPROVED

Quant Time: Aug 28 02:46:42 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 28 02:43:49 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 08/28/2024
 Supervised By :Mahesh Dadoda 08/28/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	243148	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	203826	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	64469	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	68426	18.911	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	75.640%	
7) Chloroethane-d5	2.899	69	48643	18.941	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	75.760%	
11) 1,1-Dichloroethene-d2	4.015	65	28823	18.645	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110	Recovery	=	74.560%	
21) 2-Butanone-d5	7.081	46	48874	67.759	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	135.520%#	
24) Chloroform-d	7.648	84	125087	19.077	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	76.320%	
26) 1,2-Dichloroethane-d4	8.307	65	76594	23.005	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	92.000%	
32) Benzene-d6	8.276	84	248501	20.655	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	82.600%	
36) 1,2-Dichloropropane-d6	9.270	67	81914	23.239	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	92.960%	
41) Toluene-d8	10.319	98	208415	19.032	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	76.120%	
43) trans-1,3-Dichloroprop...	10.575	79	29860	20.593	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	82.360%	
47) 2-Hexanone-d5	10.922	63	42054	77.952	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	155.900%#	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	71776	27.656	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	110.640%	
66) 1,2-Dichlorobenzene-d4	13.849	152	45907	19.687	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	78.760%	
Target Compounds						
13) Acetone	4.149	43	49232	74.624	ug/L	99
22) 2-Butanone	7.185	43	4766m	5.048	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082724\
Data File : VW030064.D
Acq On : 28 Aug 2024 00:47
Operator : SY/MD
Sample : P3733-03
Misc : 8.36g/10mL/MSVOA_W/SOIL/A
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4497

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 08/28/2024
Supervised By :Mahesh Dadoda 08/28/2024

Quant Time: Aug 28 02:46:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Aug 28 02:43:49 2024
Response via : Initial Calibration

