

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082724\
 Data File : VW030050.D
 Acq On : 27 Aug 2024 17:33
 Operator : SY/MD
 Sample : P3733-04
 Misc : 9.18g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4498

Quant Time: Aug 28 01:18:08 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 28 01:11:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	359271	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	312964	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	126591	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	92742	17.346	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	69.400%
7) Chloroethane-d5	2.893	69	66800	17.604	ug/L	-0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	70.400%
11) 1,1-Dichloroethene-d2	4.021	65	42582	18.642	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	74.560%
21) 2-Butanone-d5	7.081	46	55107	51.707	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.420%
24) Chloroform-d	7.648	84	191241	19.739	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	78.960%
26) 1,2-Dichloroethane-d4	8.301	65	108119	21.977	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	87.920%
32) Benzene-d6	8.270	84	387268	20.964	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	83.840%
36) 1,2-Dichloropropane-d6	9.270	67	121174	22.389	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	89.560%
41) Toluene-d8	10.325	98	338529	20.133	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	80.520%
43) trans-1,3-Dichloroprop...	10.575	79	47882	21.507	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	86.040%
47) 2-Hexanone-d5	10.922	63	49339	59.563	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	119.120%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	98007	24.595	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	98.360%
66) 1,2-Dichlorobenzene-d4	13.848	152	89477	19.541	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	78.160%
Target Compounds						
					Qvalue	
13) Acetone	4.143	43	27000	27.698	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082724\
Data File : VW030050.D
Acq On : 27 Aug 2024 17:33
Operator : SY/MD
Sample : P3733-04
Misc : 9.18g/10mL/MSVOA_W/SOIL/A
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4498

Quant Time: Aug 28 01:18:08 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Aug 28 01:11:30 2024
Response via : Initial Calibration

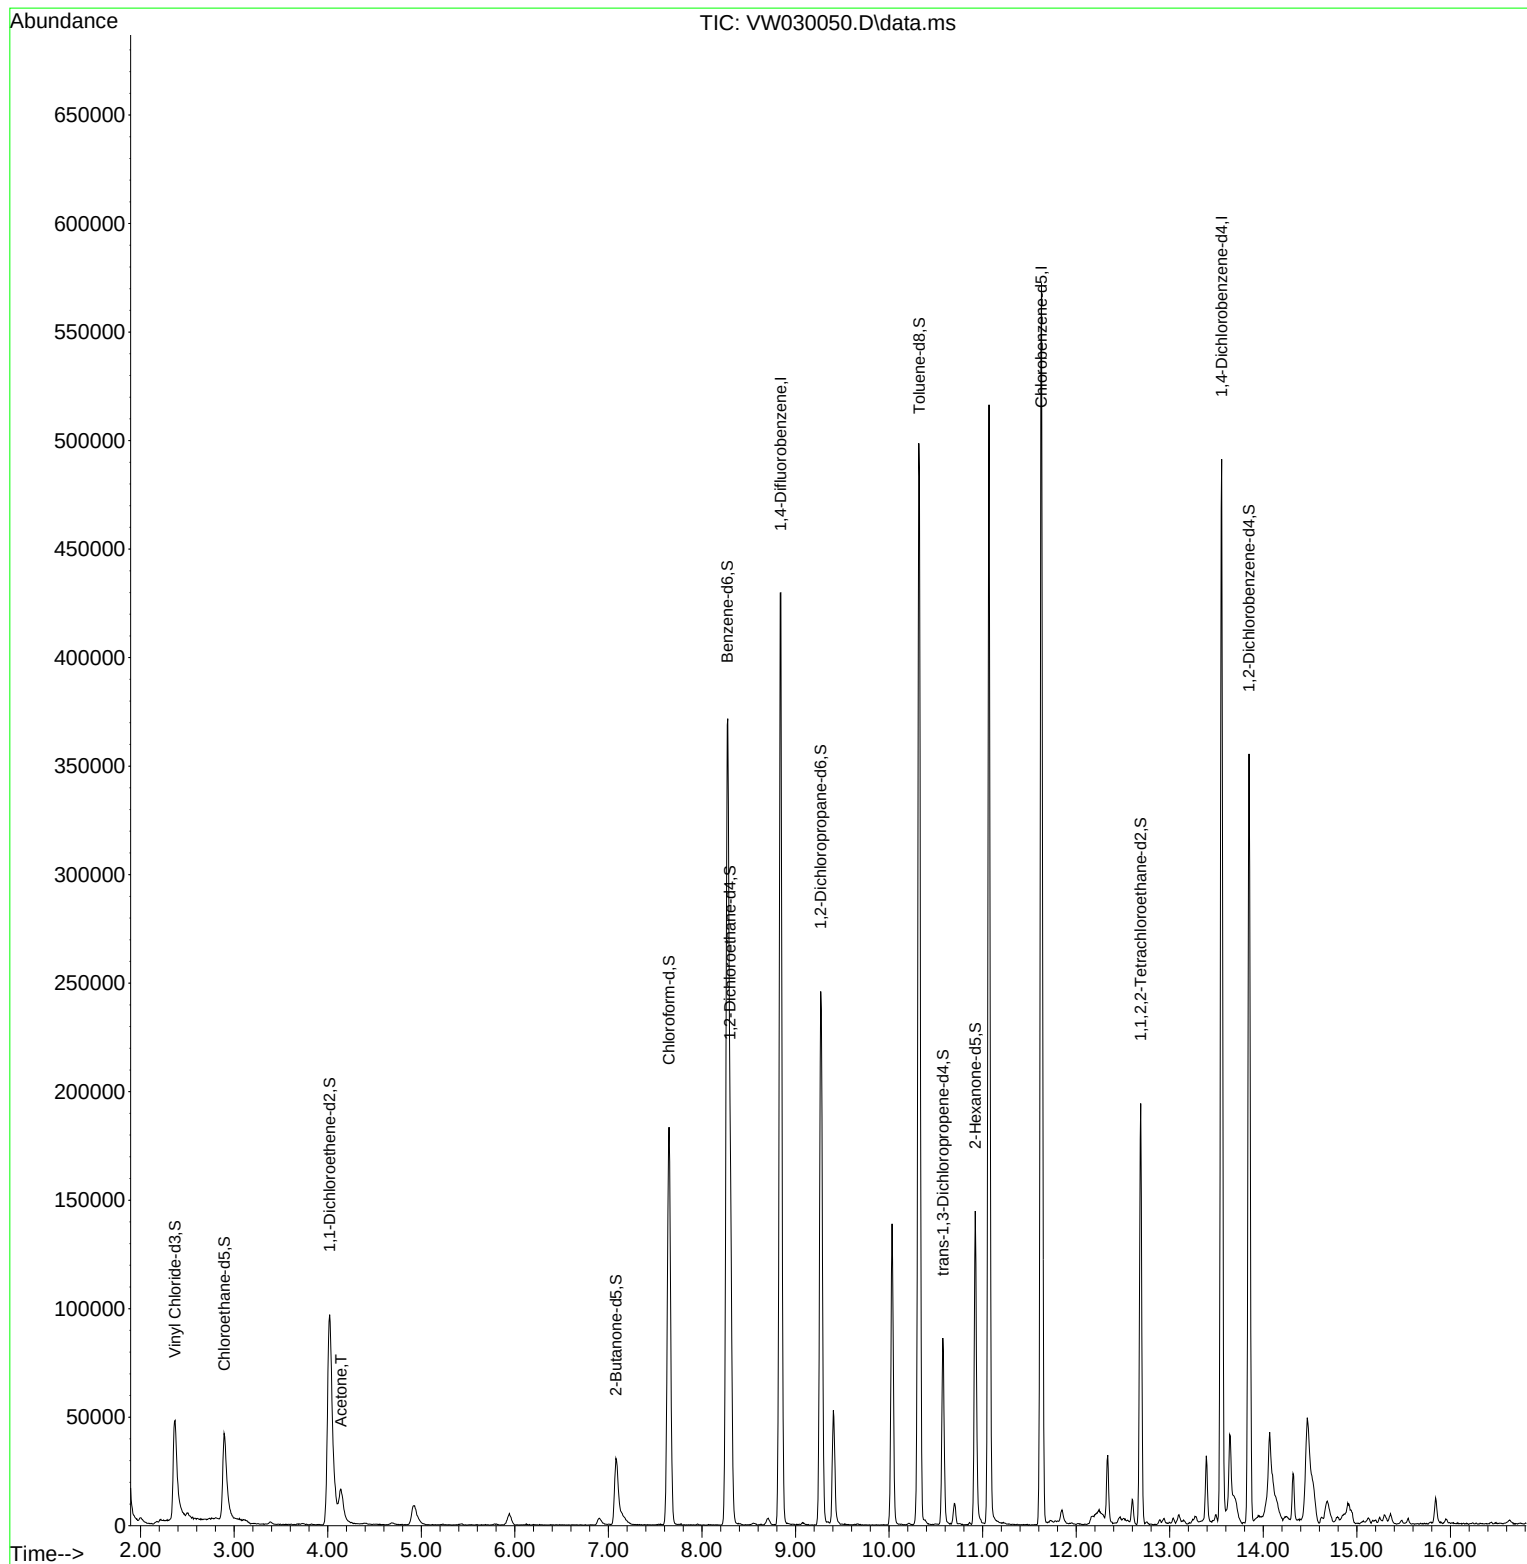

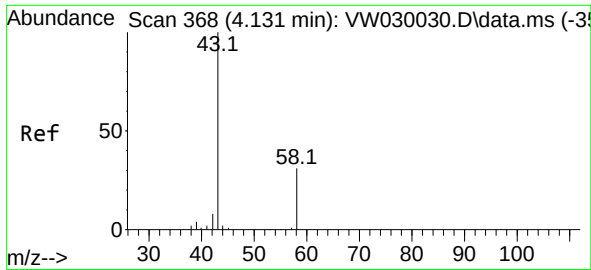

#13
 Acetone
 Concen: 27.698 ug/L
 RT: 4.143 min Scan# 31
 Delta R.T. 0.012 min
 Lab File: VW030050.D
 Acq: 27 Aug 2024 17:33

Instrument :
 MSVOA_W
 ClientSampleId :
 A4498

Tgt Ion: 43 Resp: 27000
 Ion Ratio Lower Upper
 43 100
 58 33.3 0.0 66.4

