


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082724\
Data File : VW030029.D
Acq On : 27 Aug 2024 07:57
Operator : SY/MD
Sample : BFB552
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB552

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
Title : SFAM01.0
Last Update : Thu Aug 29 01:10:06 2024

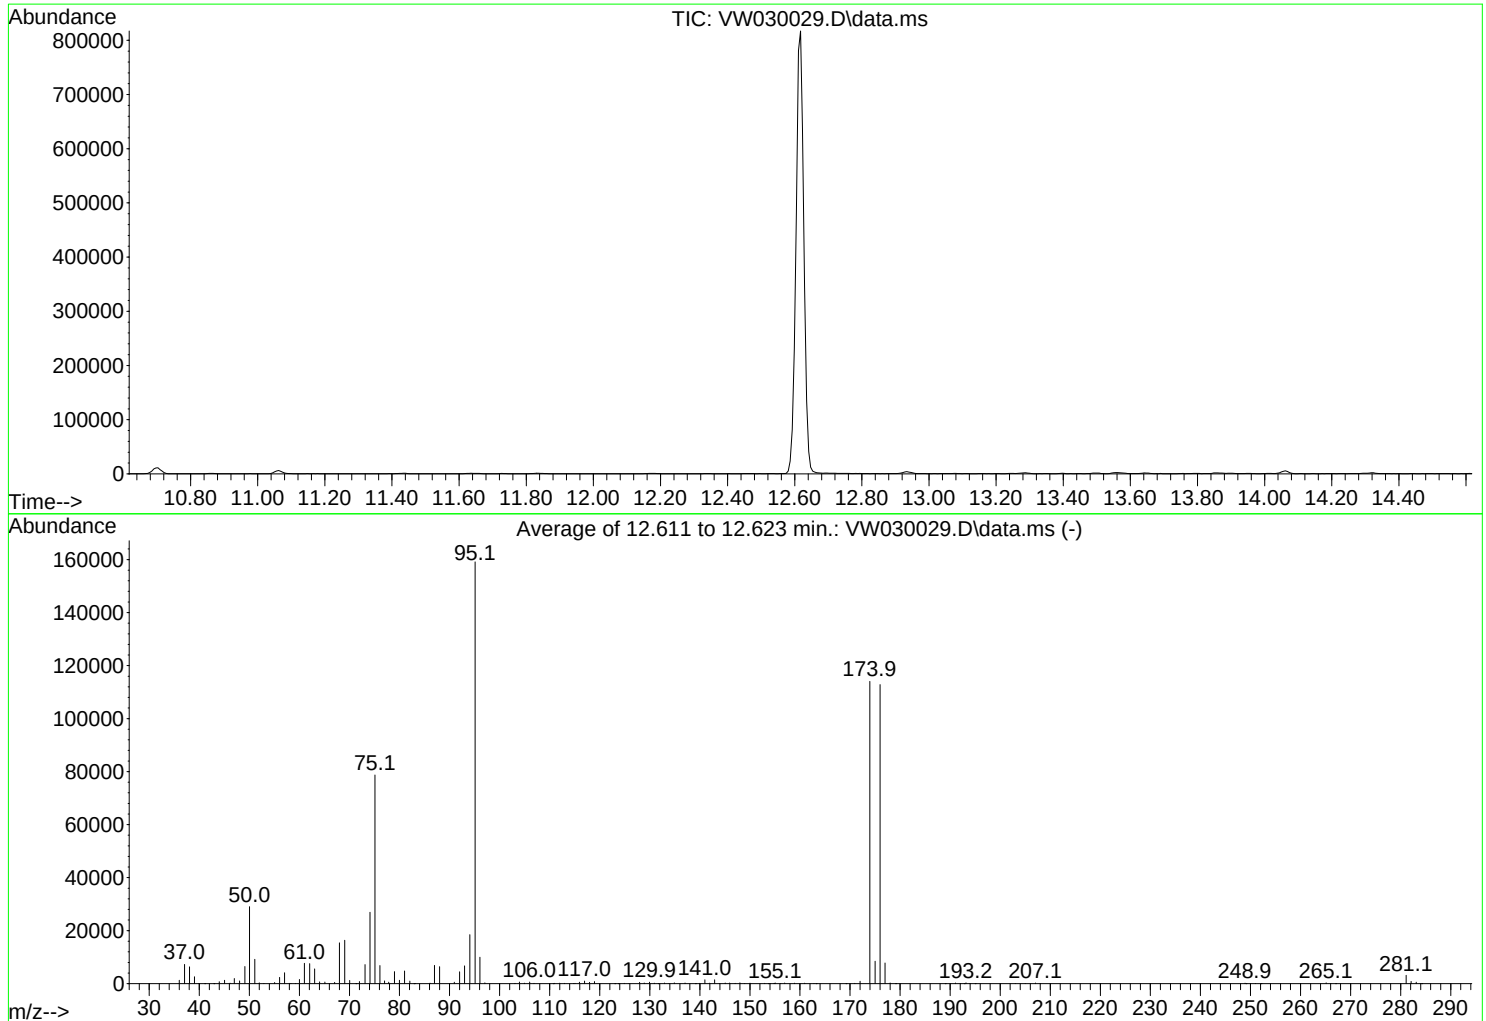

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	29064	PASS
75	95	30	80	49.5	78731	PASS
95	95	100	100	100.0	159147	PASS
96	95	5	9	6.3	9956	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	71.7	114043	PASS
175	174	5	9	7.4	8440	PASS
176	174	95	101	99.0	112861	PASS
177	176	5	9	6.9	7784	PASS

m/z	Abundance
36.00	98.0
38.20	84.0
40.00	149.0
44.00	177.0

Instrument :
MSVOA_W
ClientSampleId :
BFB552

m/z	Abundance
36.10	1568.0
37.10	7861.0
38.10	7402.0
39.00	2834.0
39.90	247.0
42.90	117.0
44.00	939.0
45.10	1419.0
46.10	194.0
47.00	2019.0
48.00	1116.0
49.10	7230.0
50.00	31296.0
51.10	9986.0
52.00	383.0
52.90	94.0
55.00	497.0
56.00	2505.0
57.00	4539.0
58.10	207.0
59.20	111.0
60.00	1740.0
61.00	8314.0
62.00	8748.0
63.00	6371.0
64.00	838.0
65.10	773.0
66.00	91.0
67.10	511.0
68.00	16992.0
69.10	18456.0
70.10	1295.0
71.30	75.0
72.00	801.0
73.10	7967.0
74.10	29192.0
75.10	84888.0
76.10	7771.0
77.00	1281.0
77.90	577.0
79.00	4905.0
80.00	1380.0
81.00	5051.0
82.00	1092.0
83.20	96.0
86.20	267.0
87.00	7146.0
88.00	6409.0
90.90	581.0
92.00	4499.0
93.00	7424.0
94.00	19256.0
95.10	165632.0
96.00	10835.0
97.10	352.0
103.00	199.0
103.90	688.0
104.90	248.0
106.00	709.0
106.80	163.0
110.00	90.0
110.90	195.0
112.00	192.0
113.00	171.0
115.00	225.0
115.90	420.0
117.00	1090.0
117.90	531.0
119.00	815.0
123.70	66.0
125.00	142.0
127.90	505.0
128.80	283.0
130.00	616.0
130.90	261.0
131.70	56.0
133.00	404.0
133.90	117.0
134.90	371.0
137.10	141.0
141.00	1472.0
141.90	172.0
143.00	1365.0
144.00	107.0
145.10	328.0
146.00	230.0
147.10	124.0
148.00	333.0
149.00	82.0
150.00	175.0
153.10	99.0
153.70	95.0

Instrument :
MSVOA_W
ClientSampleId :
BFB552

154.10	83.0
154.80	298.0
155.10	286.0
156.10	51.0
156.90	237.0
158.90	124.0
160.90	153.0
162.80	130.0
171.00	147.0
172.00	1021.0
174.00	109264.0
175.00	7829.0
176.00	114968.0
177.00	7997.0
178.00	287.0
179.10	79.0
189.00	66.0
191.10	354.0
192.00	157.0
193.10	497.0
194.00	122.0
195.00	101.0
203.00	79.0
205.00	83.0
207.10	301.0
208.00	119.0
248.90	387.0
251.00	171.0
252.10	54.0
265.10	525.0
266.00	130.0
267.00	97.0
281.20	4763.0
282.10	1427.0
283.20	799.0
283.90	188.0

Instrument :
MSVOA_W
ClientSampleId :
BFB552

m/z	Abundance
36.10	1349.0
37.10	8123.0
38.00	6928.0
39.00	2793.0
40.00	232.0
43.10	94.0
44.00	1021.0
45.00	1341.0
46.20	138.0
47.00	2155.0
48.00	1122.0
49.10	6744.0
50.10	33024.0
51.10	10271.0
52.00	345.0
52.90	50.0
55.10	463.0
56.10	2671.0
57.10	4357.0
58.30	242.0
59.20	78.0
60.00	1834.0
61.00	8032.0
62.10	8000.0
63.10	5978.0
64.10	586.0
65.10	591.0
66.00	78.0
67.10	439.0
68.00	16952.0
69.00	17424.0
70.10	1336.0
72.00	1050.0
73.10	8047.0
74.10	30320.0
75.10	88120.0
76.10	7212.0
77.00	1110.0
77.80	630.0
79.00	5170.0
80.00	1446.0
81.00	5271.0
82.00	1073.0
83.10	117.0
86.00	208.0
87.00	7928.0
88.00	7557.0
90.90	618.0
92.00	4789.0
93.00	7476.0
94.10	20720.0
95.10	179968.0
96.10	10795.0
97.00	323.0
103.10	130.0
104.00	661.0
104.90	219.0
106.00	650.0
106.90	126.0
109.90	79.0
111.00	149.0
112.00	146.0
112.90	179.0
115.10	253.0
116.00	717.0
117.00	1043.0
118.00	524.0
118.90	904.0
123.00	56.0
124.00	135.0
124.80	188.0
125.90	93.0
128.00	518.0
128.90	353.0
129.90	630.0
130.90	197.0
132.90	192.0
133.80	96.0
134.90	295.0
137.00	319.0
139.10	96.0
139.90	149.0
141.00	1640.0
141.90	191.0
142.90	1497.0
145.00	273.0
146.00	271.0
147.00	124.0
148.00	357.0
149.00	115.0
150.00	189.0
152.90	187.0

Instrument :
MSVOA_W
ClientSampleId :
BFB552

154.10	100.0
155.00	476.0
156.20	58.0
157.00	204.0
158.90	223.0
160.90	194.0
163.20	52.0
169.20	59.0
171.00	150.0
172.00	1017.0
174.00	128480.0
175.00	9596.0
176.00	112792.0
177.00	8194.0
178.00	284.0
191.00	242.0
192.10	69.0
193.20	299.0
193.90	72.0
203.00	56.0
205.00	81.0
207.00	403.0
208.00	81.0
249.00	122.0
251.00	92.0
265.10	270.0
266.10	122.0
281.00	3234.0
282.10	919.0
283.10	476.0
284.20	88.0

Instrument :
MSVOA_W
ClientSampleId :
BFB552

m/z	Abundance
36.00	1131.0
37.00	5768.0
38.00	4972.0
39.10	2093.0
40.00	215.0
41.10	67.0
43.00	105.0
44.00	816.0
45.10	1013.0
46.20	147.0
47.00	1624.0
48.10	781.0
49.10	5336.0
50.00	22872.0
51.10	7221.0
52.00	239.0
55.00	332.0
56.00	1840.0
57.00	3430.0
58.00	98.0
59.30	63.0
60.00	1207.0
61.00	6655.0
62.00	5904.0
63.10	4401.0
64.00	538.0
65.00	415.0
66.00	81.0
67.00	451.0
68.00	12278.0
69.00	13258.0
70.00	1086.0
72.00	540.0
73.10	5564.0
74.10	21336.0
75.10	63184.0
76.10	5580.0
77.00	725.0
77.90	515.0
79.00	3538.0
80.00	978.0
81.00	4087.0
82.10	764.0
82.90	83.0
86.00	140.0
87.00	5585.0
88.00	5324.0
91.00	484.0
92.00	4047.0
93.00	5184.0
94.10	15525.0
95.10	131840.0
96.00	8237.0
97.00	318.0
103.10	93.0
104.00	518.0
105.00	161.0
106.00	539.0
106.80	168.0
110.00	81.0
110.70	88.0
111.10	86.0
111.80	86.0
112.10	62.0
112.90	105.0
114.80	167.0
116.00	565.0
116.90	859.0
118.00	457.0
119.00	665.0
123.90	137.0
124.80	62.0
125.80	108.0
128.00	498.0
129.00	171.0
129.90	434.0
131.00	131.0
132.90	139.0
134.90	316.0
137.00	238.0
139.90	141.0
141.00	1306.0
142.00	171.0
143.00	1429.0
143.80	78.0
145.00	222.0
145.90	189.0
147.00	146.0
148.00	300.0
148.90	77.0
149.90	120.0
152.90	127.0

Instrument :
MSVOA_W
ClientSampleId :
BFB552

153.90	80.0
154.90	336.0
156.20	51.0
156.80	152.0
157.10	149.0
158.90	158.0
161.00	165.0
170.90	140.0
172.00	614.0
173.90	104384.0
175.00	7896.0
176.00	110824.0
177.00	7161.0
178.00	159.0
191.10	149.0
192.80	83.0
193.20	69.0
207.00	119.0
249.10	61.0
264.90	67.0
281.20	1338.0
282.00	257.0
283.00	382.0

Instrument :
MSVOA_W
ClientSampleId :
BFB552