

Data File : VW004990.D
Acq On : 28 Aug 2018 17:17
Operator : SY/AP
Sample : J4678-01
Misc : 5.94G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E5FC2

Quant Time: Aug 29 04:25:23 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM082218S.M
Quant Title : VOC Analysis
QLast Update : Wed Aug 29 04:23:47 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	629748	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	704458	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	340459	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	243645	20.47	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.88%
7) Chloroethane-d5	2.89	69	194397	22.03	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.12%
10) 1,1-Dichloroethene-d2	4.02	63	251544	16.55	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	66.20%
20) 2-Butanone-d5	7.09	46	118810	49.04	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.08%
24) Chloroform-d	7.65	84	303343	21.70	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	86.80%
26) 1,2-Dichloroethane-d4	8.31	65	198246	26.10	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	104.40%
29) Benzene-d6	8.28	84	759254	20.95	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	83.80%
33) 1,2-Dichloropropane-d6	9.28	67	227363	21.36	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	85.44%
37) Toluene-d8	10.33	98	819471	21.35	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	85.40%
38) trans-1,3-Dichloropropene-	10.58	79	95156	20.77	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	83.08%
39) 2-Hexanone-d5	10.93	63	118472	44.91	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.82%
48) 1,1,2,2-Tetrachloroethane-	12.70	84	245248	22.93	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	91.72%
61) 1,2-Dichlorobenzene-d4	13.86	152	349983	25.59	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	102.36%


Target Compounds					Qvalue
13) Acetone	4.14	43	9941	5.298 ug/L	98
25) Chloroform	7.68	83	43108	3.086 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VW004990.D
Acq On : 28 Aug 2018 17:17
Operator : SY/AP
Sample : J4678-01
Misc : 5.94G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E5FC2

Quant Time: Aug 29 04:25:23 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM082218S.M
Quant Title : VOC Analysis
QLast Update : Wed Aug 29 04:23:47 2018
Response via : Initial Calibration

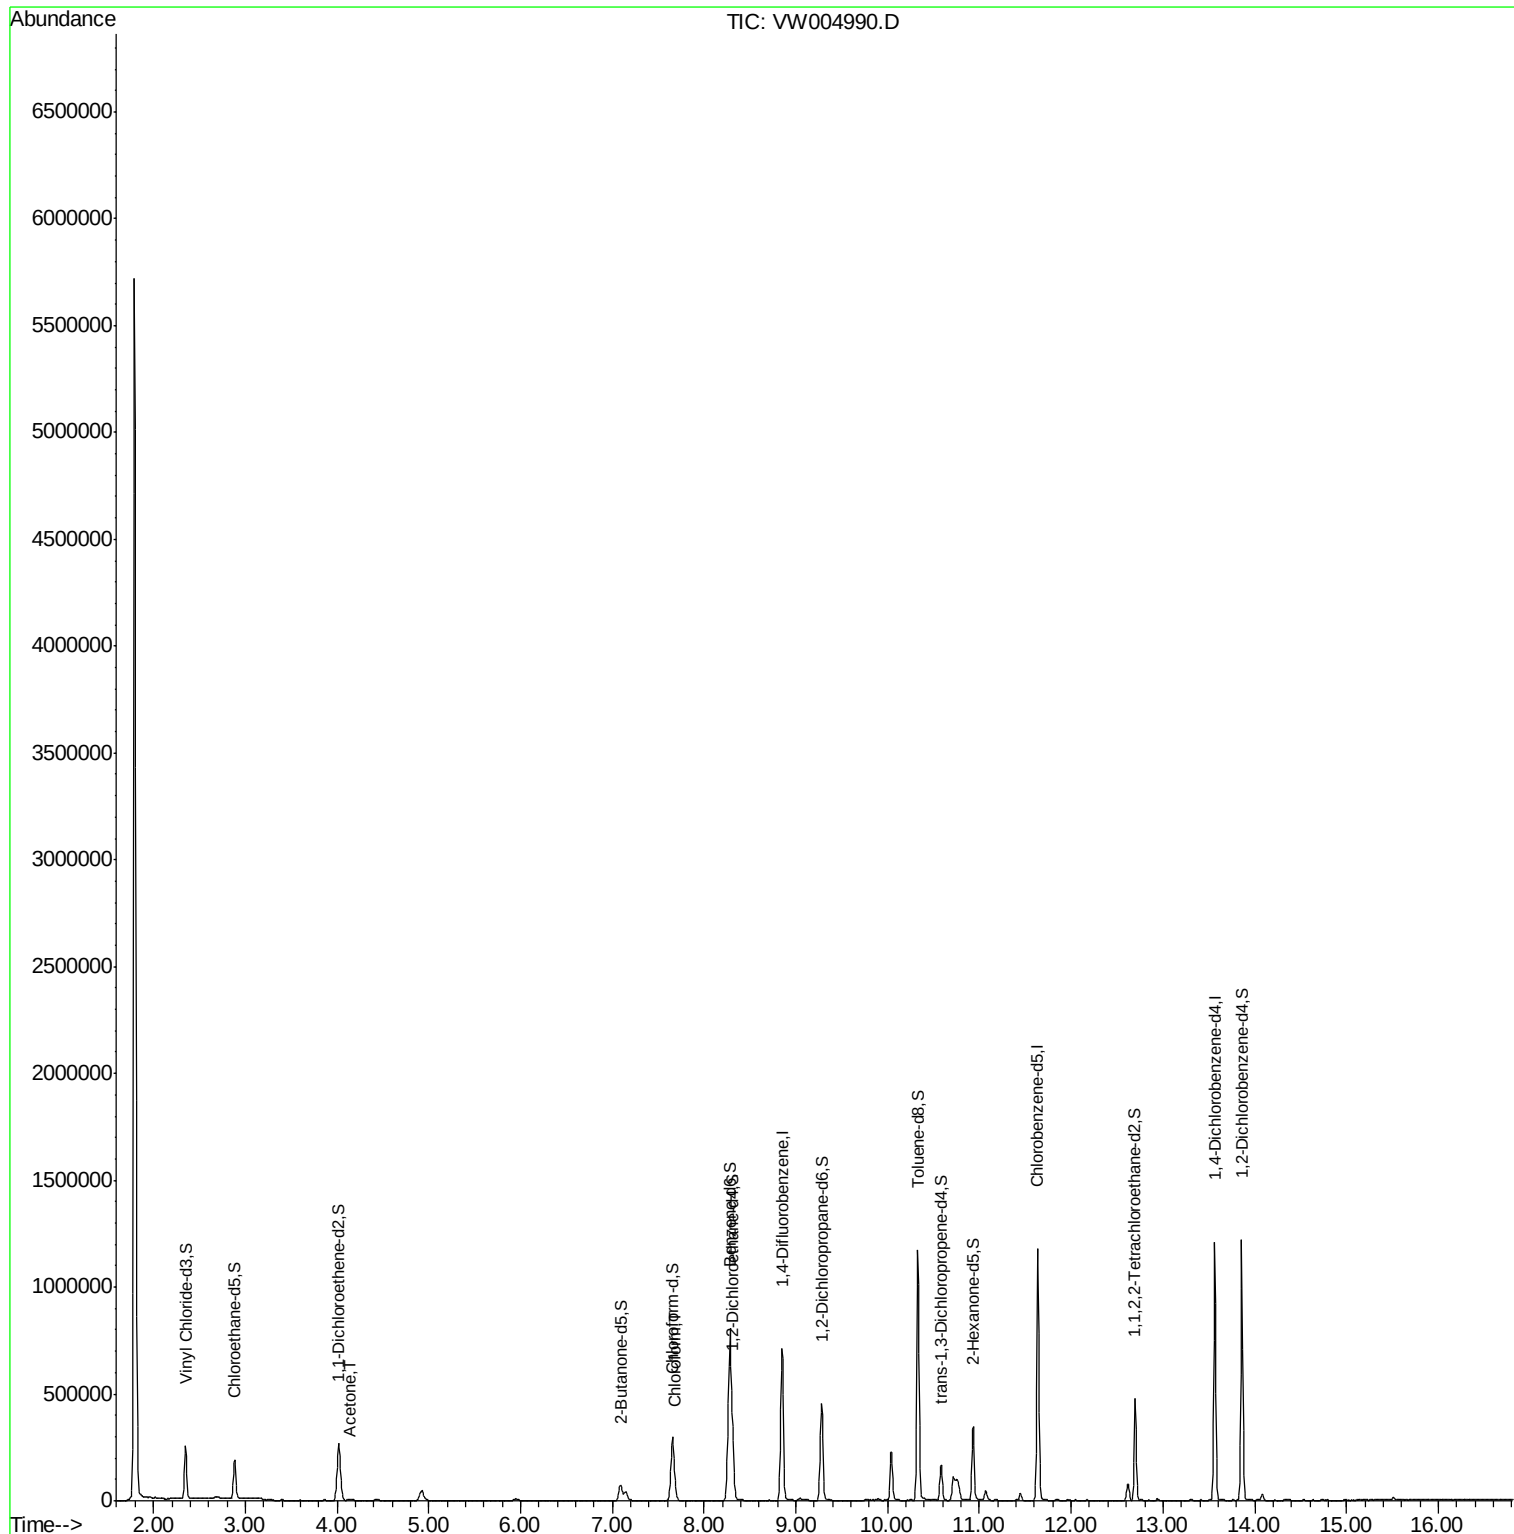

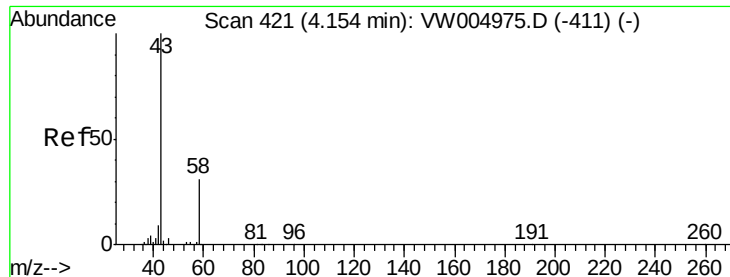

#13

Acetone

Concen: 5.298 ug/L

RT: 4.14 min Scan# 419

Delta R.T. -0.00 min

Lab File: VW004990.D

Acq: 28 Aug 2018 17:17

Instrument :

MSVOA_W

ClientSampled :


E5FC2

Tgt Ion: 43 Resp: 9941

Ion Ratio Lower Upper




43 100

58 35.7 0.0 69.4

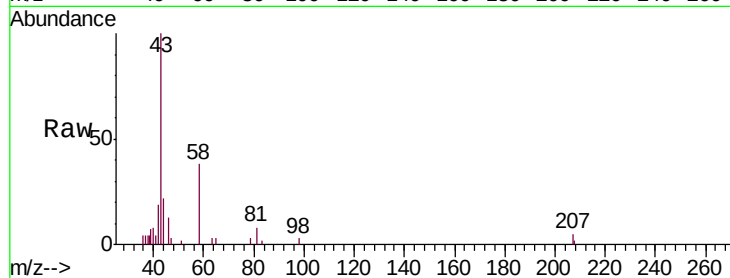

Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 58.00 (57.70 to 58.70): VW

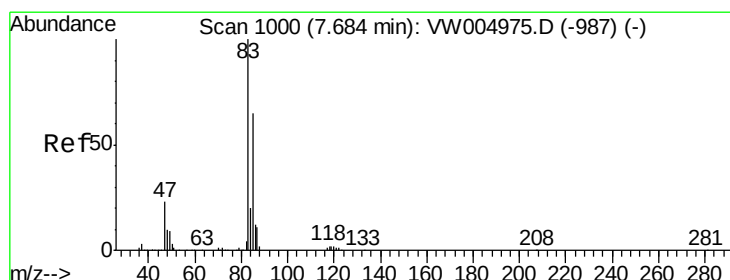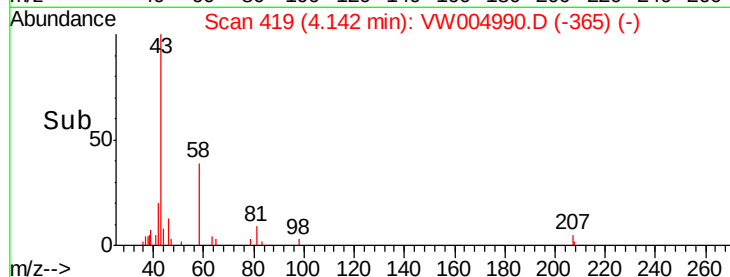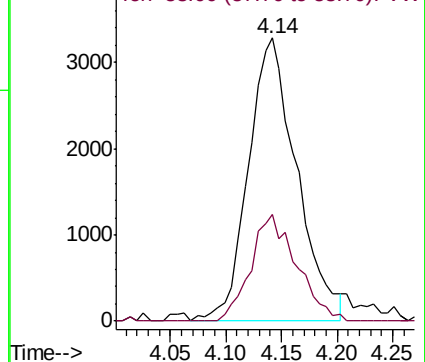

#25

Chloroform

Concen: 3.086 ug/L

RT: 7.68 min Scan# 1000

Delta R.T. -0.00 min

Lab File: VW004990.D


Acq: 28 Aug 2018 17:17

Tgt Ion: 83 Resp: 43108

Ion Ratio Lower Upper

83 100

85 71.7 46.3 85.9

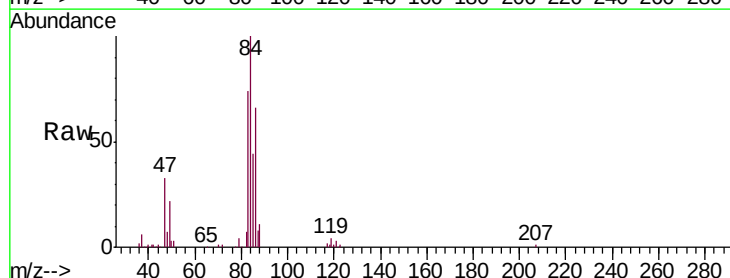

Abundance Ion 83.00 (82.70 to 83.70): VW

Ion 85.00 (84.70 to 85.70): VW

