

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW082818\

Quantitation Report (QT/LSC Reviewed)

Data File : VW004976.D

Acq On : 28 Aug 2018 10:35

Operator : SY/AP

Sample : VW0828SBL01

Misc : 5.00G/10ML/MSVOA_W/SOIL

ALS Vial : 1 Sample Multiplier: 1

Instrument :

MSVOA_W

ClientSampleId :

VBLK08

Manual Integrations
APPROVED

MMDadoda

8/29/2018 5:04:52 PM


Quant Time: Aug 29 04:34:13 2018

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM082218S.M

Quant Title : VOC Analysis

QLast Update : Wed Aug 29 04:23:47 2018

Response via : Initial Calibration

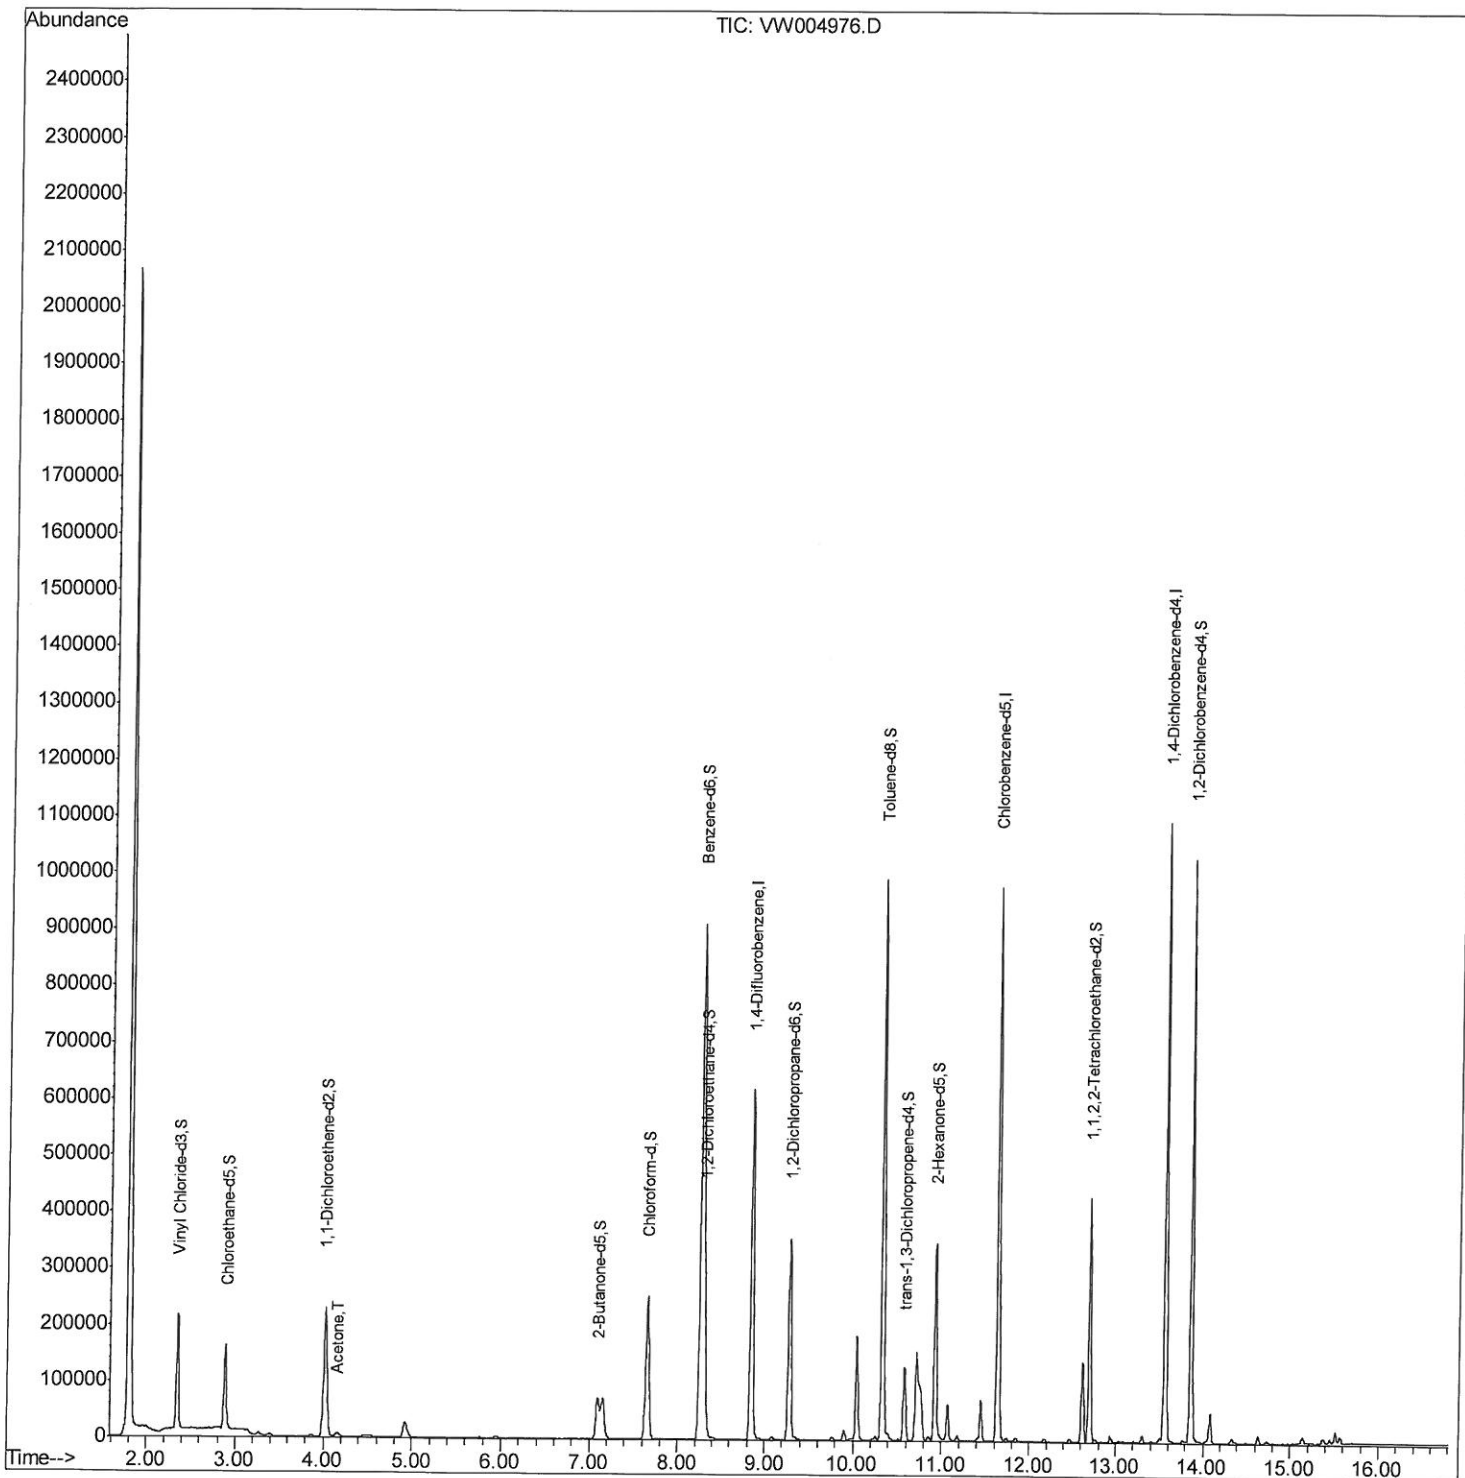

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW082818\
Quantitation Report (Qedit)




Data File : VW004976.D
Acq On : 28 Aug 2018 10:35
Operator : SY/AP
Sample : VW0828SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK08

Manual Integrations
APPROVED

MMDadoda
8/29/2018 5:04:52 PM

Quant Time: Aug 29 04:23:57 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM082218S.M
Quant Title : VOC Analysis
QLast Update : Wed Aug 29 04:23:47 2018
Response via : Initial Calibration

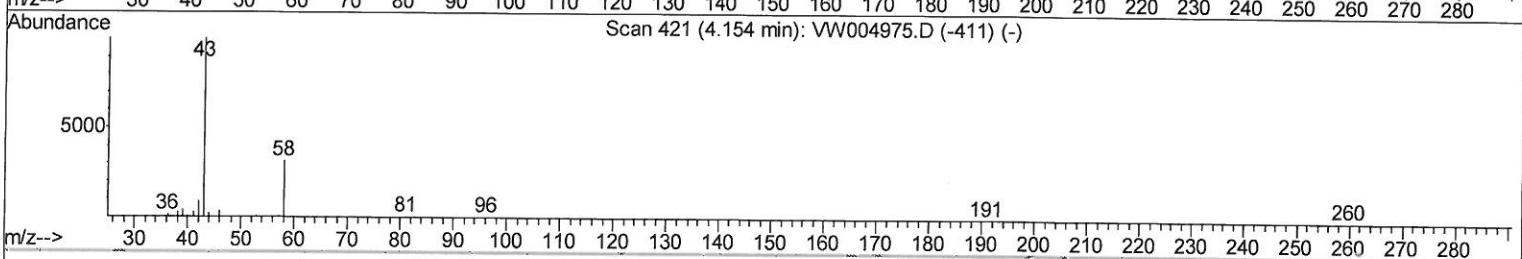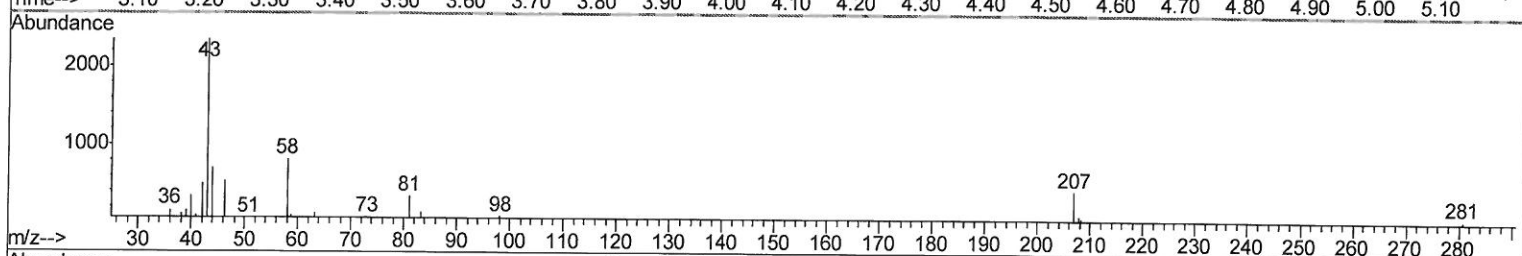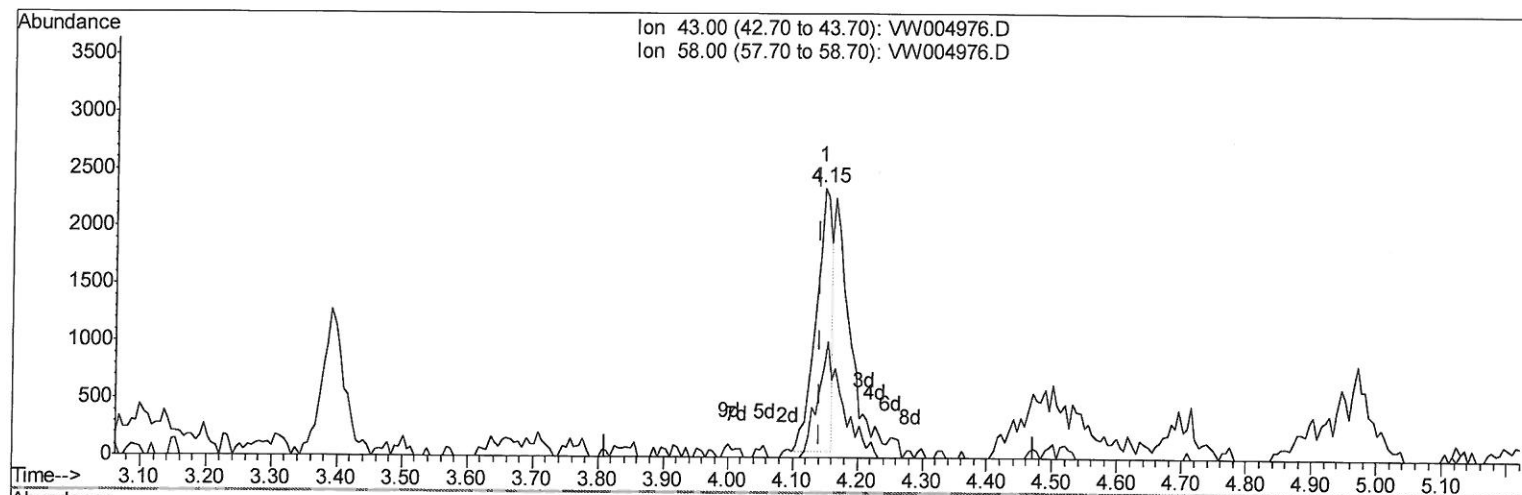

TIC: VW004976.D

(13) Acetone (T)

4.147min (+0.006) 2.43ug/L

response 4072

Ion	Exp%	Act%
43.00	100	100
58.00	34.70	60.81
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW082818\
Quantitation Report (Qedit)




Data File : VW004976.D
Acq On : 28 Aug 2018 10:35
Operator : SY/AP
Sample : VW0828SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK08

Manual Integrations
APPROVED

MMDadoda
8/29/2018 5:04:52 PM

Quant Time: Aug 29 04:23:57 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM082218S.M
Quant Title : VOC Analysis
QLast Update : Wed Aug 29 04:23:47 2018
Response via : Initial Calibration

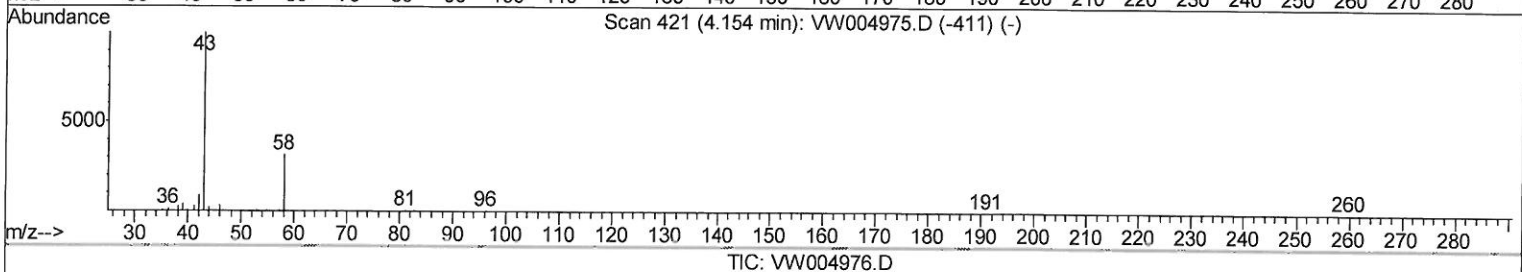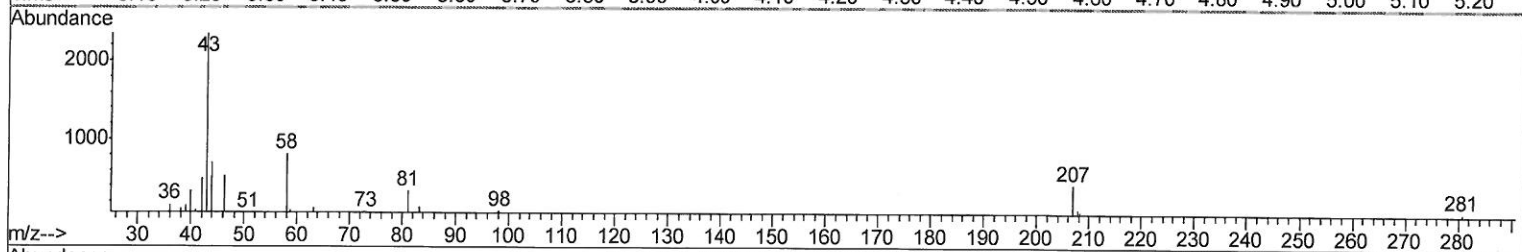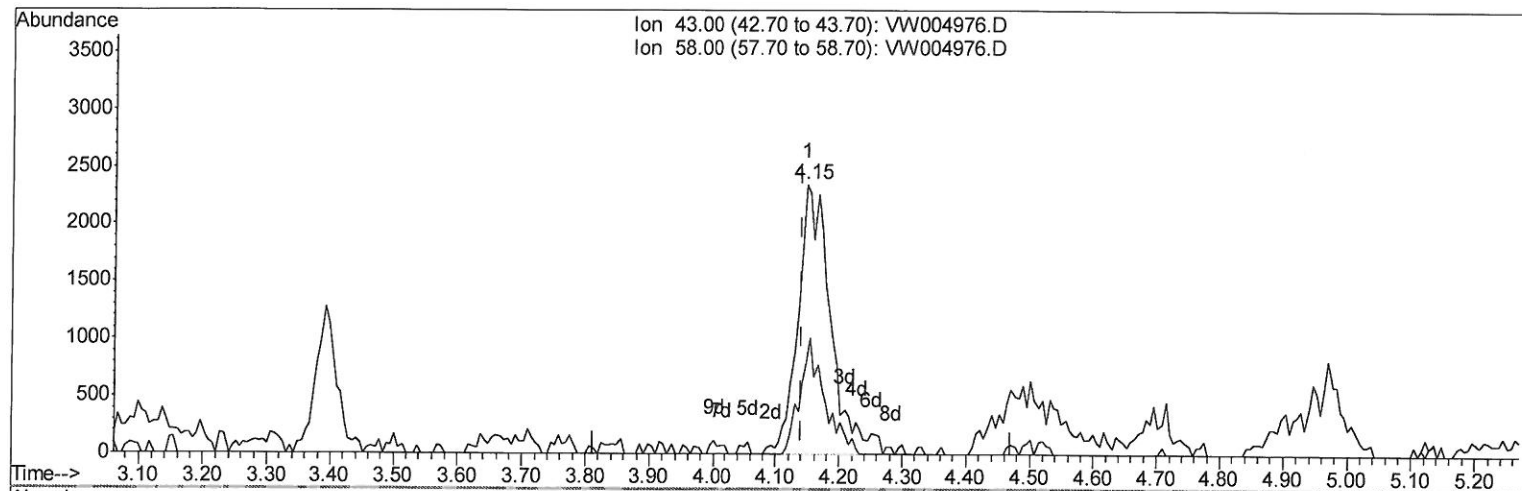

(13) Acetone (T)

4.147min (+0.006) 5.01ug/L m

response 8410

Ion	Exp%	Act%
-----	------	------

43.00	100	100
-------	-----	-----

58.00	34.70	29.44
-------	-------	-------

0.00	0.00	0.00
------	------	------

0.00	0.00	0.00
------	------	------

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW082818\

Quantitation Report (QT/LSC Reviewed)

Data File : VW004976.D

Acq On : 28 Aug 2018 10:35

Operator : SY/AP

Sample : VW0828SBL01

Misc : 5.00G/10ML/MSVOA_W/SOIL

ALS Vial : 1 Sample Multiplier: 1

Instrument :

MSVOA_W

ClientSampleId :

VBLK08

Manual Integrations

APPROVED

MMDadoda

8/29/2018 5:04:52 PM

Quant Time: Aug 29 04:34:13 2018

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM082218S.M

Quant Title : VOC Analysis

QLast Update : Wed Aug 29 04:23:47 2018

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	562844	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	598928	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	302123	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	208308	19.58	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	78.32%
7) Chloroethane-d5	2.89	69	165180	20.94	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.76%
10) 1,1-Dichloroethene-d2	4.02	63	213324	15.70	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	62.80%
20) 2-Butanone-d5	7.09	46	129205	59.67	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	119.34%
24) Chloroform-d	7.65	84	268218	21.46	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	85.84%
26) 1,2-Dichloroethane-d4	8.31	65	156589	23.06	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	92.24%
29) Benzene-d6	8.28	84	635993	20.64	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	82.56%
33) 1,2-Dichloropropane-d6	9.28	67	182423	20.15	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	80.60%
37) Toluene-d8	10.33	98	693780	21.26	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	85.04%
38) trans-1,3-Dichloropropene-	10.59	79	76159	19.56	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	78.24%
39) 2-Hexanone-d5	10.93	63	125727	56.06	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	112.12%
48) 1,1,2,2-Tetrachloroethane-	12.70	84	218174	23.99	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	95.96%
61) 1,2-Dichlorobenzene-d4	13.86	152	292645	24.11	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	96.44%

Target Compounds

13) Acetone	4.15	43	8410m	>	5.015	ug/L	Qvalue
-------------	------	----	-------	---	-------	------	--------

08/29/18 SY

(#)=qualifier out of range (m)=manual integration (+)=signals summed