

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082823\
Data File : VW026929.D
Acq On : 28 Aug 2023 09:58
Operator : SY/MD
Sample : VW0828SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1




Instrument :
MSVOA_W
ClientSampleId :
VBLK561

Manual IntegrationsAPPROVED

Quant Time: Aug 28 14:13:02 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Aug 26 05:14:45 2023
Response via : Initial Calibration

Reviewed By :Semsettin
Yesilyurt

08/29/2023
Supervised By :Mahesh
Dadoda

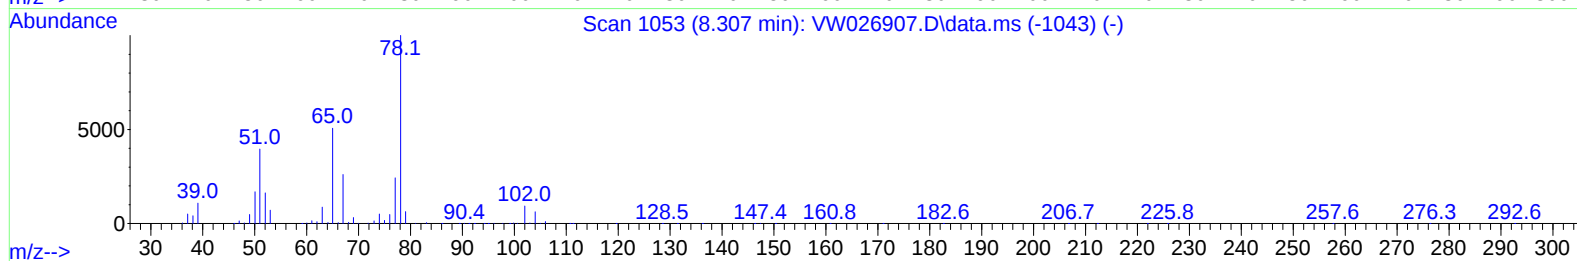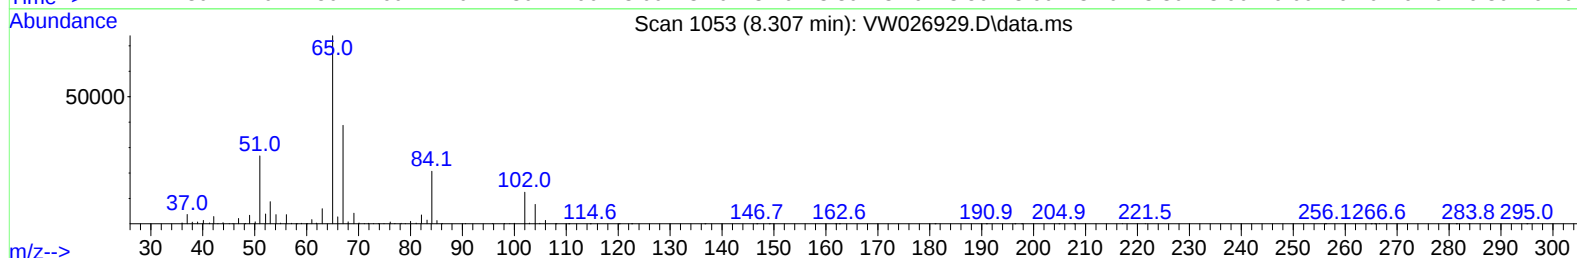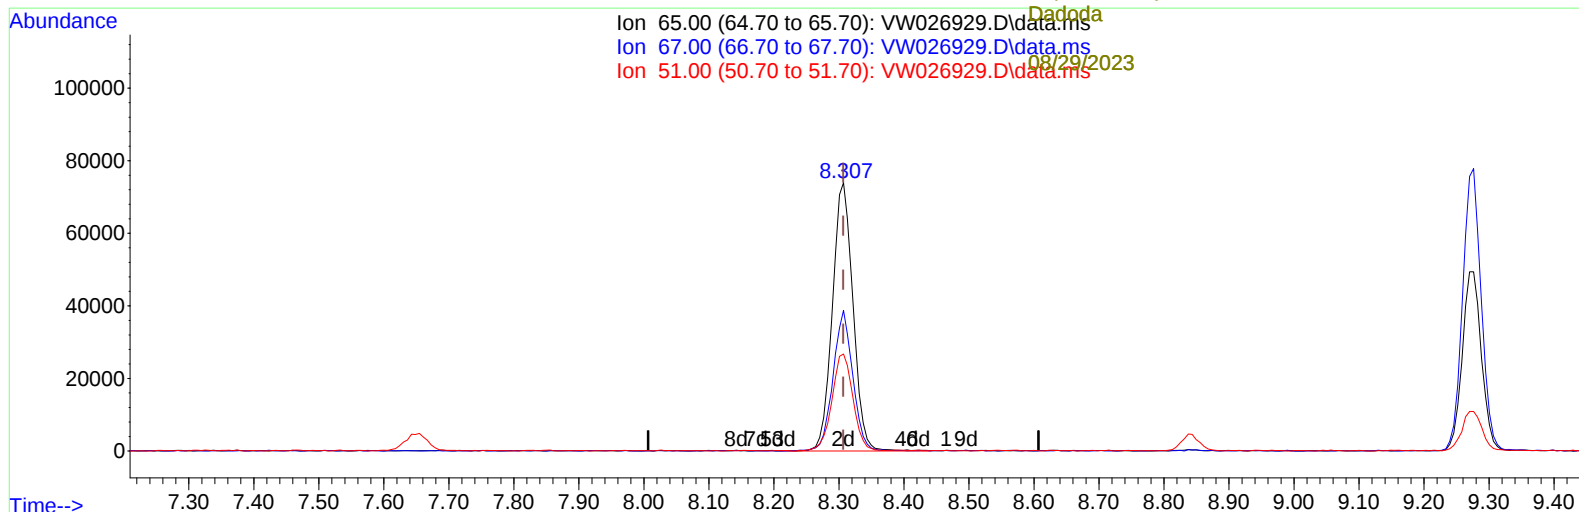

TIC: VW026929.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (+ 0.000) 25.63 ug/L m

response 163288

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.60	0.05#
51.00	112.90	0.08#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082823\
Data File : VW026929.D
Acq On : 28 Aug 2023 09:58
Operator : SY/MD
Sample : VW0828SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1




Instrument :
MSVOA_W
ClientSampleId :
VBLK561

Manual IntegrationsAPPROVED

Quant Time: Aug 28 14:13:02 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Aug 26 05:14:45 2023
Response via : Initial Calibration

Reviewed By :Semsettin
Yesilyurt

08/29/2023
Supervised By :Mahesh
Dadoda

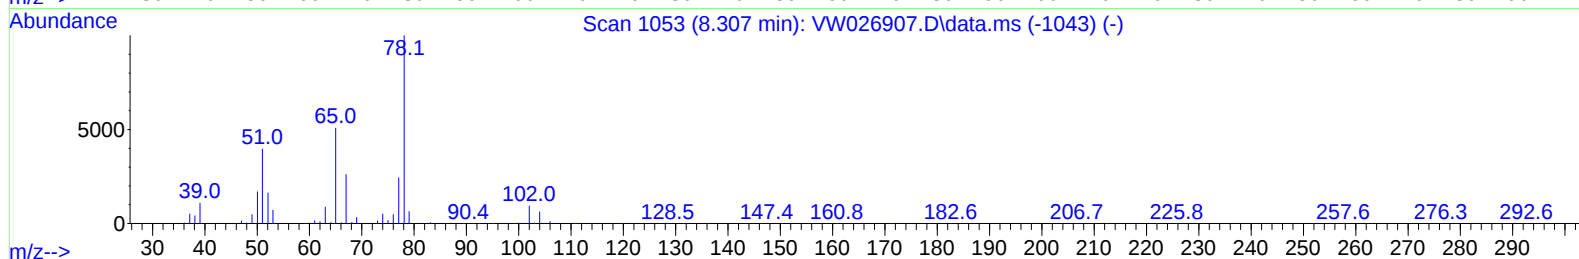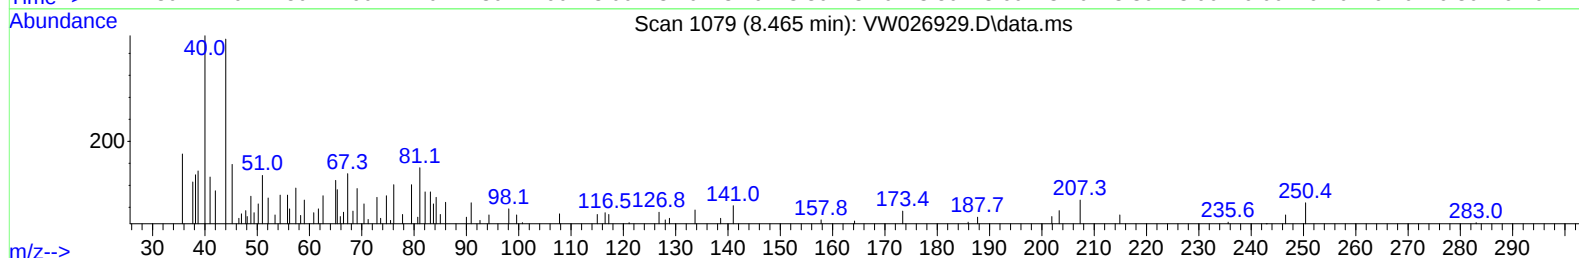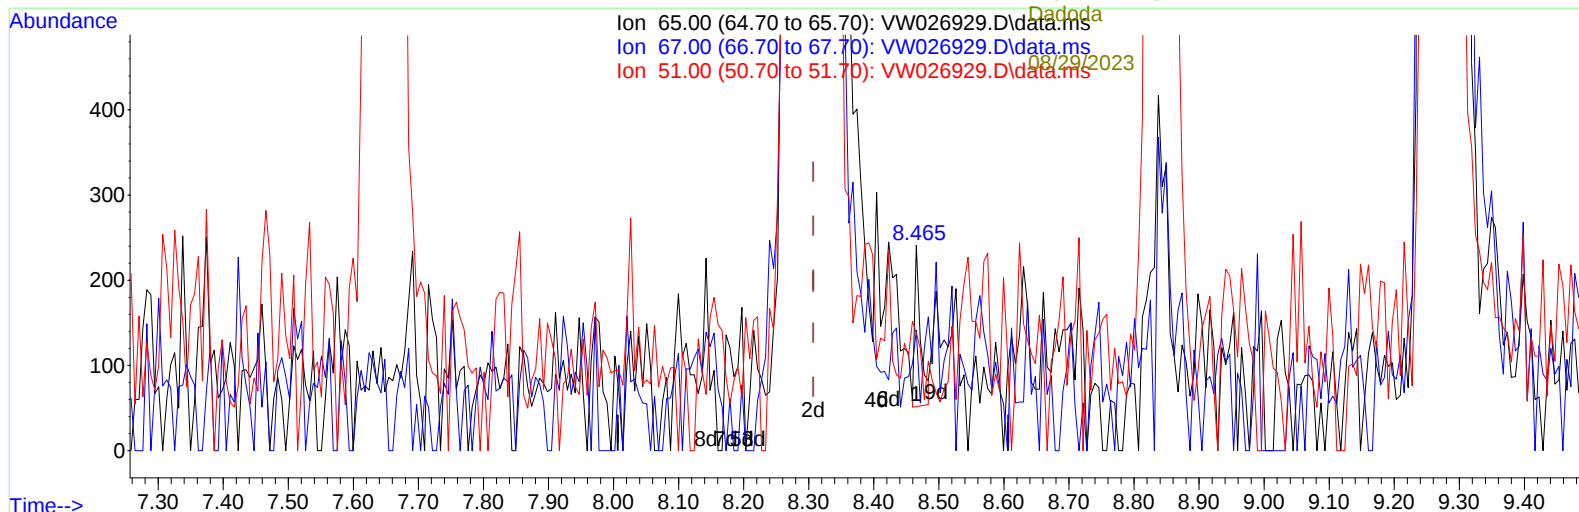

TIC: VW026929.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.465min (+ 0.159) 0.02 ug/L

response 121

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.60	65.29
51.00	112.90	104.96
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082823\
 Data File : VW026929.D
 Acq On : 28 Aug 2023 09:58
 Operator : SY/MD
 Sample : VW0828SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK561

Manual IntegrationsAPPROVED

Quant Time: Aug 28 14:13:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 26 05:14:45 2023
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

08/29/2023
 Supervised By :Mahesh
 Dadoda

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	343916	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	330192	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	170248	25.000	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.369	65	103682	18.339	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	73.360%
7) Chloroethane-d5	2.893	69	83163	19.782	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.120%
11) 1,1-Dichloroethene-d2	4.021	65	56265	20.235	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	80.920%
21) 2-Butanone-d5	7.075	46	71381	43.928	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.860%
24) Chloroform-d	7.648	84	258921	22.431	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.720%
26) 1,2-Dichloroethane-d4	8.307	65	163288m	25.634	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	102.520%
32) Benzene-d6	8.276	84	480953	21.135	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	84.520%
36) 1,2-Dichloropropane-d6	9.276	67	153919	21.714	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	86.840%
41) Toluene-d8	10.325	98	417125	21.353	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	85.400%
43) trans-1,3-Dichloroprop...	10.581	79	62815	21.463	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	85.840%
47) 2-Hexanone-d5	10.922	63	32368	43.457	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	86.920%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	120596	21.543	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	86.160%
66) 1,2-Dichlorobenzene-d4	13.849	152	137721	22.601	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	90.400%

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082823\
Data File : VW026929.D
Acq On : 28 Aug 2023 09:58
Operator : SY/MD
Sample : VW0828SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK561

Manual IntegrationsAPPROVED

Reviewed By :Semsettin
Yesilyurt

08/29/2023
Supervised By :Mahesh
Dadoda

08/29/2023

