




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082823\
 Data File : VW026934.D
 Acq On : 28 Aug 2023 12:18
 Operator : SY/MD
 Sample : 04175-05RE
 Misc : 6.89g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZYX0RE

Manual IntegrationsAPPROVED

Quant Time: Aug 28 22:26:32 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 26 05:14:45 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/29/2023
 Supervised By :Mahesh Dadoda 08/29/2023

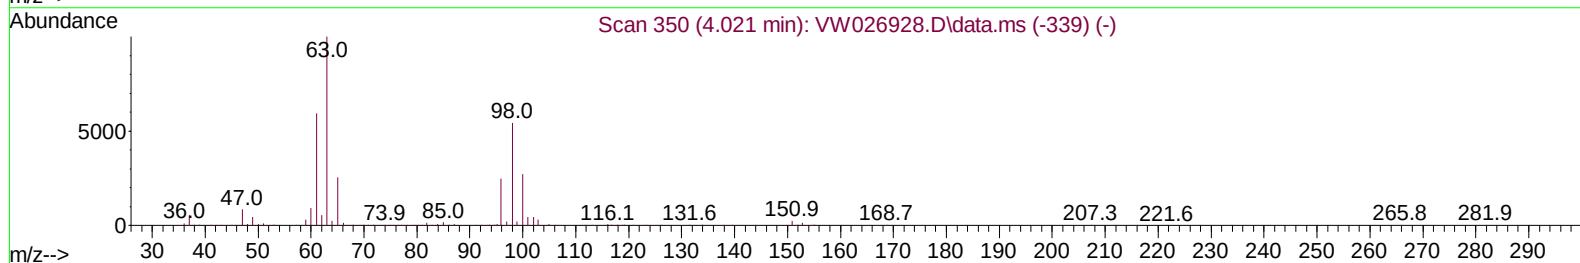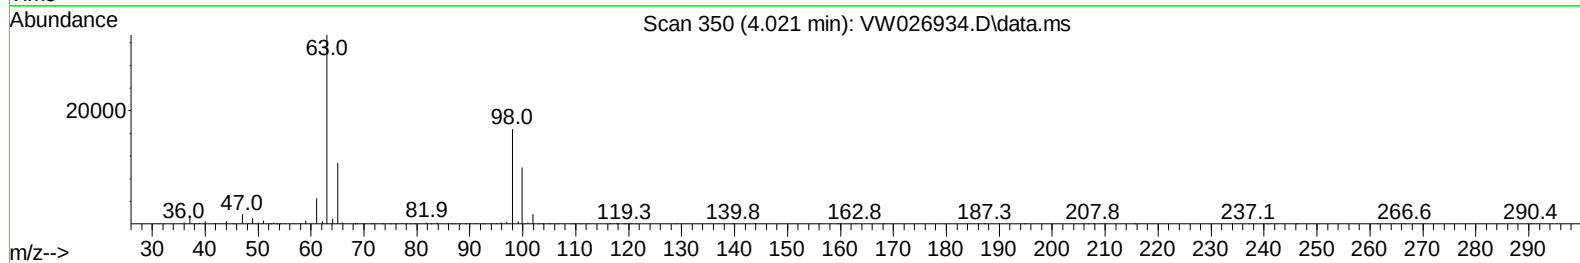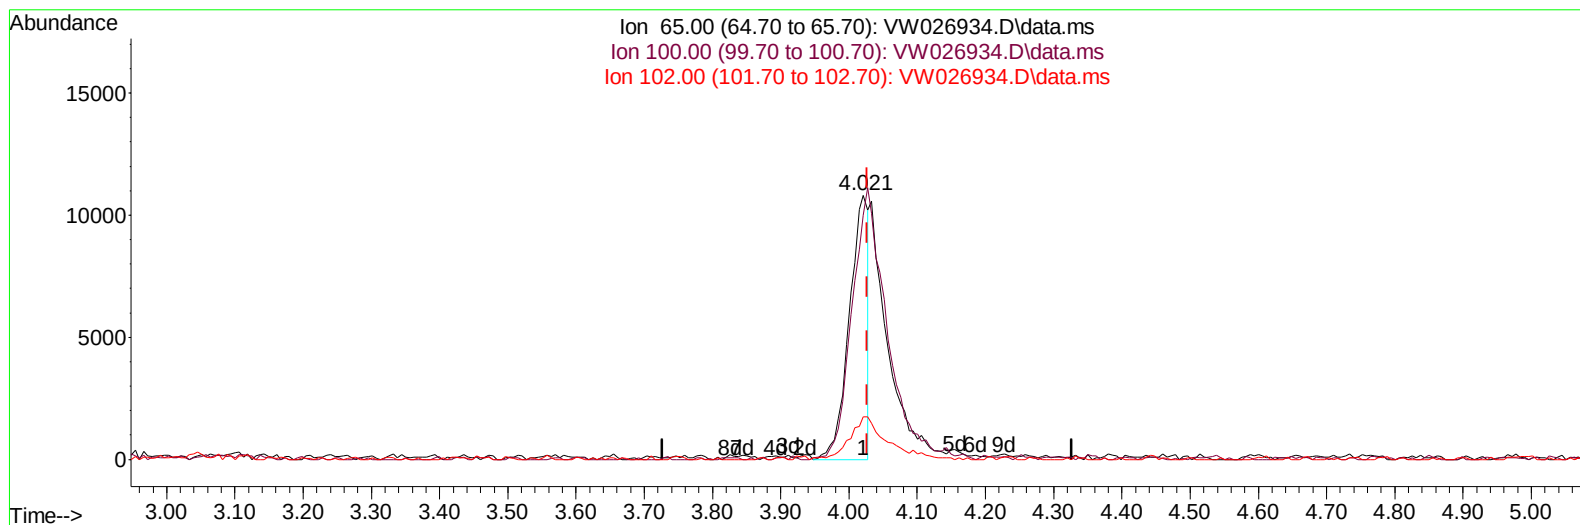

TIC: VW026934.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.021min (-0.006) 7.50 ug/L

response 20880

Ion	Exp%	Act%
65.00	100.00	100.00
100.00	124.90	187.60#
102.00	16.90	28.41#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082823\
 Data File : VW026934.D
 Acq On : 28 Aug 2023 12:18
 Operator : SY/MD
 Sample : 04175-05RE
 Misc : 6.89g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZYX0RE

Manual IntegrationsAPPROVED

Quant Time: Aug 28 22:26:32 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 26 05:14:45 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/29/2023
 Supervised By :Mahesh Dadoda 08/29/2023

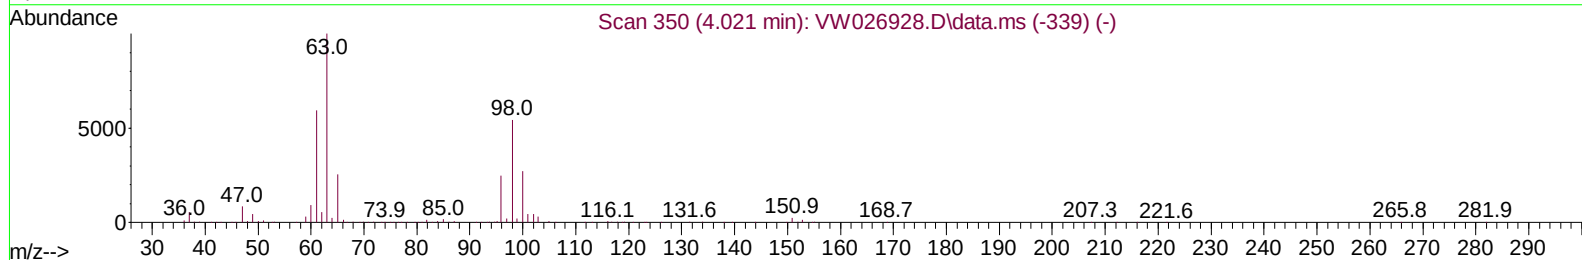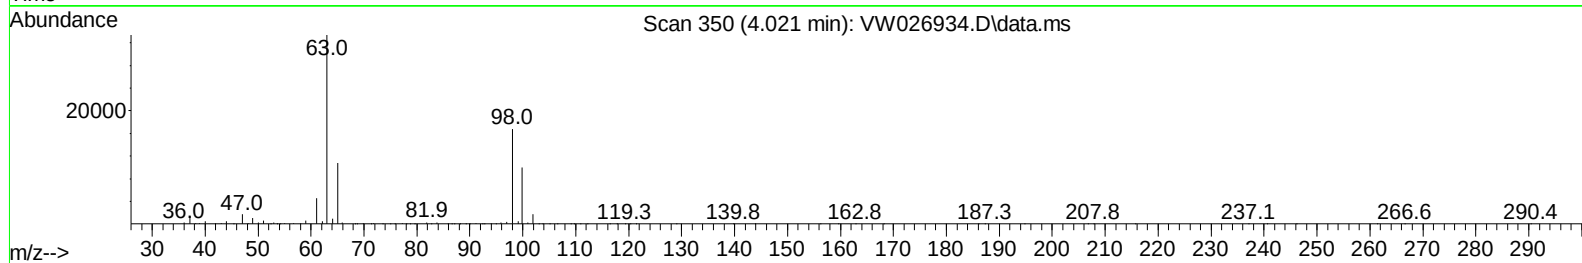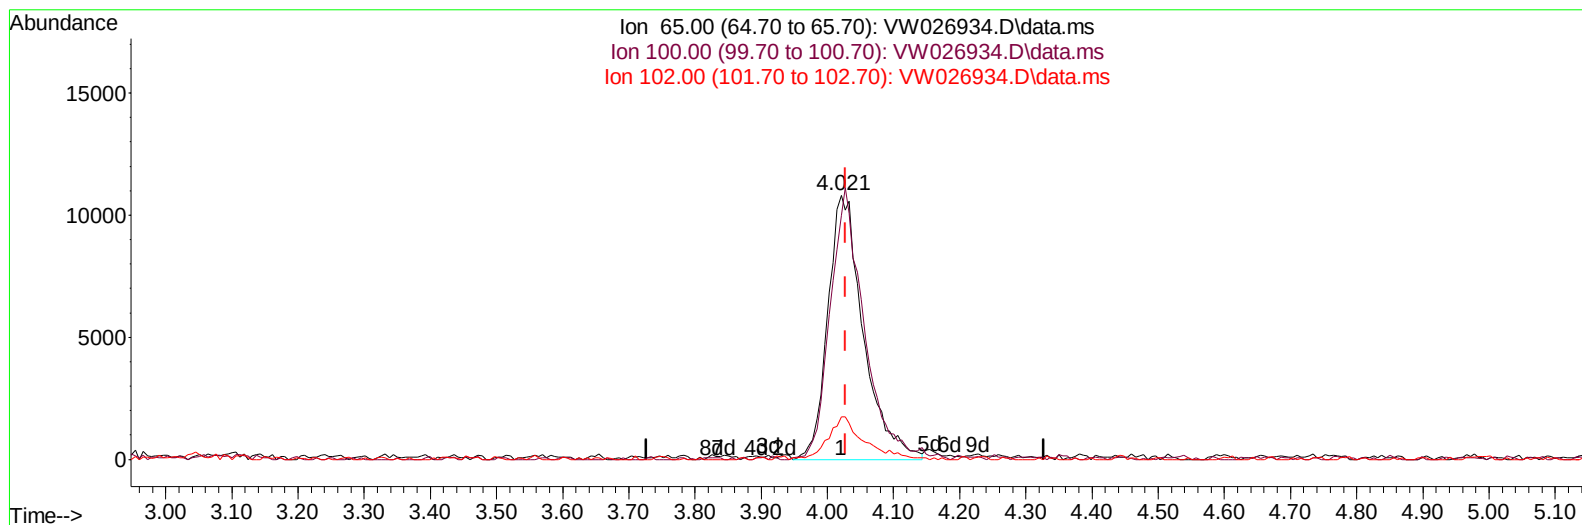

TIC: VW026934.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.021min (-0.006) 14.48 ug/L m

response 40288

Ion	Exp%	Act%
65.00	100.00	100.00
100.00	124.90	97.22
102.00	16.90	14.72
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082823\
 Data File : VW026934.D
 Acq On : 28 Aug 2023 12:18
 Operator : SY/MD
 Sample : 04175-05RE
 Misc : 6.89g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZYX0RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/29/2023
 Supervised By :Mahesh Dadoda 08/29/2023

Quant Time: Aug 28 22:26:32 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 26 05:14:45 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.837	114		344177	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		252866	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		58590	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		68652	12.134	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	48.520%		
7) Chloroethane-d5	2.899	69		64652	15.367	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	61.480%		
11) 1,1-Dichloroethene-d2	4.021	65		40288m	14.478	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	57.920%		
21) 2-Butanone-d5	7.075	46		84262	51.816	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	103.640%		
24) Chloroform-d	7.648	84		232886	20.161	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	80.640%		
26) 1,2-Dichloroethane-d4	8.307	65		157230	24.664	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	98.640%		
32) Benzene-d6	8.276	84		384292	22.051	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	88.200%		
36) 1,2-Dichloropropane-d6	9.276	67		133554	24.603	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	98.400%		
41) Toluene-d8	10.325	98		280759	18.768	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	75.080%		
43) trans-1,3-Dichloroprop...	10.581	79		50802	22.666	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	90.680%		
47) 2-Hexanone-d5	10.922	63		35996	63.106	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	126.220%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		82540	19.254	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	77.000%		
66) 1,2-Dichlorobenzene-d4	13.848	152		38788	18.496	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	74.000%#		
Target Compounds							
16) Methylene chloride	4.923	84		34662	5.206	ug/L	Qvalue 92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082823\
Data File : VW026934.D
Acq On : 28 Aug 2023 12:18
Operator : SY/MD
Sample : 04175-05RE
Misc : 6.89g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EZYX0RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/29/2023
Supervised By :Mahesh Dadoda 08/29/2023

Quant Time: Aug 28 22:26:32 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Aug 26 05:14:45 2023
Response via : Initial Calibration

