

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082824\
 Data File : VW030068.D
 Acq On : 28 Aug 2024 11:35
 Operator : SY/MD
 Sample : VW0828SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Aug 29 01:13:34 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Aug 29 01:10:06 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	193178	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	188534	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	79896	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	66738	23.215	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 92.880%			
7) Chloroethane-d5	2.899	69	48774	23.905	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 95.640%			
11) 1,1-Dichloroethene-d2	4.021	65	28999	23.611	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 94.440%			
21) 2-Butanone-d5	7.081	46	31209	54.461	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 108.920%			
24) Chloroform-d	7.648	84	131122	25.170	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 100.680%			
26) 1,2-Dichloroethane-d4	8.307	65	72174	27.285	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 109.120%			
32) Benzene-d6	8.276	84	257454	23.134	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 92.520%			
36) 1,2-Dichloropropane-d6	9.270	67	82520	25.309	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 101.240%			
41) Toluene-d8	10.318	98	232579	22.961	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 91.840%			
43) trans-1,3-Dichloroprop...	10.575	79	30290	22.584	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 90.320%			
47) 2-Hexanone-d5	10.922	63	25207	50.514	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 101.020%			
56) 1,1,2,2-Tetrachloroeth...	12.690	84	60732	25.299	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 101.200%			
66) 1,2-Dichlorobenzene-d4	13.848	152	72804	25.193	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 100.760%			
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	2347	0.499	ug/L	# 75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082824\
Data File : VW030068.D
Acq On : 28 Aug 2024 11:35
Operator : SY/MD
Sample : VW0828SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Aug 29 01:13:34 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Aug 29 01:10:06 2024
Response via : Initial Calibration

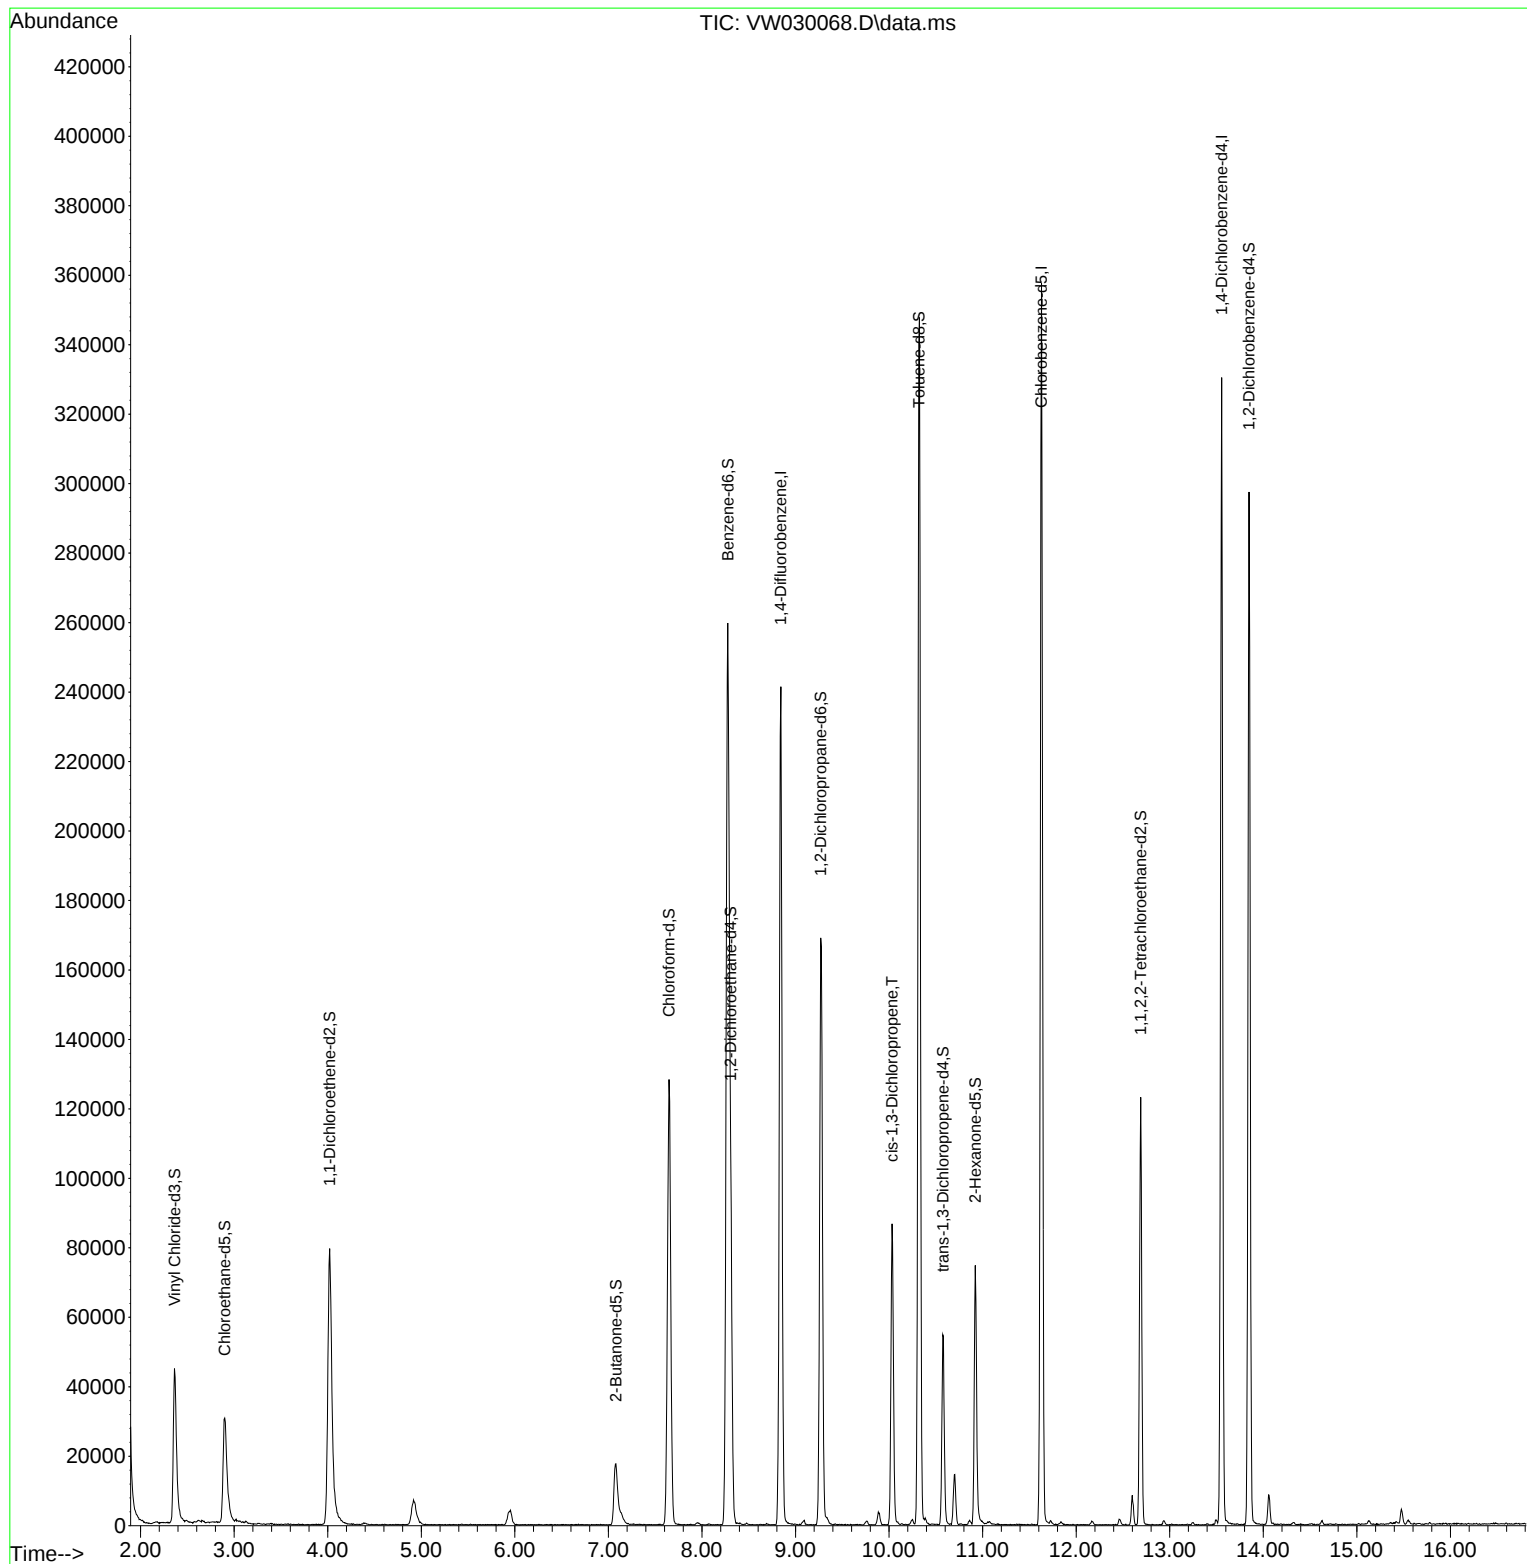

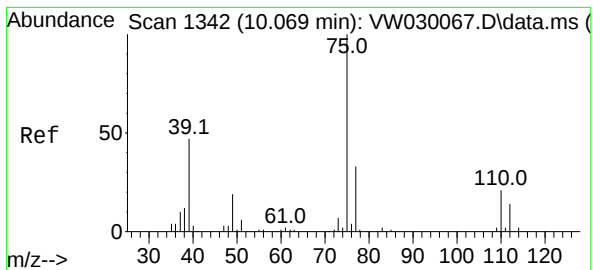

#39
 cis-1,3-Dichloropropene
 Concen: 0.499 ug/L
 RT: 10.032 min Scan# 14
 Delta R.T. -0.037 min
 Lab File: VW030068.D
 Acq: 28 Aug 2024 11:35

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 2347
 Ion Ratio Lower Upper
 75 100
 77 46.4 22.8 42.4#

