

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082824\
 Data File : VW030070.D
 Acq On : 28 Aug 2024 12:45
 Operator : SY/MD
 Sample : P3721-07
 Misc : 6.16g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCXZ0

Quant Time: Aug 29 01:14:10 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Aug 29 01:10:06 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	238651	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	209321	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	76703	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	69543	19.582	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	78.320%
7) Chloroethane-d5	2.905	69	50088	19.872	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.480%
11) 1,1-Dichloroethene-d2	4.027	65	30149	19.870	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	79.480%
21) 2-Butanone-d5	7.075	46	38236	54.010	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	108.020%
24) Chloroform-d	7.648	84	127257	19.773	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	79.080%
26) 1,2-Dichloroethane-d4	8.307	65	71822	21.978	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	87.920%
32) Benzene-d6	8.276	84	253433	20.512	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	82.040%
36) 1,2-Dichloropropane-d6	9.276	67	80880	22.343	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	89.360%
41) Toluene-d8	10.325	98	216391	19.242	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	76.960%
43) trans-1,3-Dichloroprop...	10.575	79	31594	21.217	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	84.880%
47) 2-Hexanone-d5	10.922	63	32079	57.901	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	115.800%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	63512	23.830	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	95.320%
66) 1,2-Dichlorobenzene-d4	13.848	152	52232	18.827	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	75.320%
Target Compounds						
13) Acetone	4.118	43	92604	143.011	ug/L	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082824\
Data File : VW030070.D
Acq On : 28 Aug 2024 12:45
Operator : SY/MD
Sample : P3721-07
Misc : 6.16g/10mL/MSVOA_W/SOIL/B
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCXZ0

Quant Time: Aug 29 01:14:10 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Aug 29 01:10:06 2024
Response via : Initial Calibration

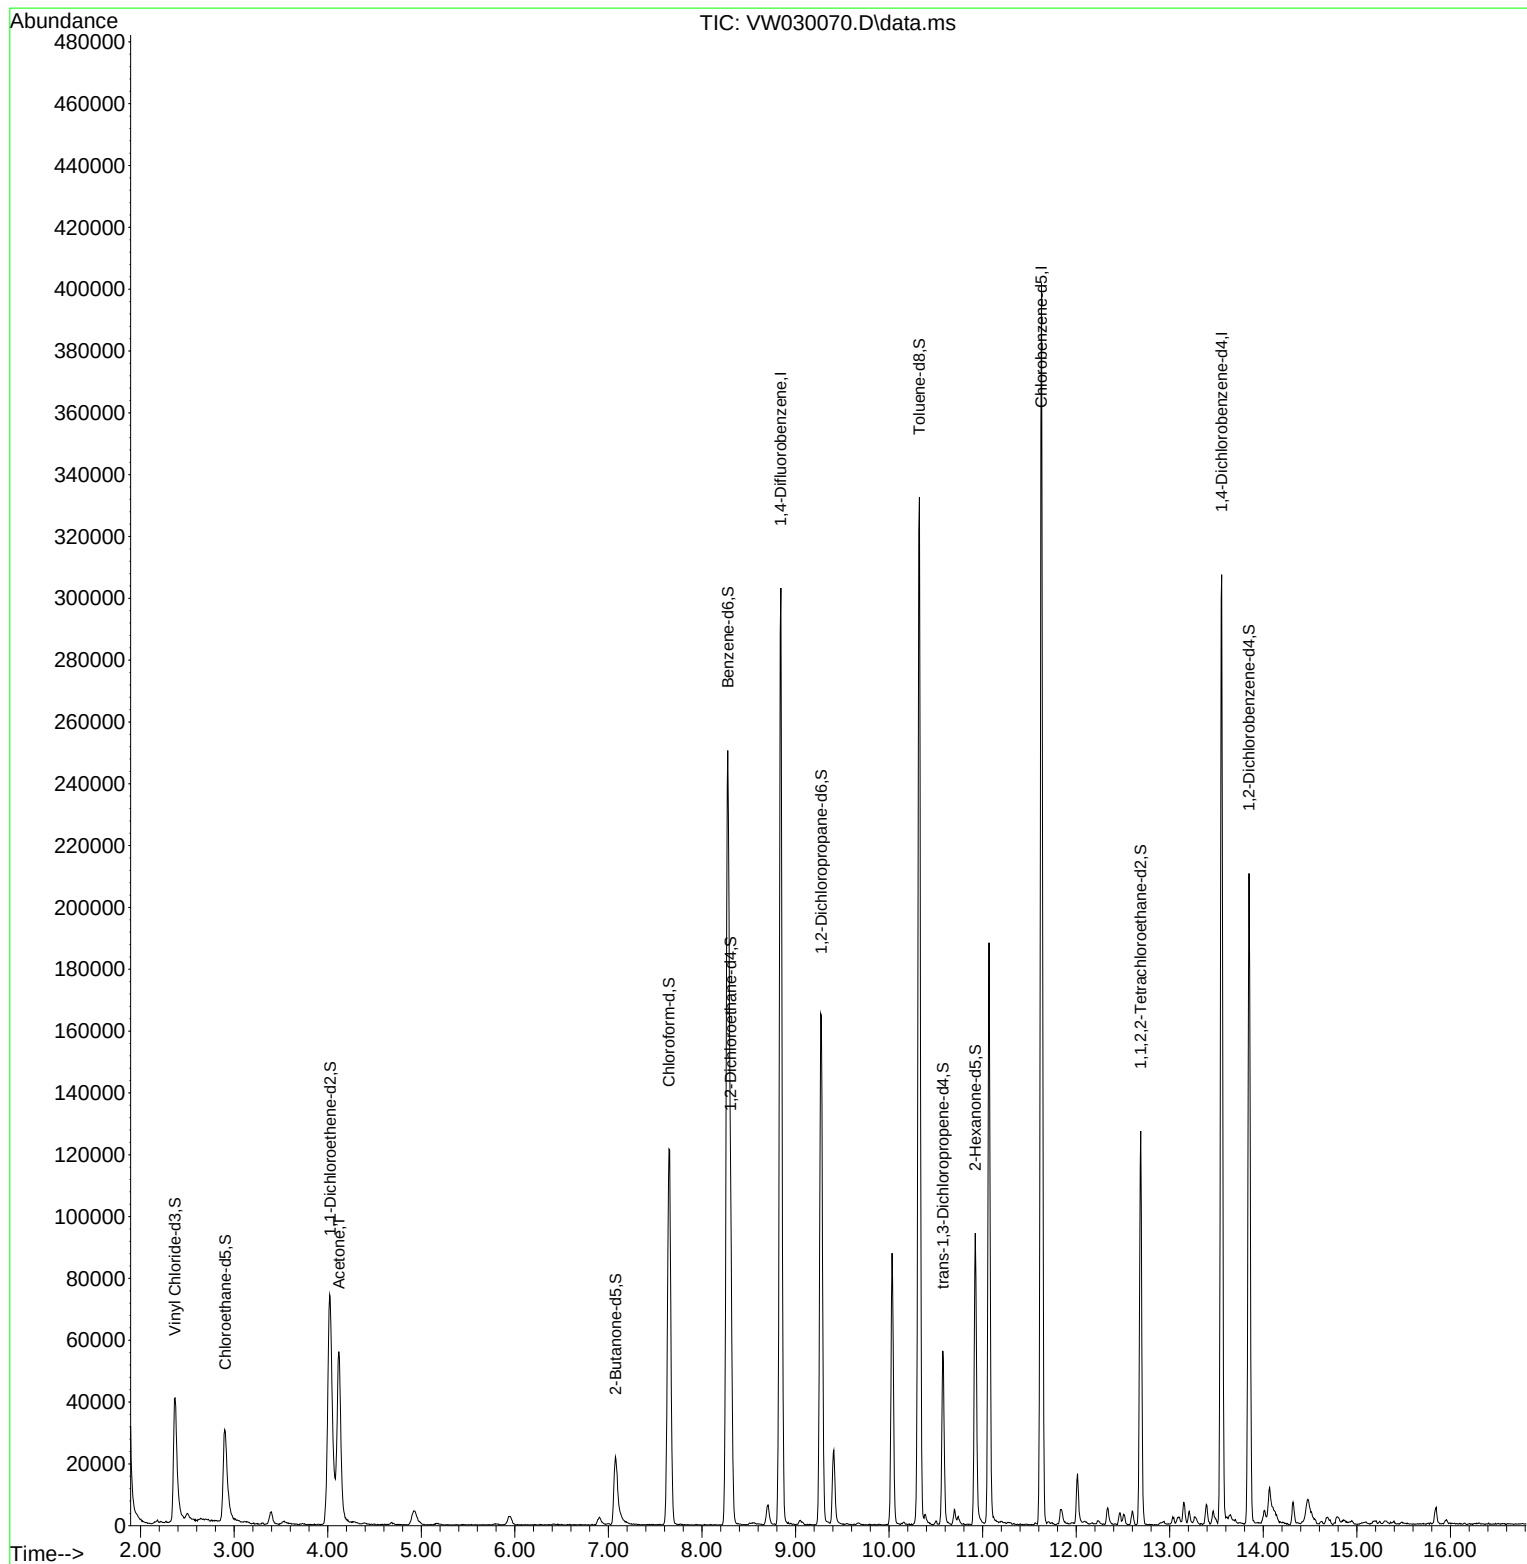

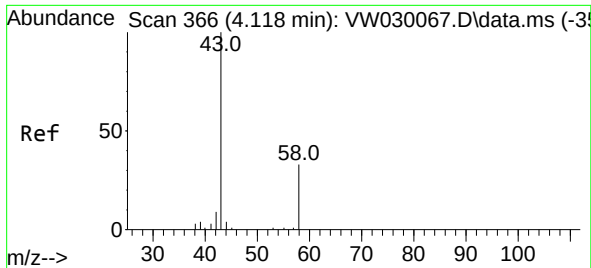

#13
 Acetone
 Concen: 143.011 ug/L
 RT: 4.118 min Scan# 30
 Delta R.T. -0.000 min
 Lab File: VW030070.D
 Acq: 28 Aug 2024 12:45

Instrument :
 MSVOA_W
 ClientSampleId :
 DCXZ0

Tgt Ion: 43 Resp: 92604
 Ion Ratio Lower Upper
 43 100
 58 31.6 0.0 66.4

