

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082824\
 Data File : VW030075.D
 Acq On : 28 Aug 2024 14:45
 Operator : SY/MD
 Sample : P3733-19
 Misc : 5.00g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A44B4

Quant Time: Aug 29 01:15:22 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Aug 29 01:10:06 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	198927	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	184963	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	82037	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.362	65	71350	24.102	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	96.400%
7) Chloroethane-d5	2.899	69	52403	24.942	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	99.760%
11) 1,1-Dichloroethene-d2	4.021	65	32441	25.650	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	102.600%
21) 2-Butanone-d5	7.075	46	37020	62.734	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	125.460%
24) Chloroform-d	7.648	84	139795	26.059	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	104.240%
26) 1,2-Dichloroethane-d4	8.307	65	78527	28.828	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	115.320%
32) Benzene-d6	8.270	84	277886	25.453	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	101.800%
36) 1,2-Dichloropropane-d6	9.270	67	89584	28.006	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	112.040%
41) Toluene-d8	10.324	98	254380	25.599	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	102.400%
43) trans-1,3-Dichloroprop...	10.574	79	34703	26.374	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	105.480%
47) 2-Hexanone-d5	10.922	63	30445	62.189	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	124.380%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	70799	30.062	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	120.240%#
66) 1,2-Dichlorobenzene-d4	13.848	152	78485	26.450	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	105.800%
Target Compounds					Qvalue	
13) Acetone	4.118	43	6532	12.102	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082824\
Data File : VW030075.D
Acq On : 28 Aug 2024 14:45
Operator : SY/MD
Sample : P3733-19
Misc : 5.00g/10mL/MSVOA_W/SOIL/A
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A44B4

Quant Time: Aug 29 01:15:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Aug 29 01:10:06 2024
Response via : Initial Calibration

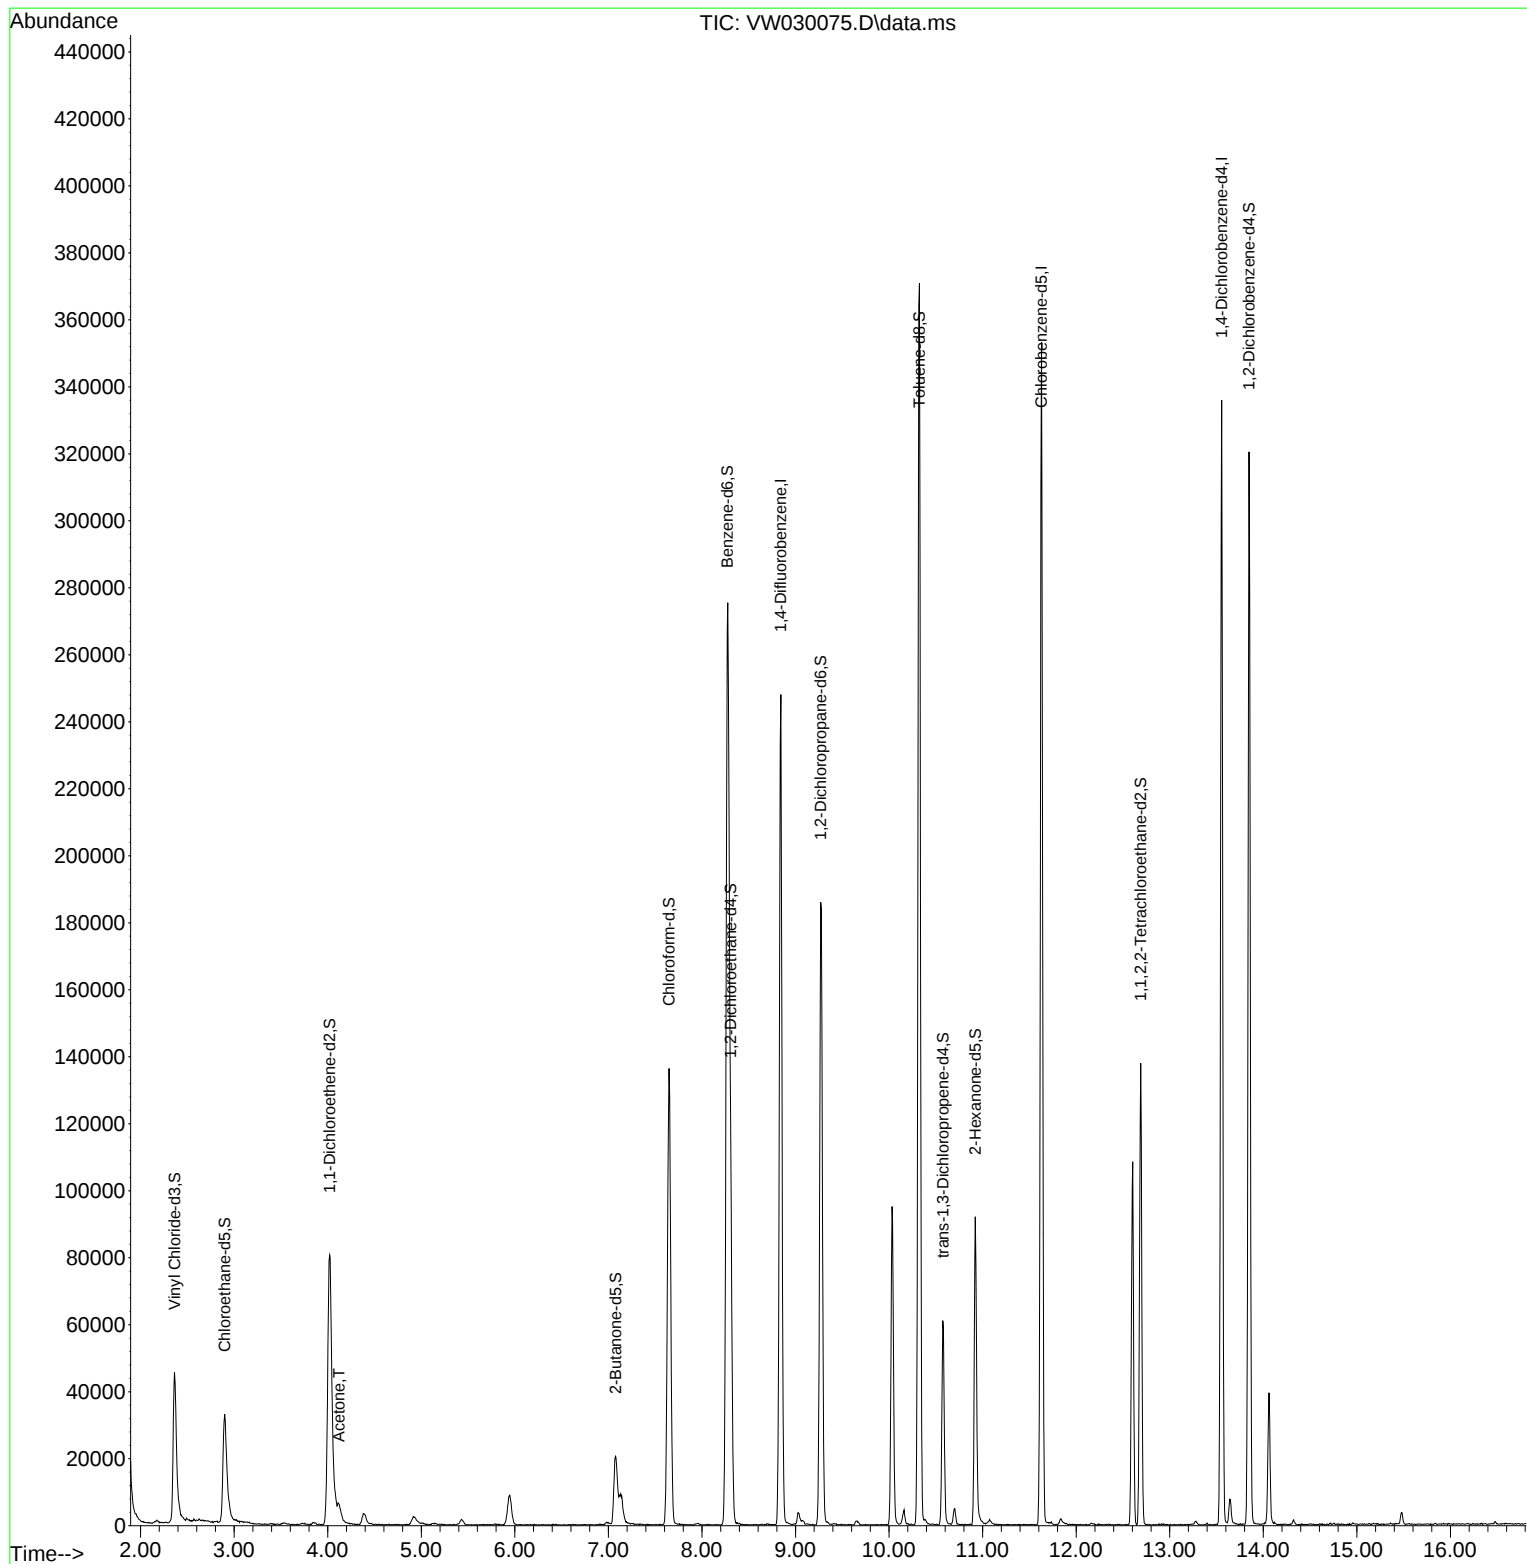

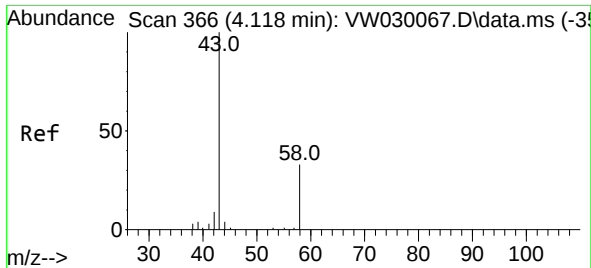

#13

Acetone

Concen: 12.102 ug/L

RT: 4.118 min Scan# 3

Delta R.T. -0.000 min

Lab File: VW030075.D


Acq: 28 Aug 2024 14:45

Instrument :

MSVOA_W

ClientSampleId :

A44B4

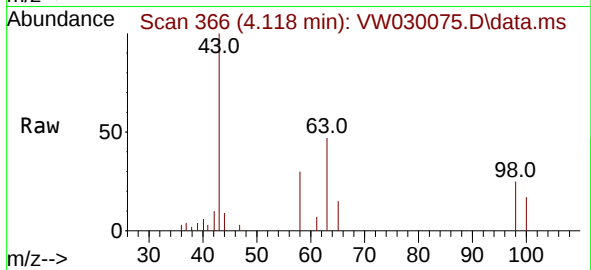

Tgt Ion: 43 Resp: 6532

Ion Ratio Lower Upper

43 100

58 31.1 0.0 66.4

