

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082824\
 Data File : VW030081.D
 Acq On : 28 Aug 2024 17:09
 Operator : SY/MD
 Sample : P3675-22
 Misc : 9.68g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCYA6

Quant Time: Aug 29 01:17:11 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Aug 29 01:10:06 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	238067	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	225900	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	99286	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	69449	19.603	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	78.400%
7) Chloroethane-d5	2.899	69	49168	19.555	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	78.200%
11) 1,1-Dichloroethene-d2	4.021	65	30181	19.940	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	79.760%
21) 2-Butanone-d5	7.069	46	39956	56.578	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	113.160%
24) Chloroform-d	7.648	84	132504	20.639	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	82.560%
26) 1,2-Dichloroethane-d4	8.301	65	76106	23.346	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	93.400%
32) Benzene-d6	8.270	84	263344	19.750	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	79.000%
36) 1,2-Dichloropropane-d6	9.270	67	85491	21.883	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	87.520%
41) Toluene-d8	10.325	98	237042	19.531	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	78.120%
43) trans-1,3-Dichloroprop...	10.575	79	32189	20.030	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	80.120%
47) 2-Hexanone-d5	10.922	63	32844	54.931	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	109.860%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	71172	24.744	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	98.960%
66) 1,2-Dichlorobenzene-d4	13.849	152	70038	19.503	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	78.000%
Target Compounds					Qvalue	
13) Acetone	4.125	43	21176	32.783	ug/L	96
14) Carbon disulfide	4.393	76	5433	0.574	ug/L	# 84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082824\
Data File : VW030081.D
Acq On : 28 Aug 2024 17:09
Operator : SY/MD
Sample : P3675-22
Misc : 9.68g/10mL/MSVOA_W/SOIL/B
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCYA6

Quant Time: Aug 29 01:17:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Aug 29 01:10:06 2024
Response via : Initial Calibration

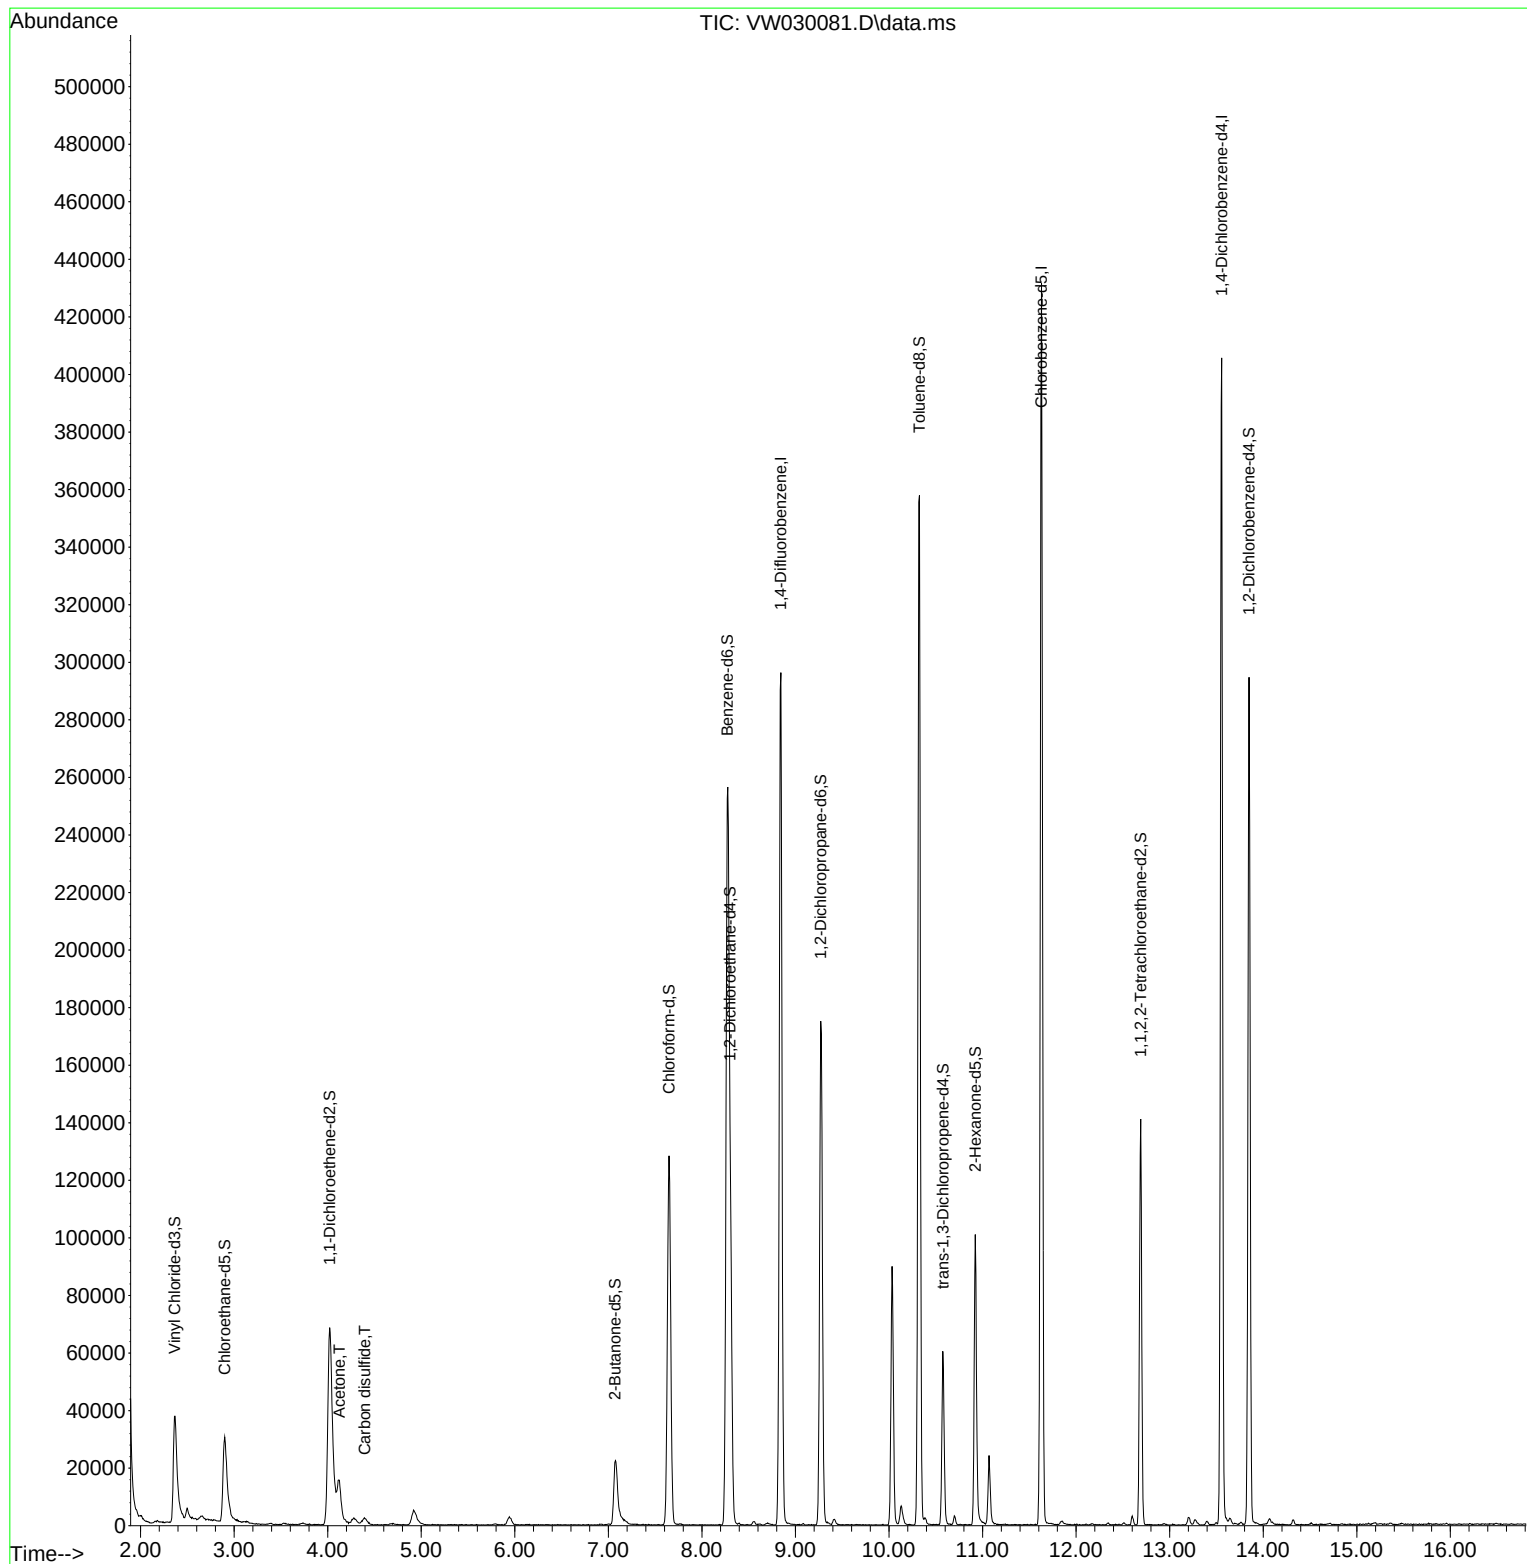

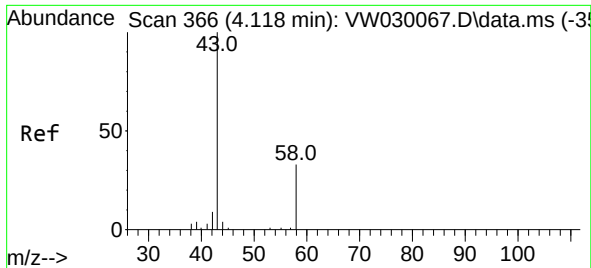

#13

Acetone

Concen: 32.783 ug/L

RT: 4.125 min Scan# 367

Delta R.T. 0.006 min

Lab File: VW030081.D

Acq: 28 Aug 2024 17:09

Instrument :

MSVOA_W

ClientSampleId :





DCYA6

Tgt Ion: 43 Resp: 21176

Ion Ratio Lower Upper

43 100

58 30.7 0.0 66.4

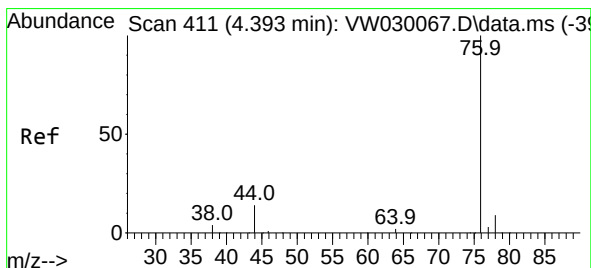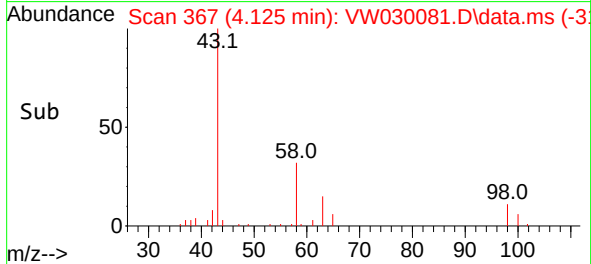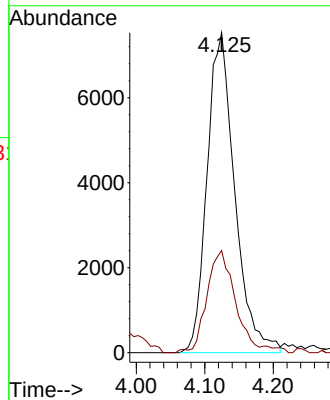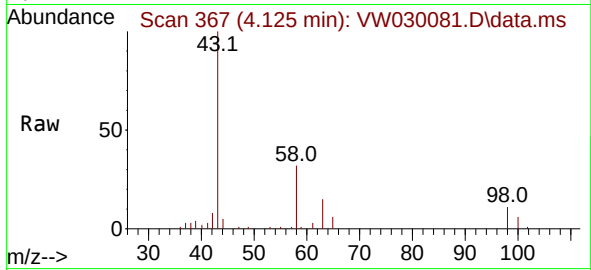

#14

Carbon disulfide

Concen: 0.574 ug/L

RT: 4.393 min Scan# 411

Delta R.T. 0.000 min

Lab File: VW030081.D

Acq: 28 Aug 2024 17:09

Tgt Ion: 76 Resp: 5433

Ion Ratio Lower Upper

76 100

78 14.0 6.6 9.8#

